

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)


Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 06:07:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

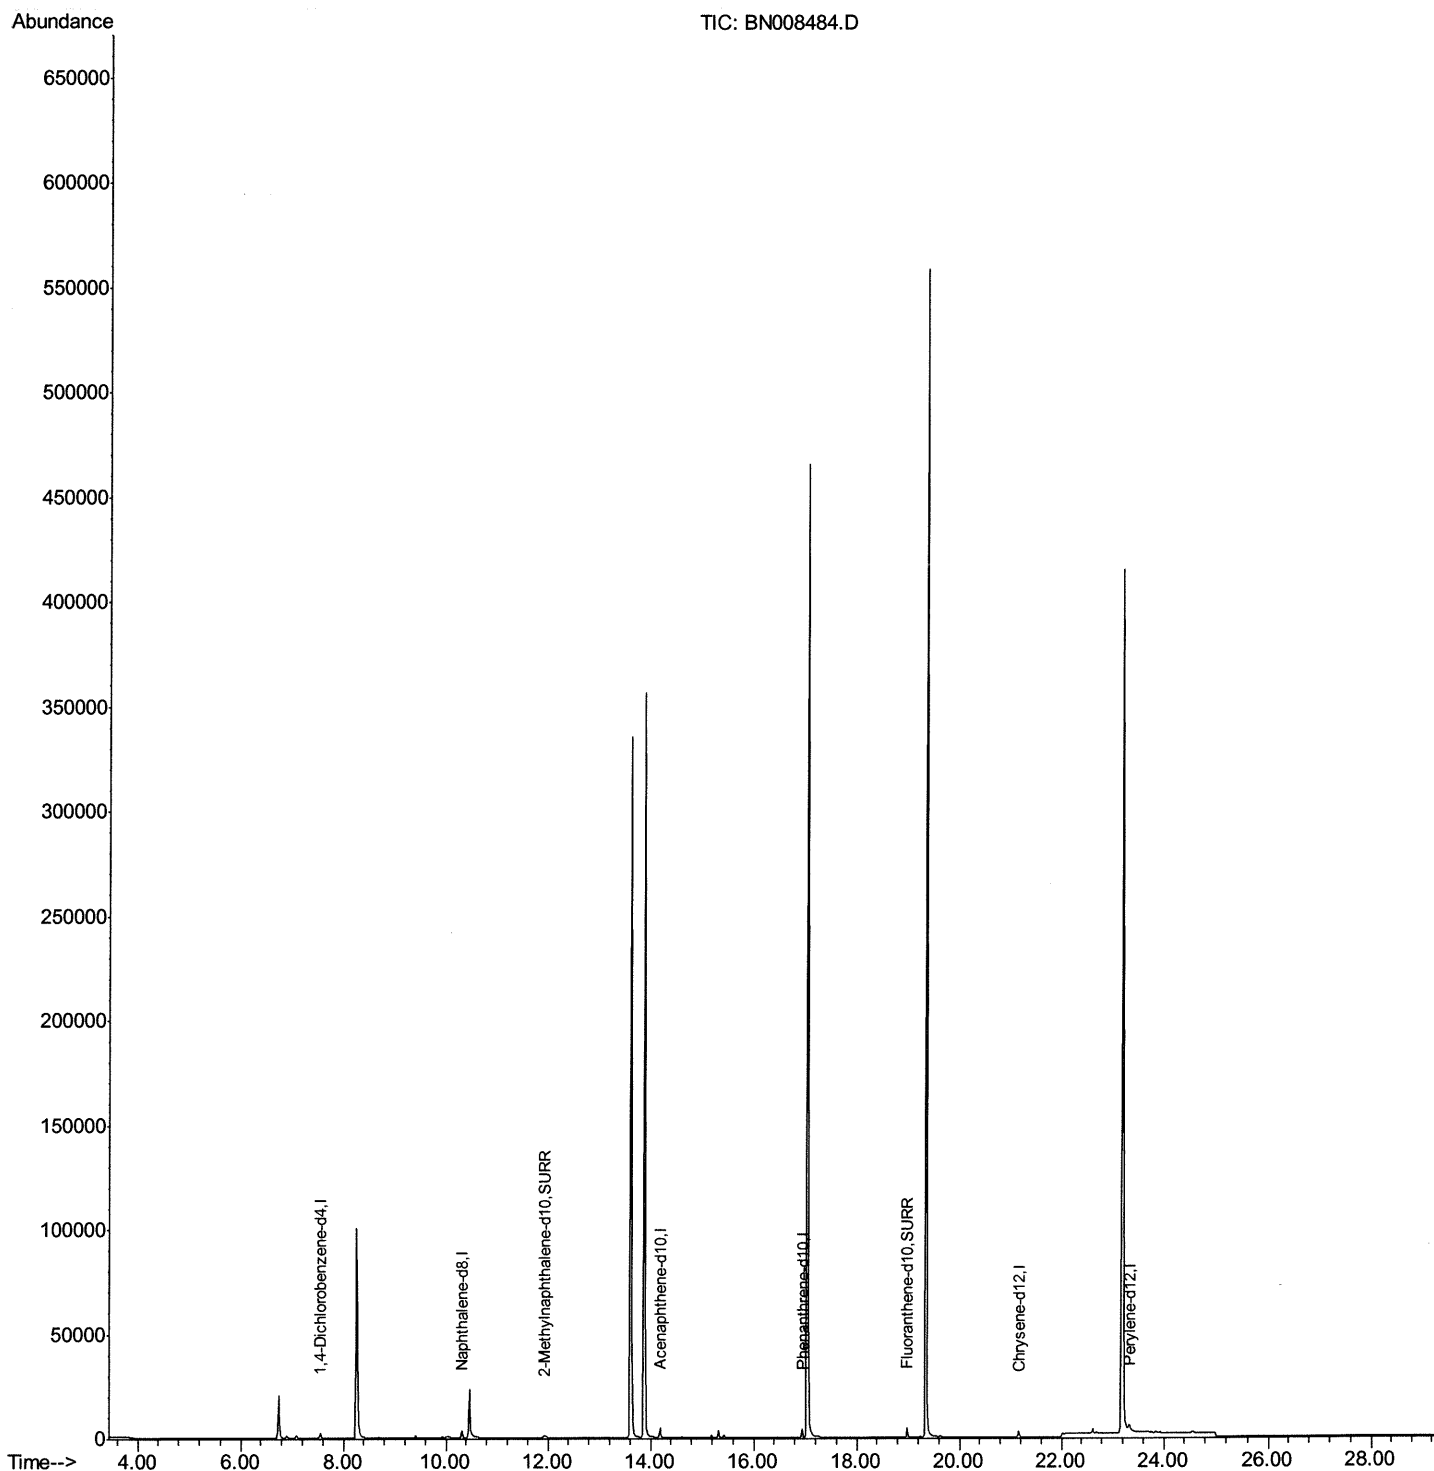

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 05:45:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

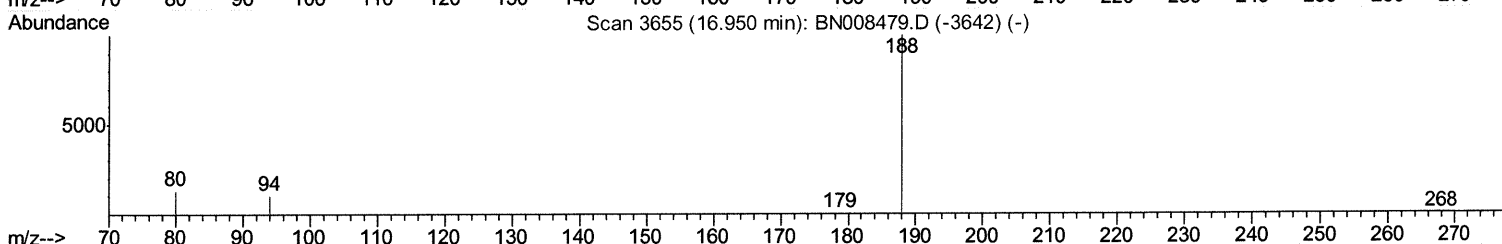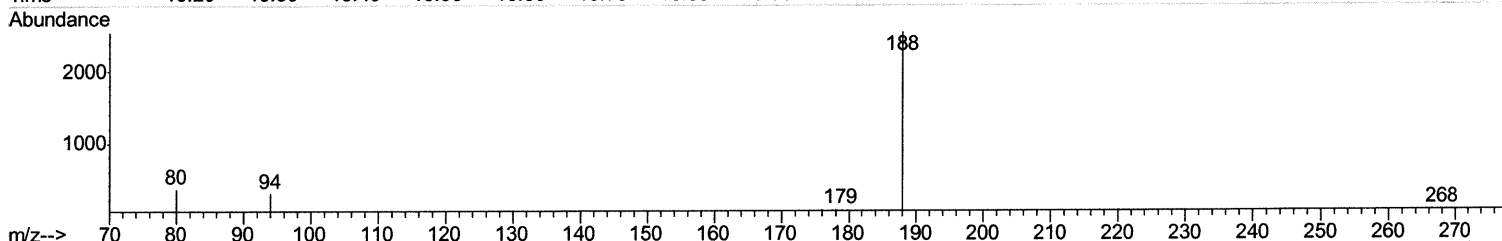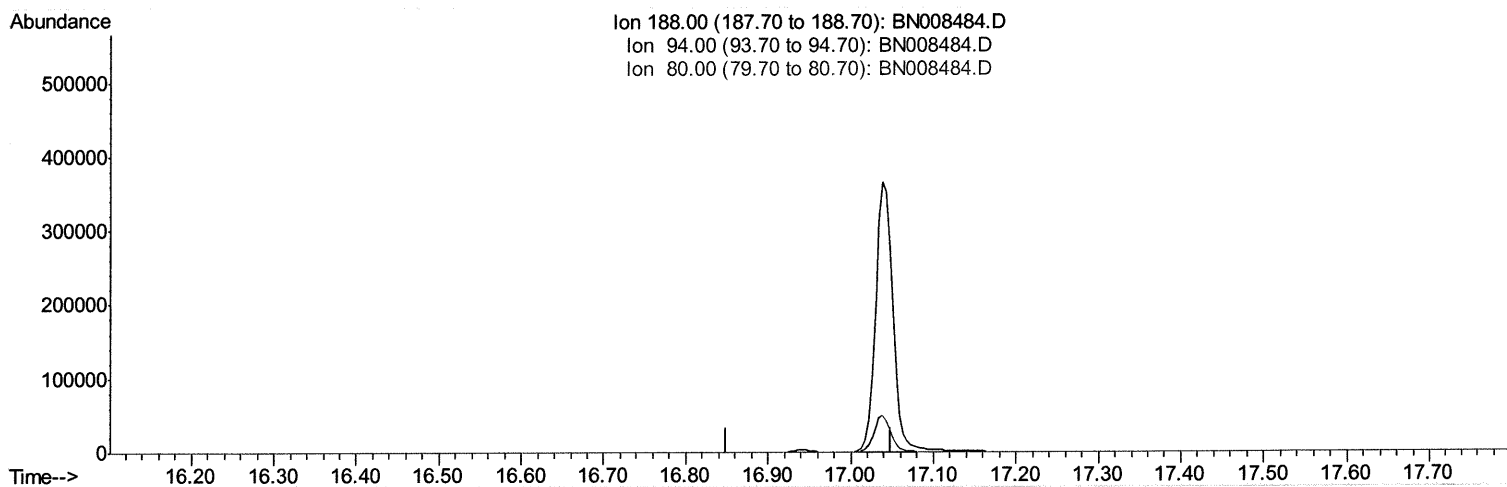

TIC: BN008484.D

(10) Phenanthrene-d10 (I)

16.950min (-16.950) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 05:45:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

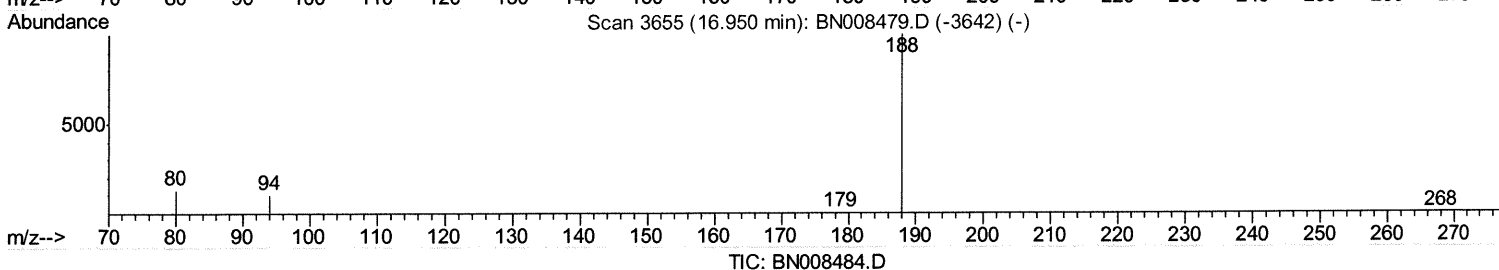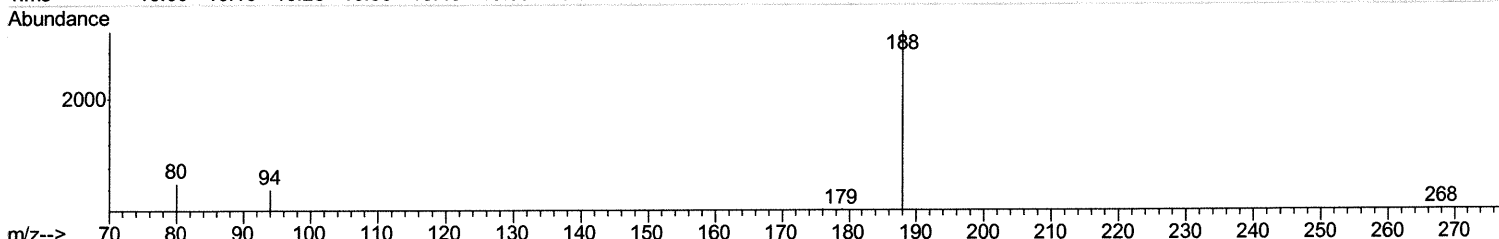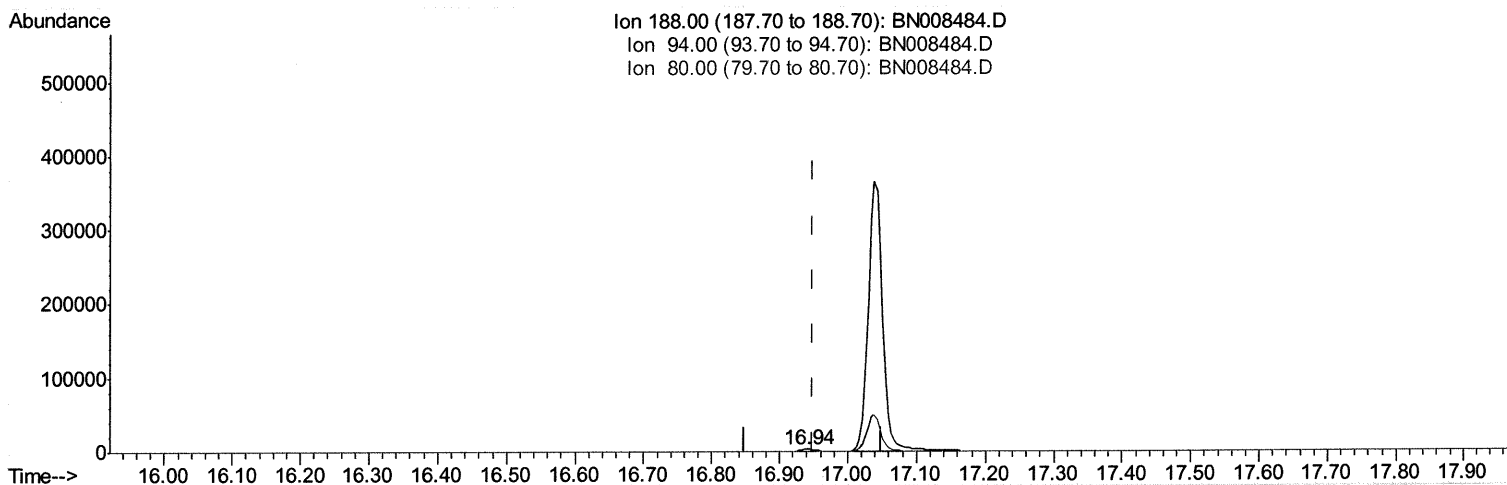

(10) Phenanthrene-d10 (I)

16.941min (-0.009) 0.40ng/ul m

response 4839

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	13.00
80.00	15.50	16.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 06:05:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

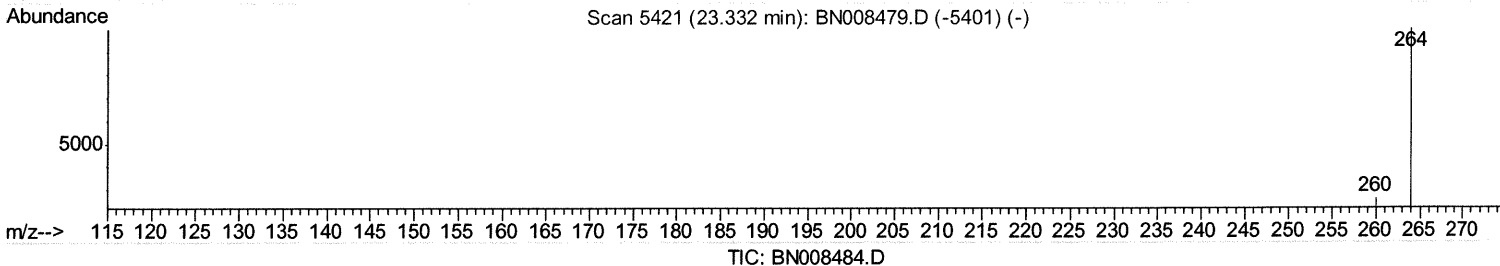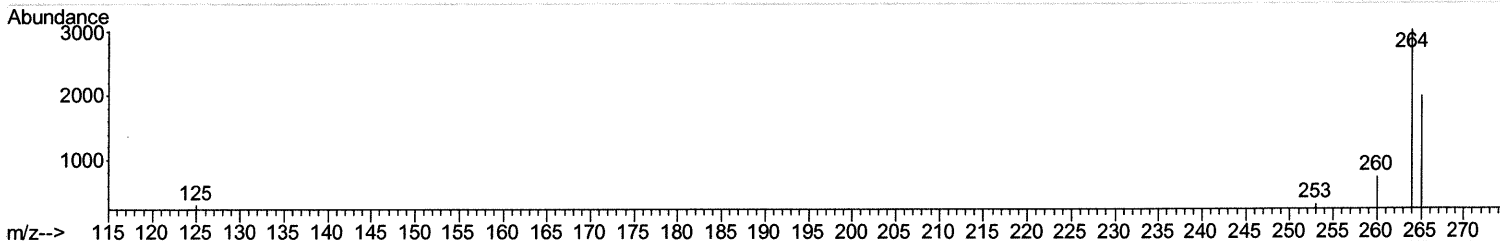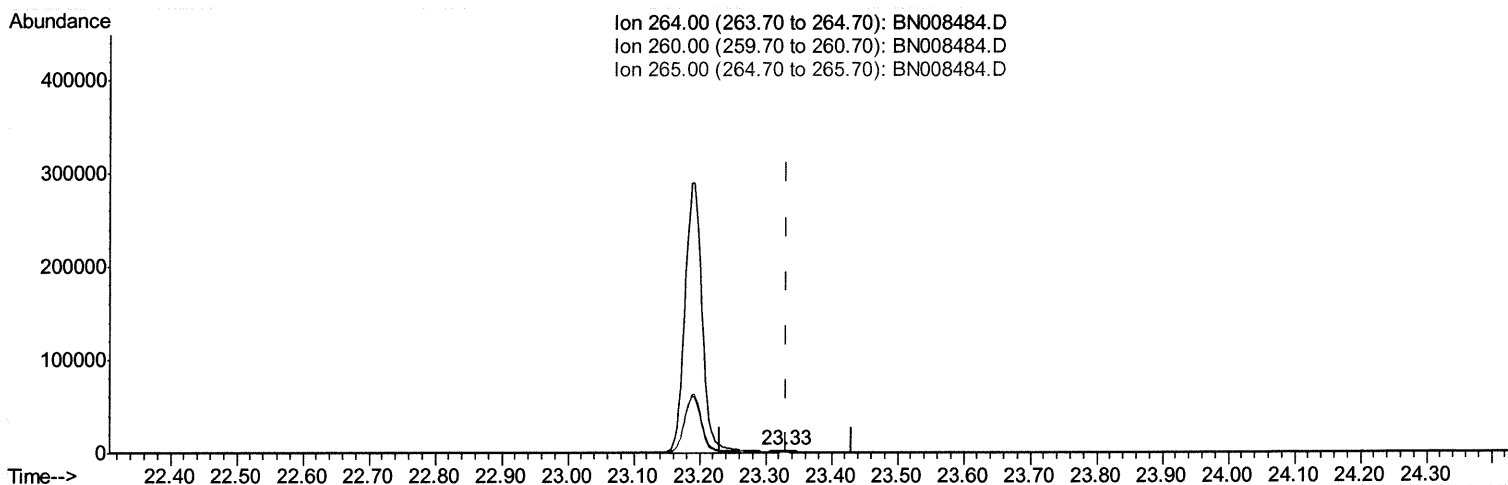

(20) Perylene-d12 (I)

23.328min (-0.004) 0.40ng/ul

response 6030

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	24.29
265.00	98.40	66.21#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 06:06:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

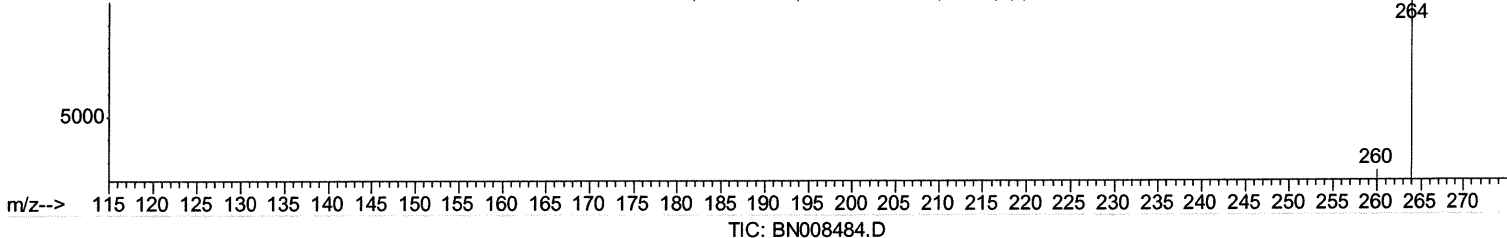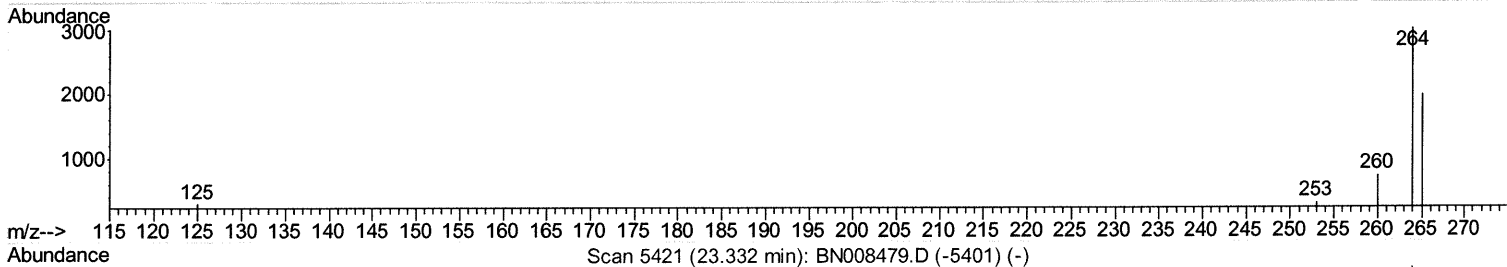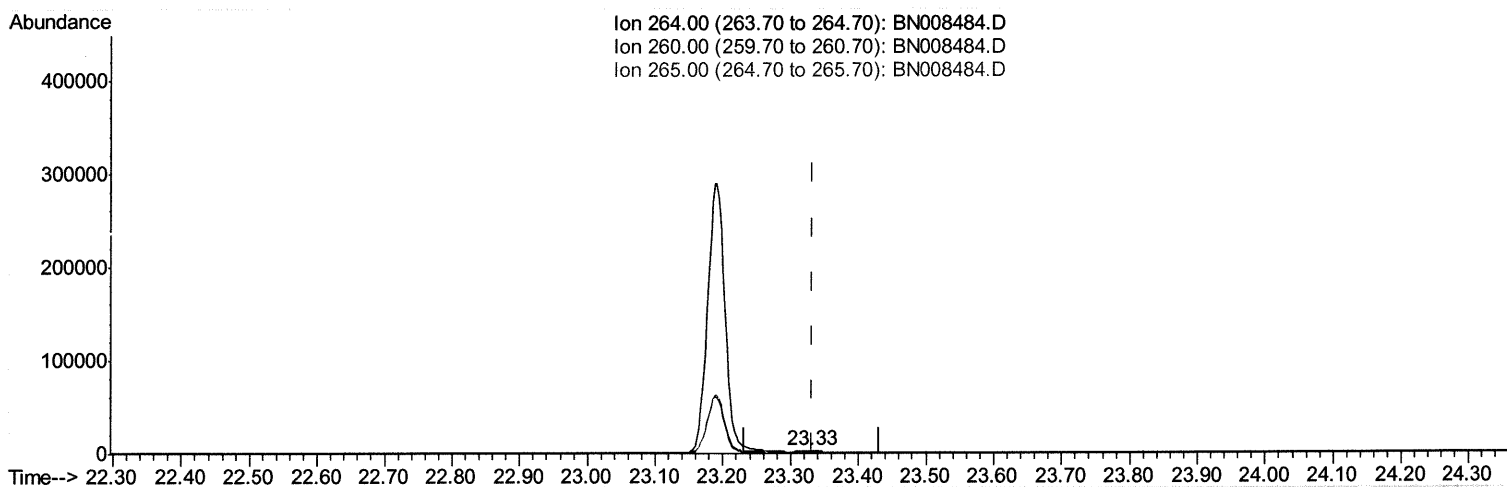

(20) Perylene-d12 (I)

23.328min (-0.004) 0.40ng/ul m

response 2559

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	24.29
265.00	98.40	66.21#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)

Data File : BN008484.D
Acq On : 07 Nov 2019 14:38
Operator : JU
Sample : PB124433BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
11/11/2019 8:07:58 AM

Quant Time: Nov 08 06:07:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 05:42:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	Q	Ion	Response	Conc	Units	Dev (Min)
--------------------	------	---	-----	----------	------	-------	-----------

1) 1,4-Dichlorobenzene-d4	7.55	152		1291	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.31	136		5148	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.19	164		2633	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188		4839m>	0.40	ng/ul>	0.00>
16) Chrysene-d12	21.17	240		3737	0.40	ng/ul	0.00
20) Perylene-d12	23.33	264		2559m>	0.40	ng/ul>	0.00>

Je 11/11/19
Je 11/11/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.93	152		2745	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.99	212		5762	0.40	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed