

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)


Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 07:32:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

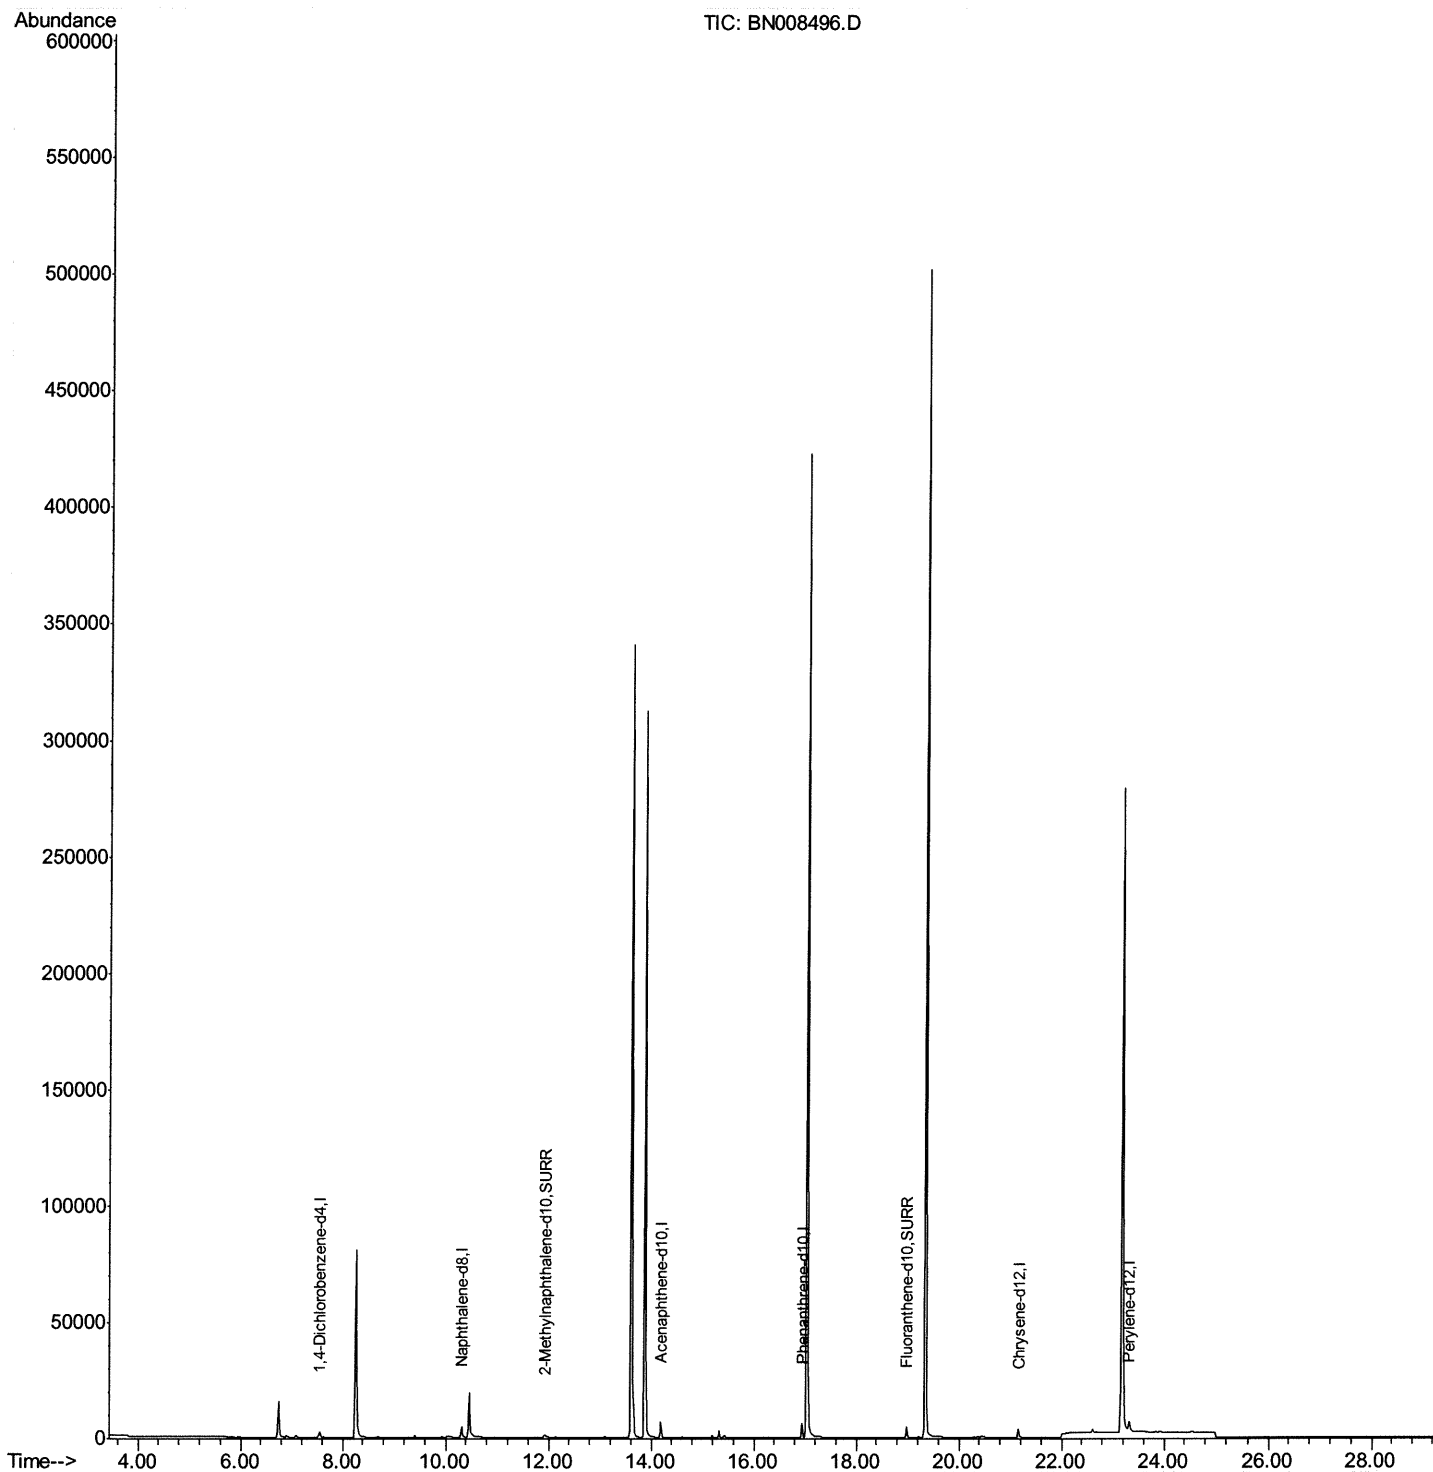

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 06:47:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

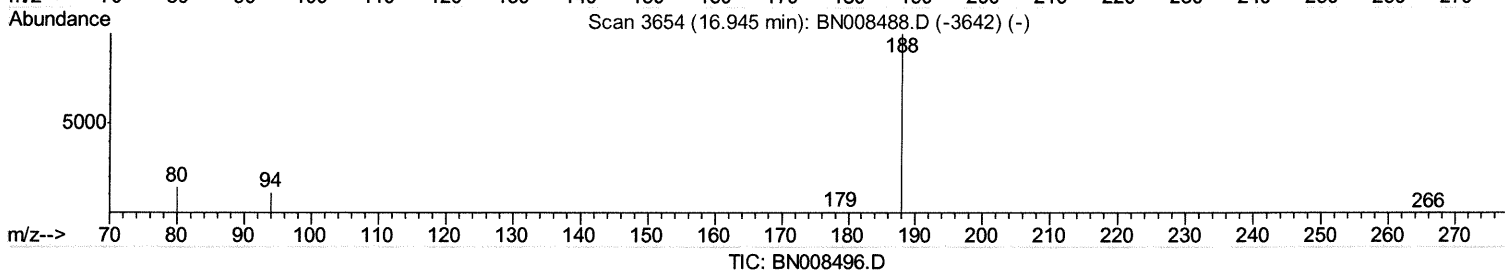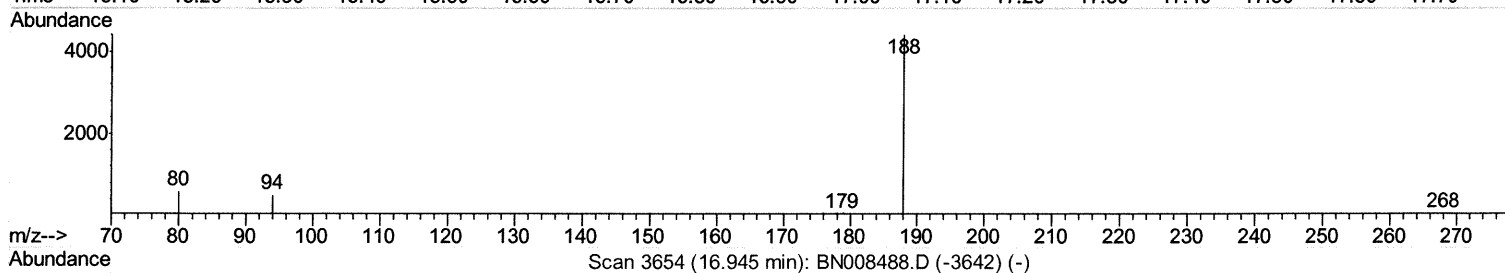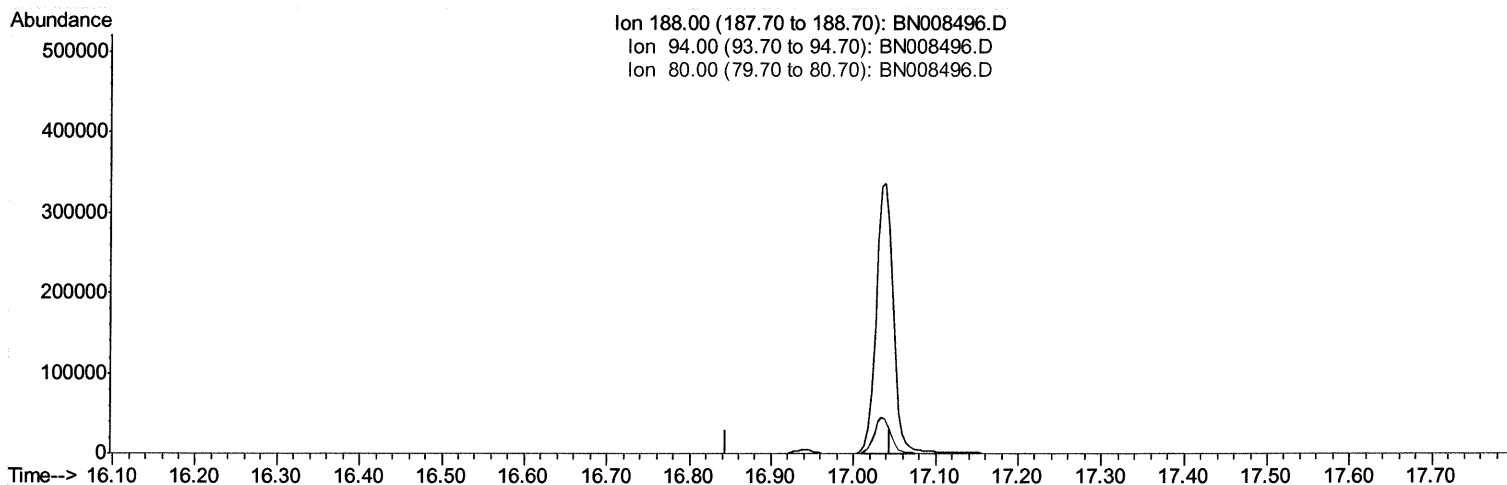

(10) Phenanthrene-d10 (I)

16.945min (-16.945) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.40	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 06:47:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

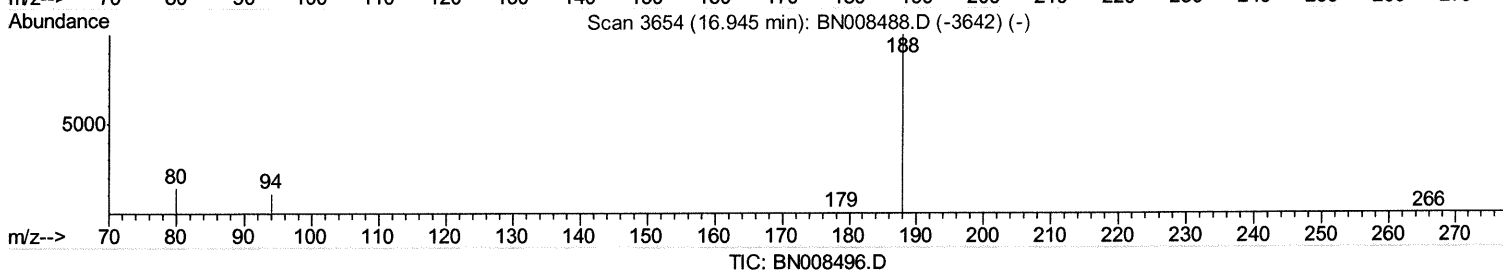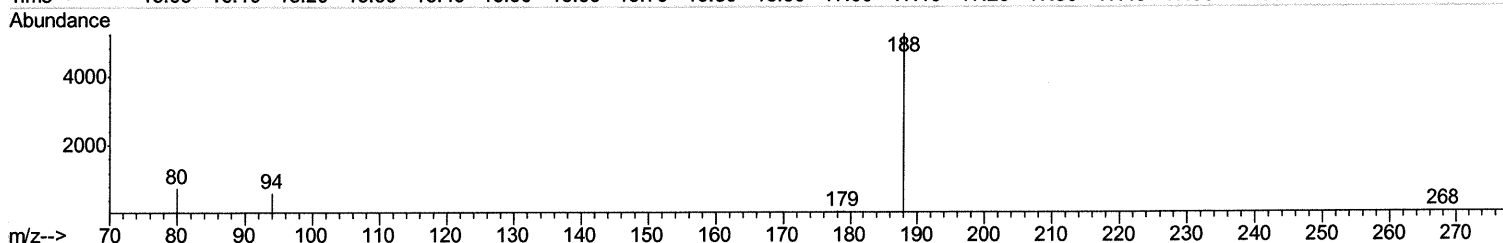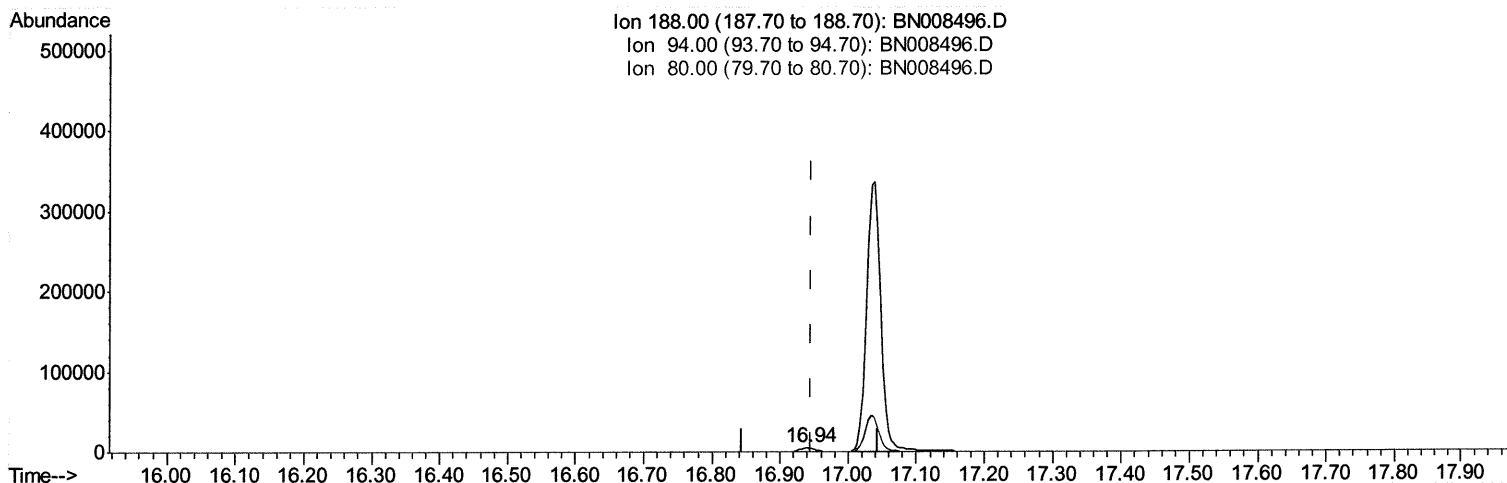

(10) Phenanthrene-d10 (I)

16.941min (-0.004) 0.40ng/ul m JU 11/11/19

response 7453

Ion	Exp%	Act%
188.00	100	100
94.00	12.40	11.72
80.00	15.50	14.30
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 07:32:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

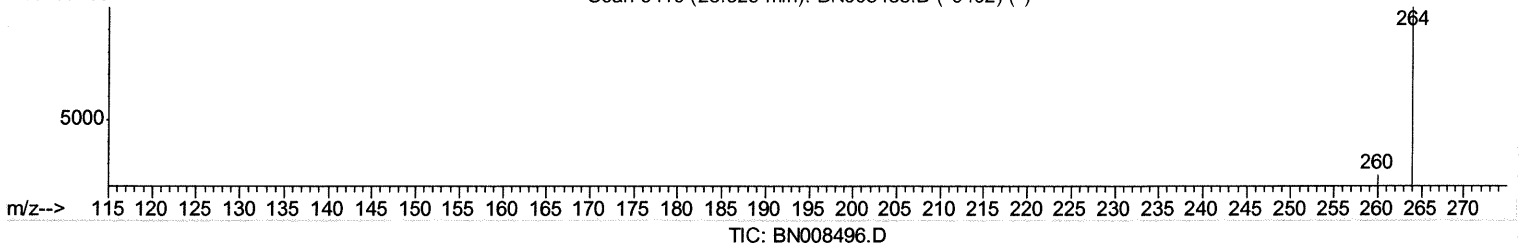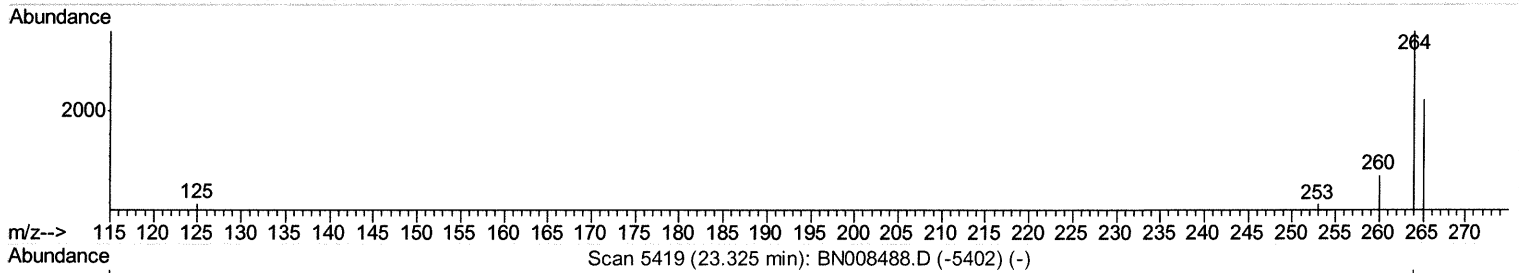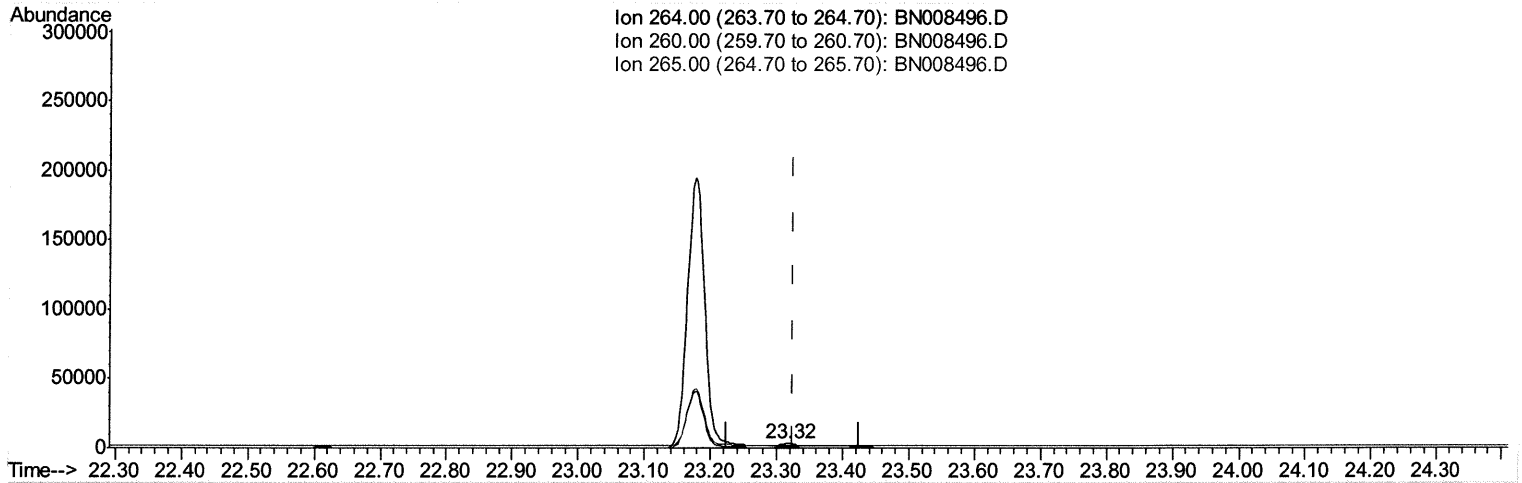

(20) Perylene-d12 (I)

23.317min (-0.008) 0.40ng/ul

response 6355

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	25.63
265.00	98.40	64.66#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (Qedit)




Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 07:32:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

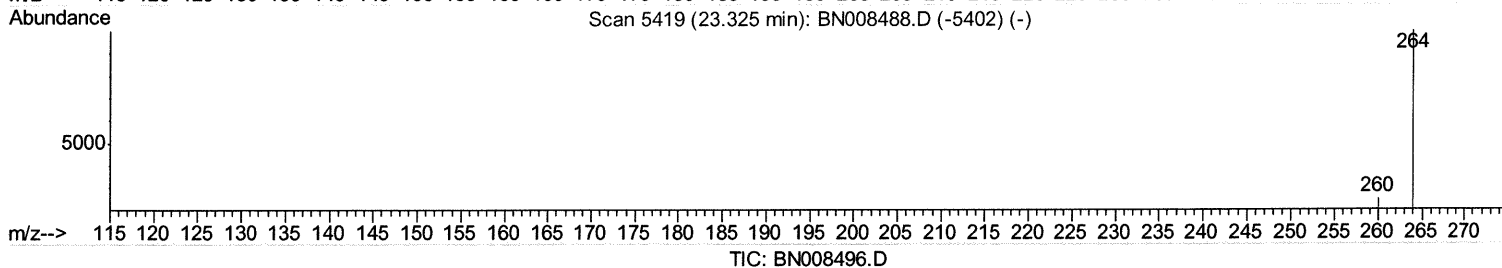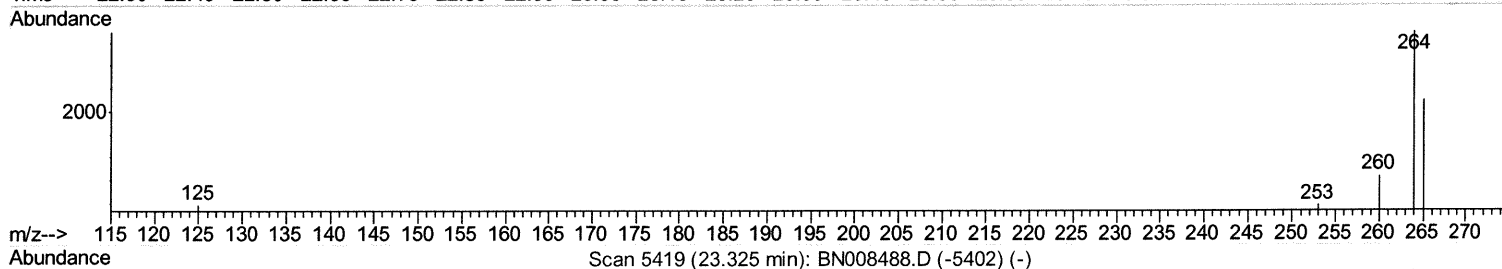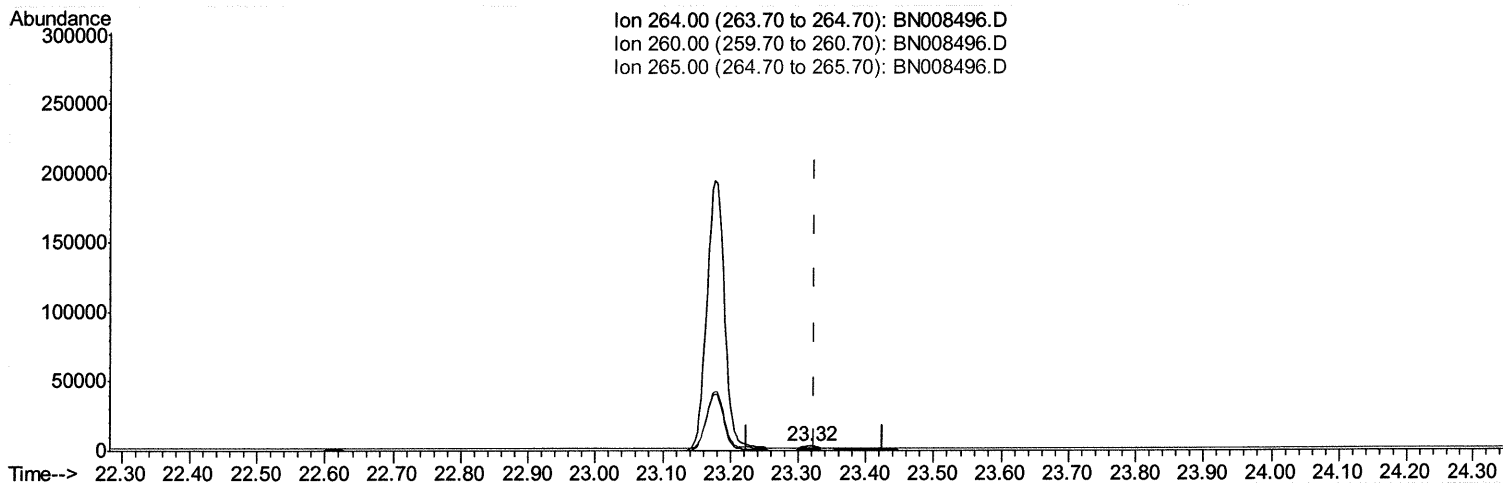

(20) Perylene-d12 (I)

23.317min (-0.008) 0.40ng/ul m JU 11/11/19

response 4004

Ion	Exp%	Act%
264.00	100	100
260.00	27.90	25.63
265.00	98.40	64.66#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN110719\
Quantitation Report (QT Reviewed)

Data File : BN008496.D
Acq On : 07 Nov 2019 22:01
Operator : JU
Sample : K5565-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLNB7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:34 AM

Quant Time: Nov 08 07:32:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1468	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	6520	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.19	164	3768	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	7453m>	0.40	ng/ul>	0.00>
16) Chrysene-d12	21.15	240	4929	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	4004m>	0.40	ng/ul>	0.00>

Ju 11/11/19
Ju 11/11/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.92	152	2473	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	5490	0.25	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed