

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110719\
 Data File : BN008493.D
 Acq On : 07 Nov 2019 20:14
 Operator : JU
 Sample : K5565-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLNA7

Manual Integrations
 APPROVED

mohammad
 11/11/2019 8:08:27 AM

Quant Time: Nov 08 07:28:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 08 06:44:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	1603	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	6818	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3900	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	7020	0.40	ng/ul	0.00
16) Chrysene-d12	21.15	240	4838	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	4528m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	1850	0.17	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	3752	0.18	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.36	128	686	0.035	ng/ul#	73
5) 2-Methylnaphthalene	11.99	142	392	0.030	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110719\
Data File : BN008493.D
Acq On : 07 Nov 2019 20:14
Operator : JU
Sample : K5565-08
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
JLNA7

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:27 AM

Quant Time: Nov 08 07:28:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN110519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 08 06:44:20 2019
Response via : Initial Calibration

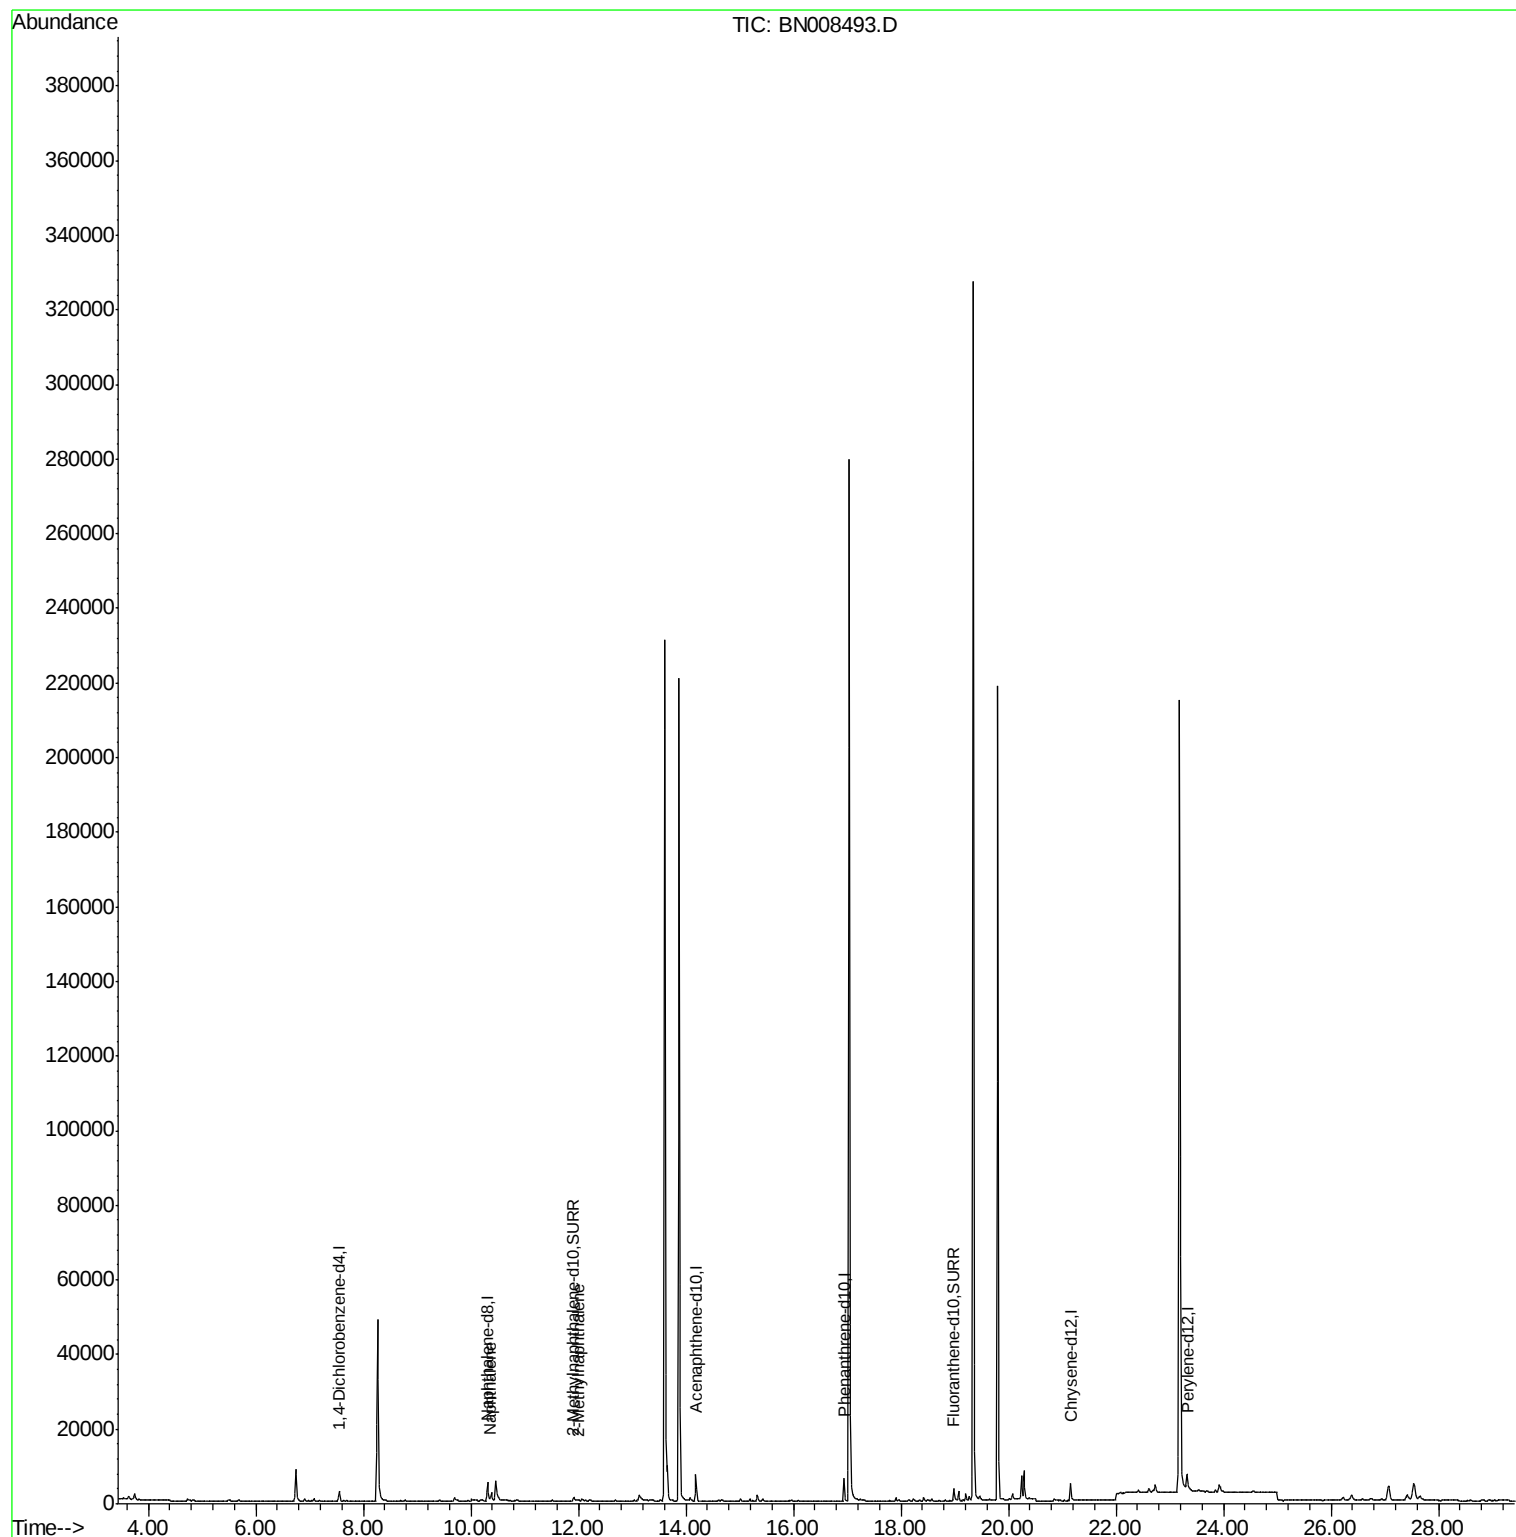

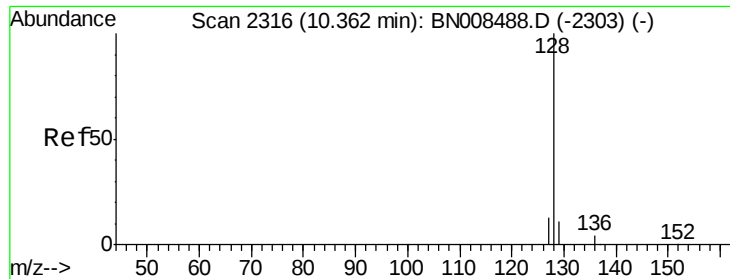

#3

Naphthalene

Concen: 0.035 ng/ul

RT: 10.36 min Scan# 2315

Delta R.T. -0.01 min

Lab File: BN008493.D

Acq: 07 Nov 2019 20:14

Instrument :

BNA_N





ClientSampleId :

JLNA7

Tot Ion:	128	Resp:	686
Ion Ratio	Lower	Upper	
128	100		
129	24.9	10.0	15.0#
127	23.6	11.6	17.4#

Manual Integrations
APPROVED

mohammad
11/11/2019 8:08:27 AM

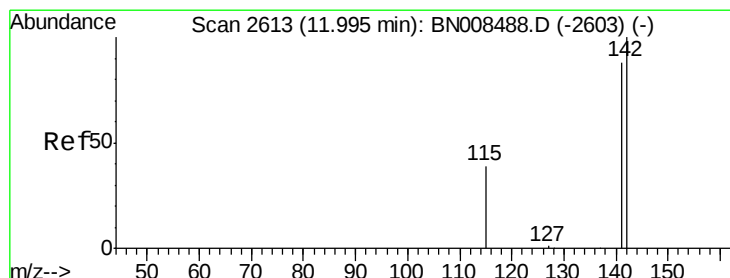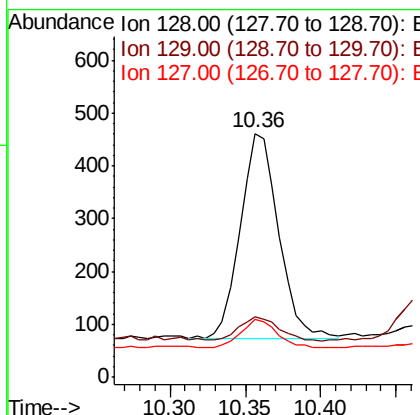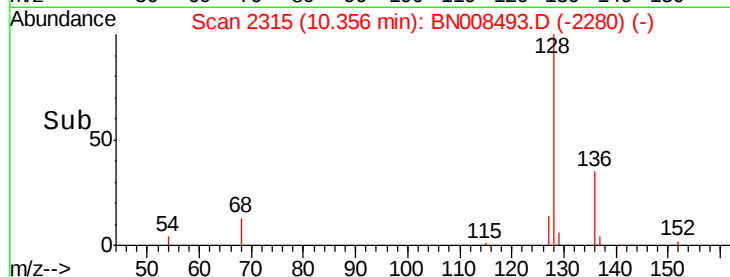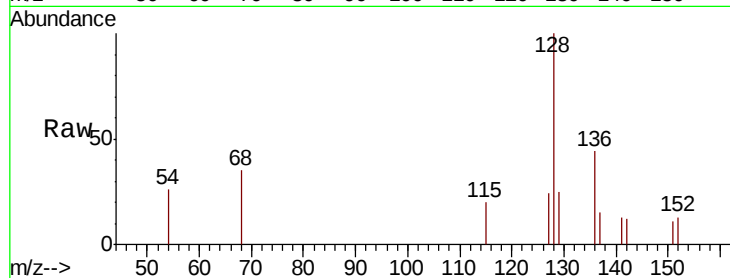

#5

2-Methylnaphthalene

Concen: 0.030 ng/ul

RT: 11.99 min Scan# 2612

Delta R.T. -0.01 min

Lab File: BN008493.D

Acq: 07 Nov 2019 20:14

Tgt Ion:	142	Resp:	392
Ion Ratio	Lower	Upper	
142	100		
141	94.9	72.8	109.2

