
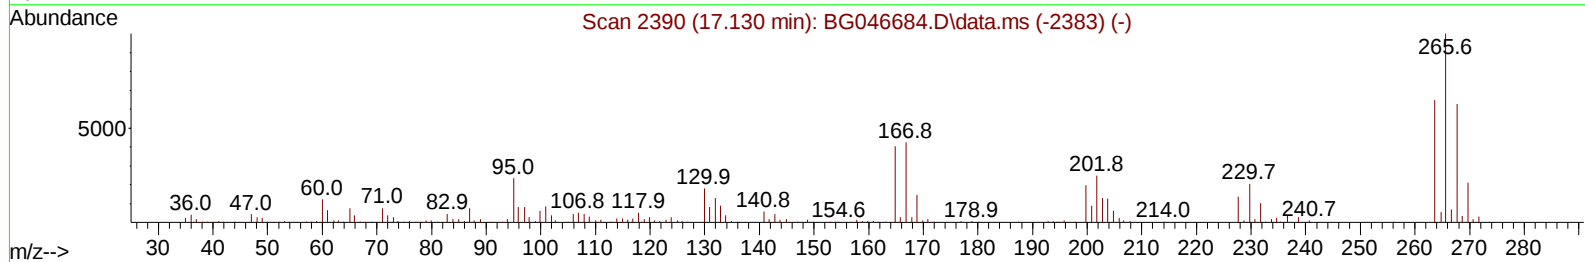
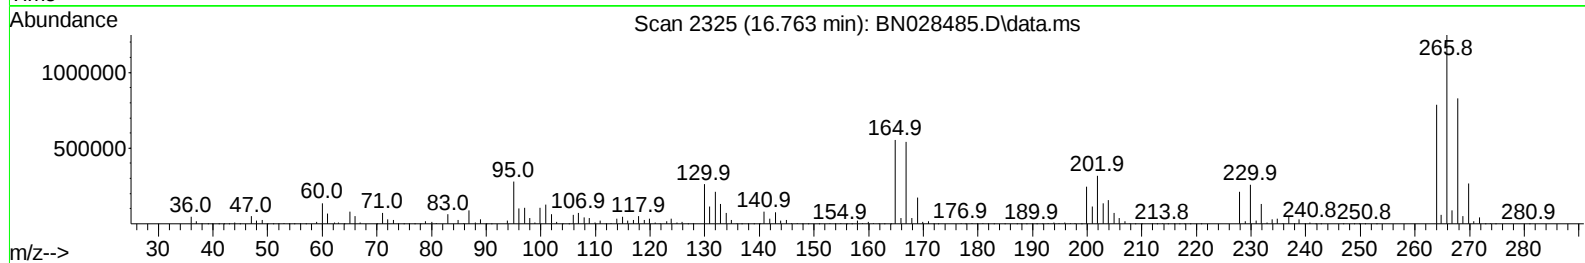


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110723\
Data File : BN028485.D
Acq On : 07 Nov 2023 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 03:31:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 03:31:26 2023
Response via : Initial Calibration

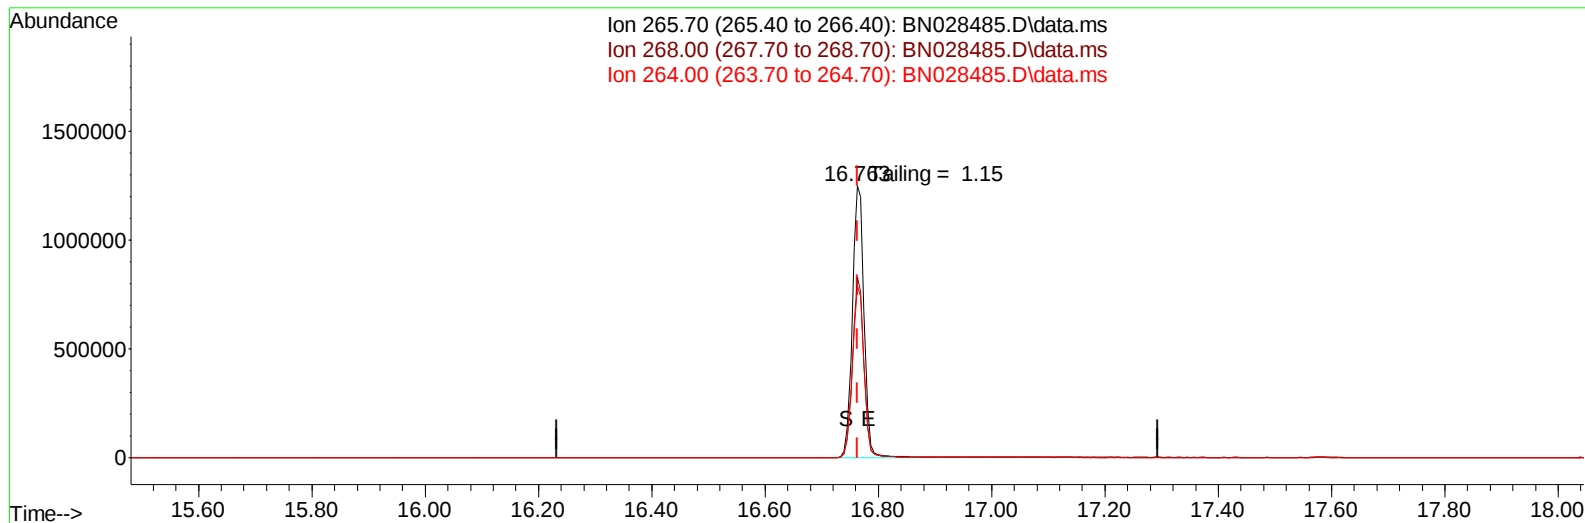




TIC: BN028485.D\data.ms

(70) Pentachlorophenol (C)**16.763min (0.000) 28130.70 ng****response 1796787**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.43
264.00	61.60	62.99
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110723\
Data File : BN028485.D
Acq On    : 07 Nov 2023 10:49
Operator  : MA/JU
Sample    : DFTPP
Misc      :
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 08 03:31:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 03:31:26 2023
Response via : Initial Calibration

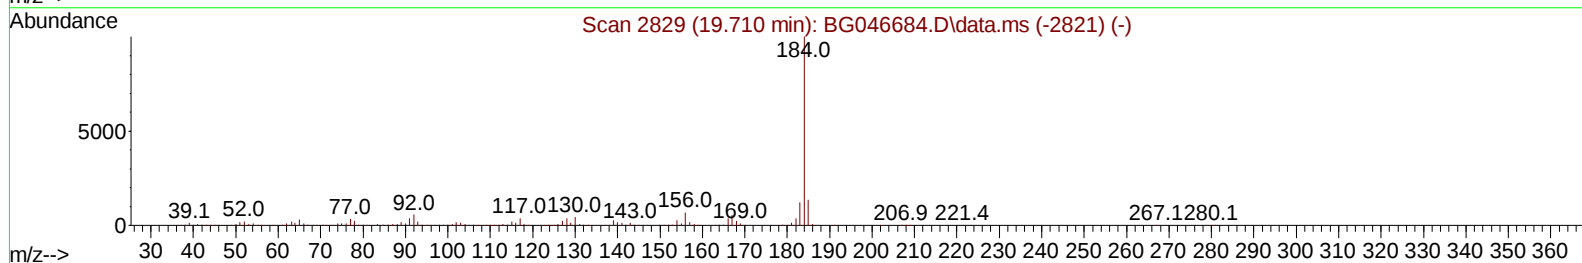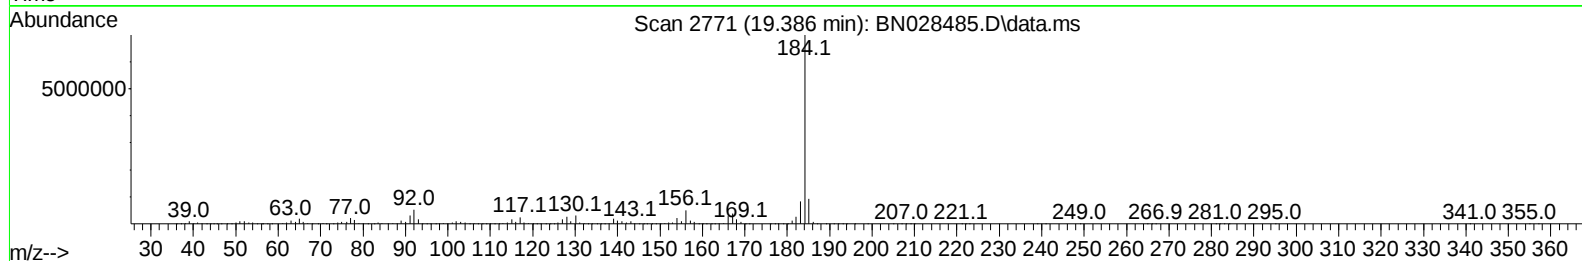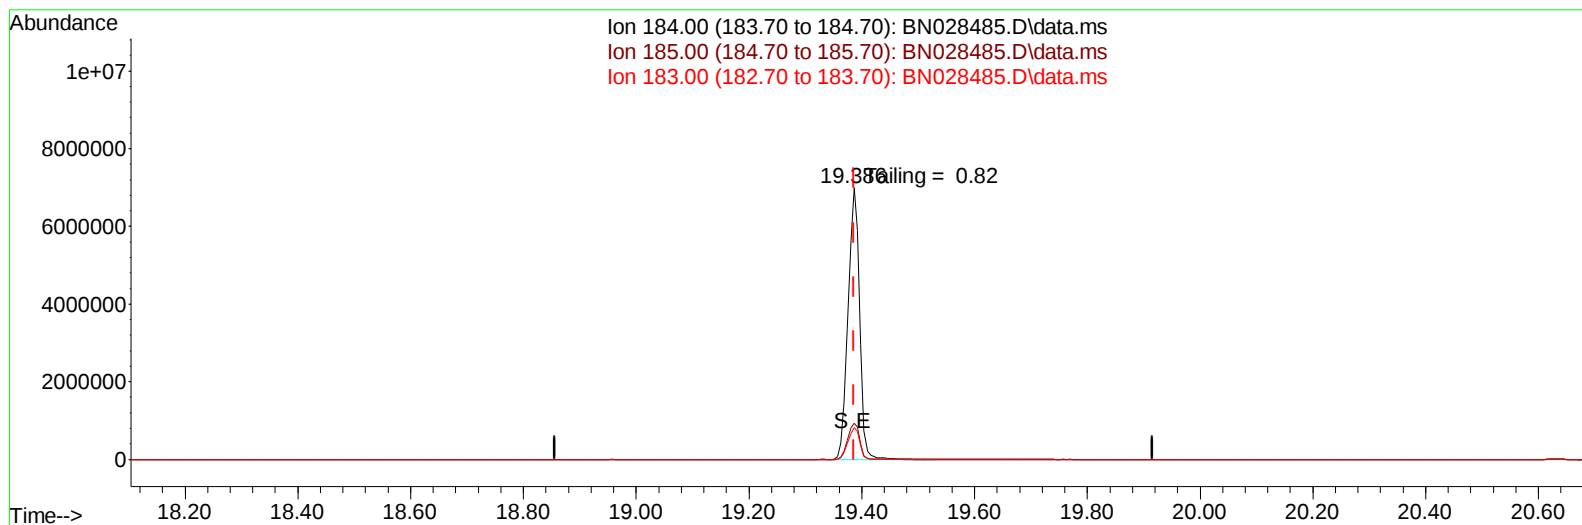

TIC: BN028485.D\data.ms

(77) Benzidine

19.386min (0.000) 2753800.49 ng

response **10016657**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.34
183.00	13.20	11.72
0.00	0.00	0.00