


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110723\
Data File : BN028485.D
Acq On : 07 Nov 2023 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 08 00:27:19 2023

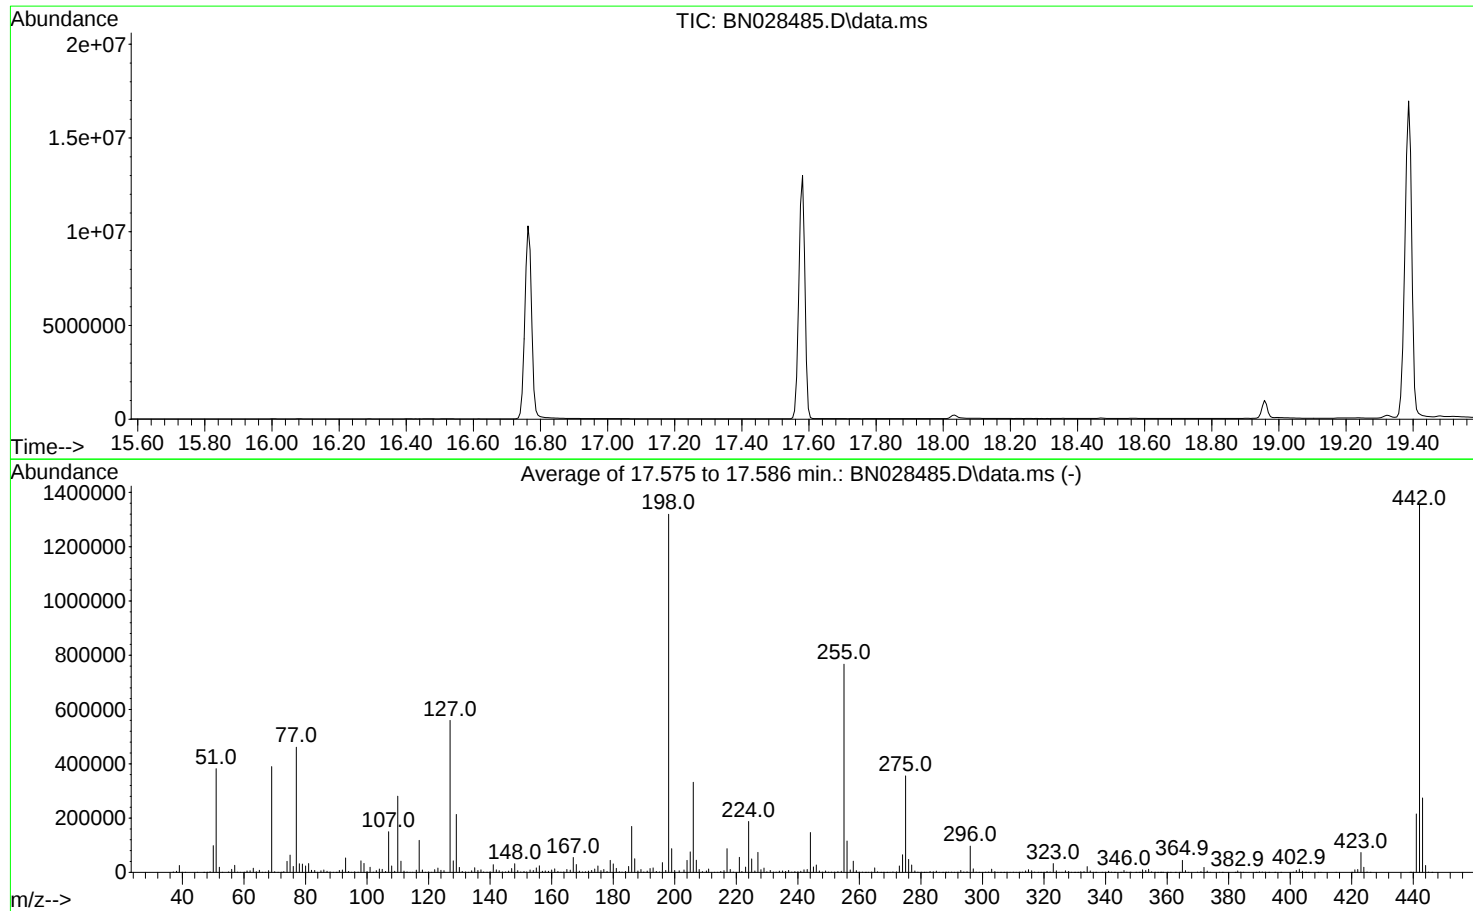




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	382153	PASS
68	69	0.00	2	1.8	6847	PASS
69	198	0.00	100	29.5	389837	PASS
70	69	0.00	2	0.5	2134	PASS
127	198	10	80	42.4	559915	PASS
197	198	0.00	2	0.5	7096	PASS
198	198	100	100	100.0	1319701	PASS
199	198	5	9	6.6	87280	PASS
275	198	10	60	26.9	355477	PASS
365	198	1	100	3.4	44512	PASS
441	198	0.01	100	16.3	214955	PASS
442	442	50	100	100.0	1355435	PASS
443	442	15	24	20.2	274368	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110723\
Data File : BN028485.D
Acq On : 07 Nov 2023 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 03:31:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 03:31:26 2023
Response via : Initial Calibration

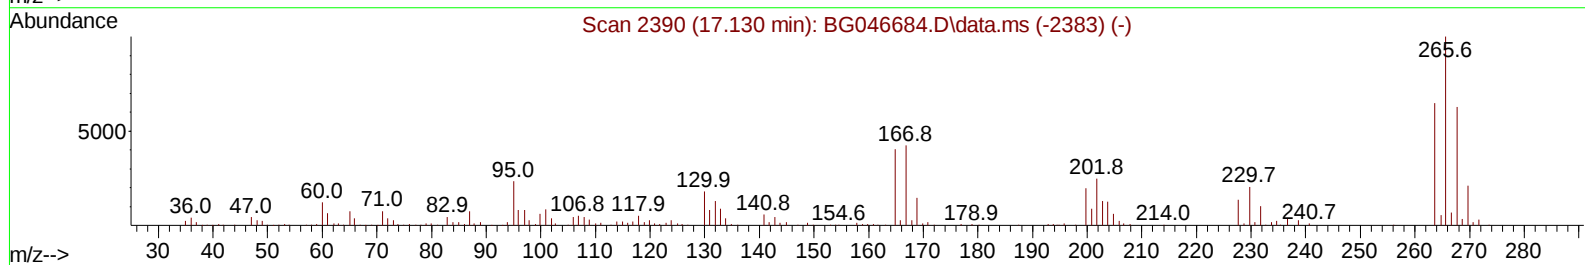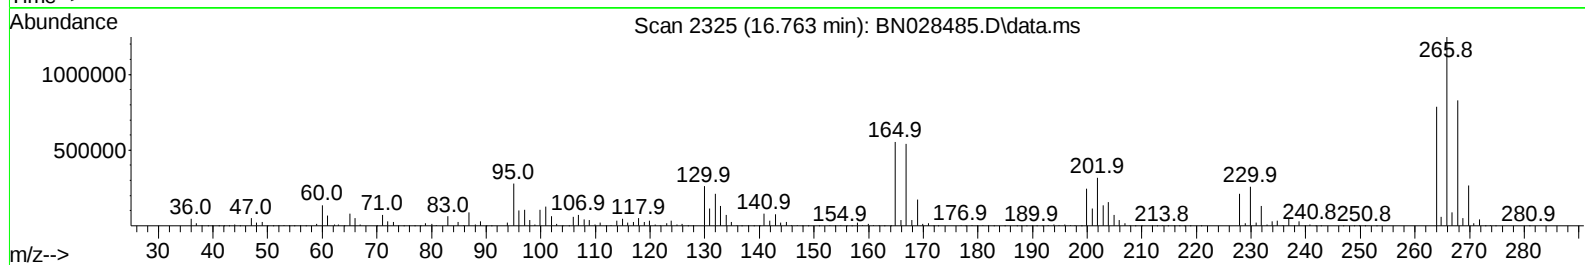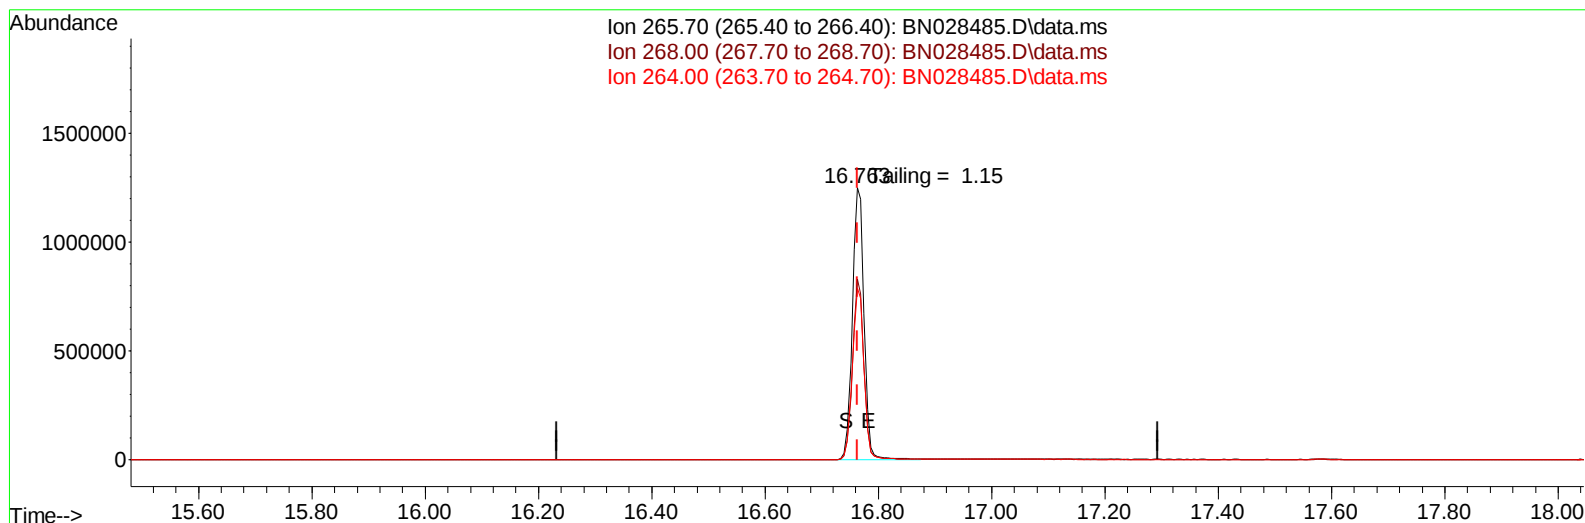

TIC: BN028485.D\data.ms

(70) Pentachlorophenol (C)

16.763min (0.000) 28130.70 ng




response 1796787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.43
264.00	61.60	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110723\
Data File : BN028485.D
Acq On : 07 Nov 2023 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 08 03:31:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 08 03:31:26 2023
Response via : Initial Calibration

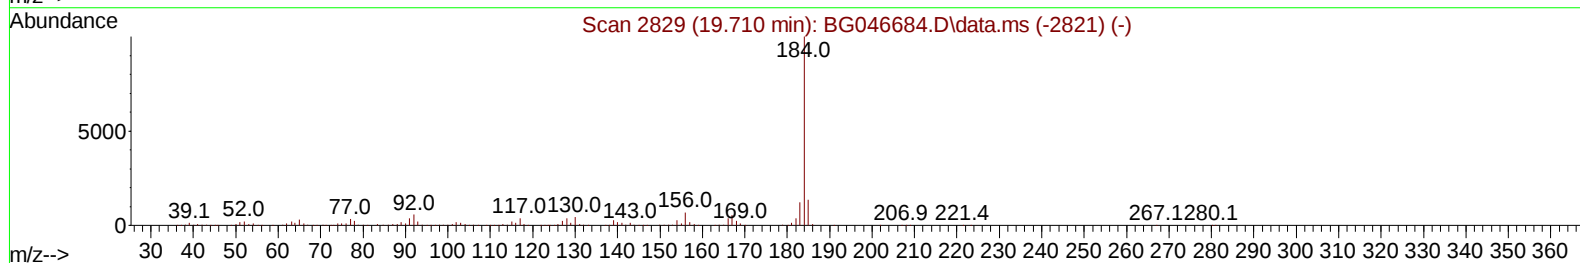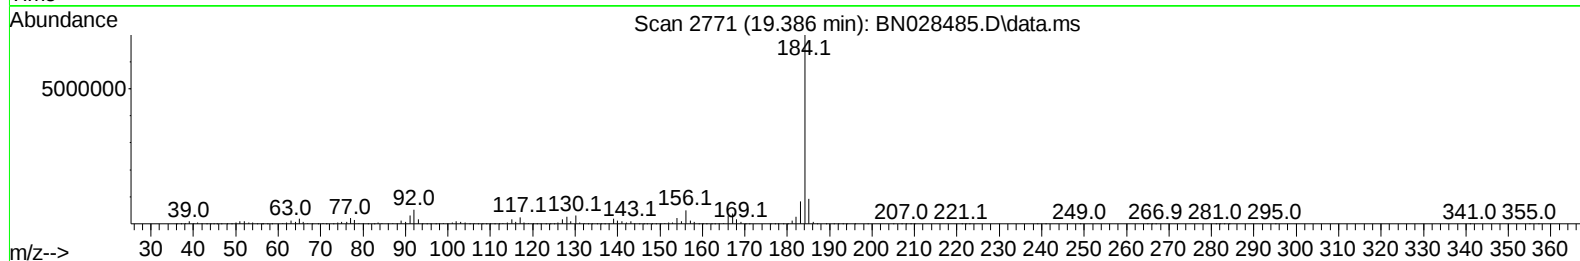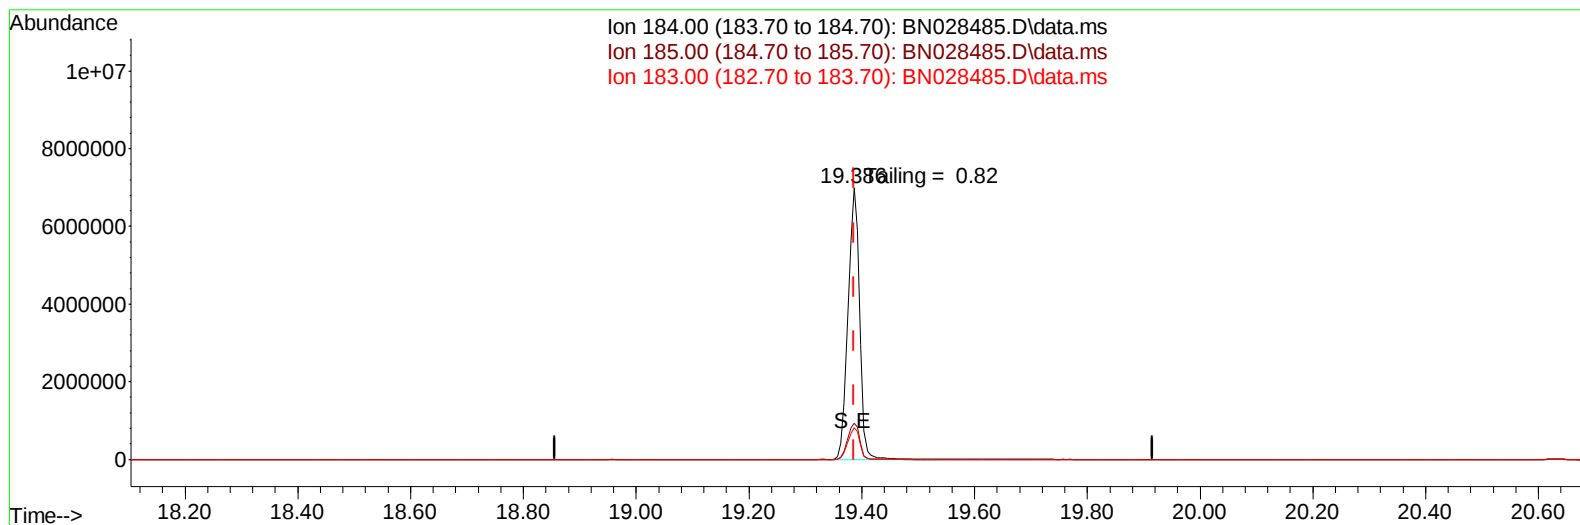

TIC: BN028485.D\data.ms

(77) Benzidine

19.386min (0.000) 2753800.49 ng

response 10016657

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.34
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/7/2023	BNA_N	<u>BN028485.D</u>
Compound Name	Response	Retention Time
DDT	4976828	20.633
DDD	49397	20.239
DDE	2591	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
51988	5028816	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP