
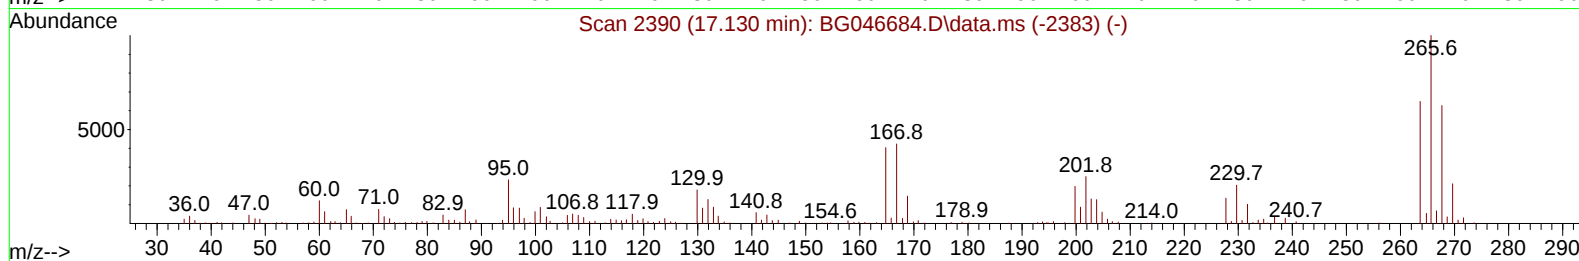
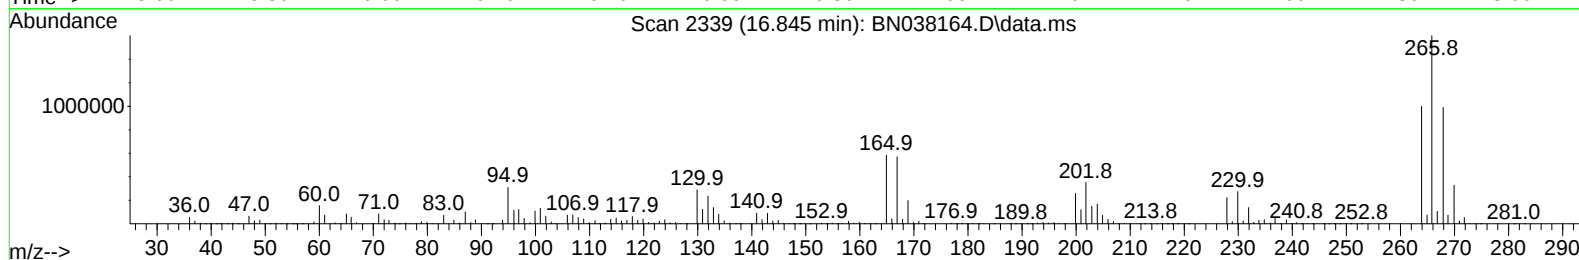


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038164.D
Acq On : 07 Nov 2025 21:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 04:08:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 08 04:08:47 2025
Response via : Initial Calibration

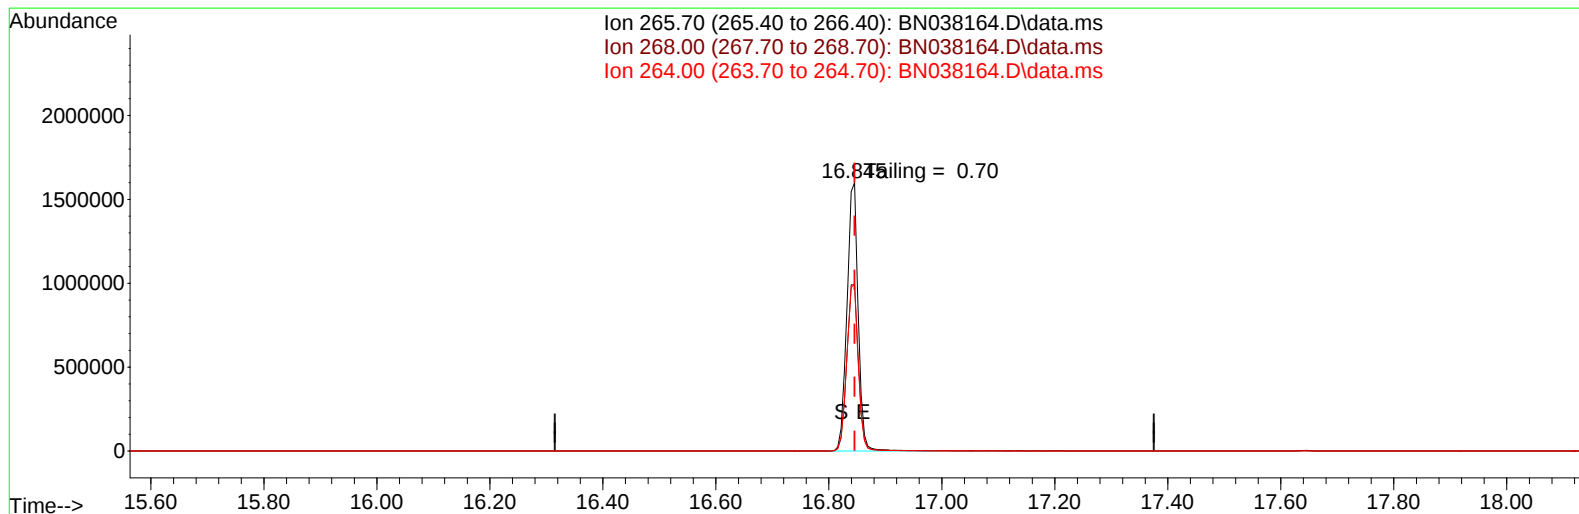

TIC: BN038164.D\data.ms

(70) Pentachlorophenol (C)




16.845min (0.000) 236023.12 ng

response 2207882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.90
264.00	61.60	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110725\
Data File : BN038164.D
Acq On : 07 Nov 2025 21:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 04:08:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 08 04:08:47 2025
Response via : Initial Calibration

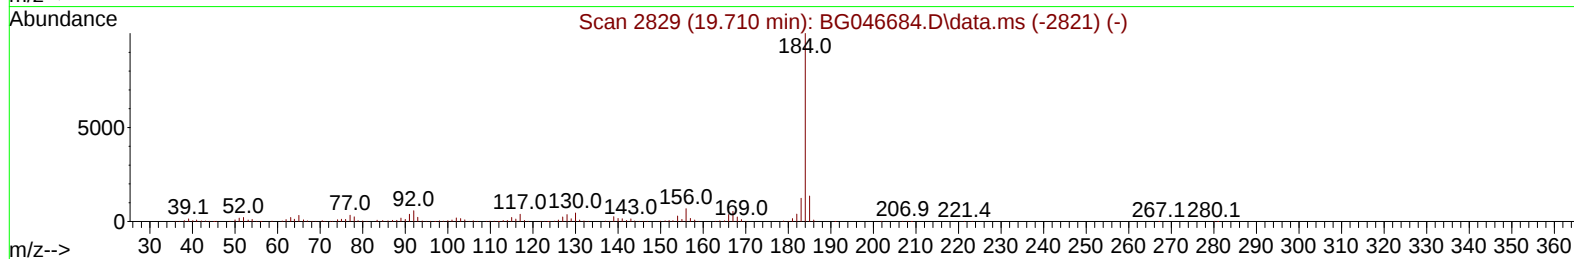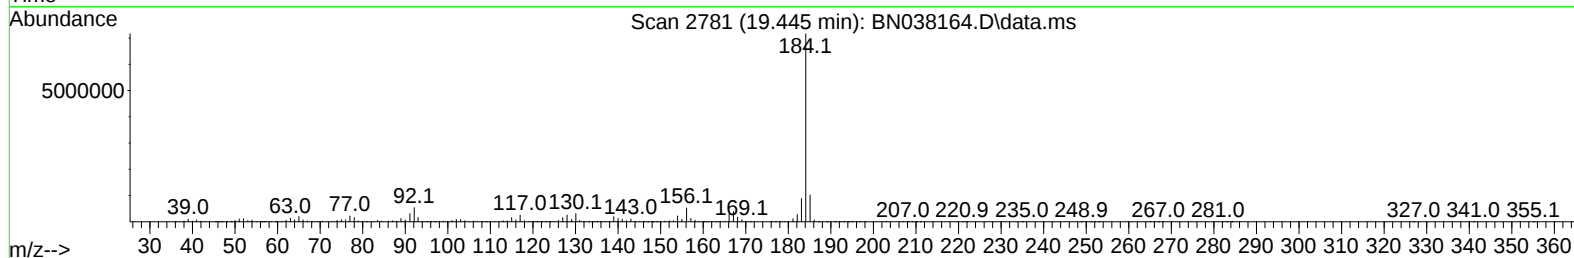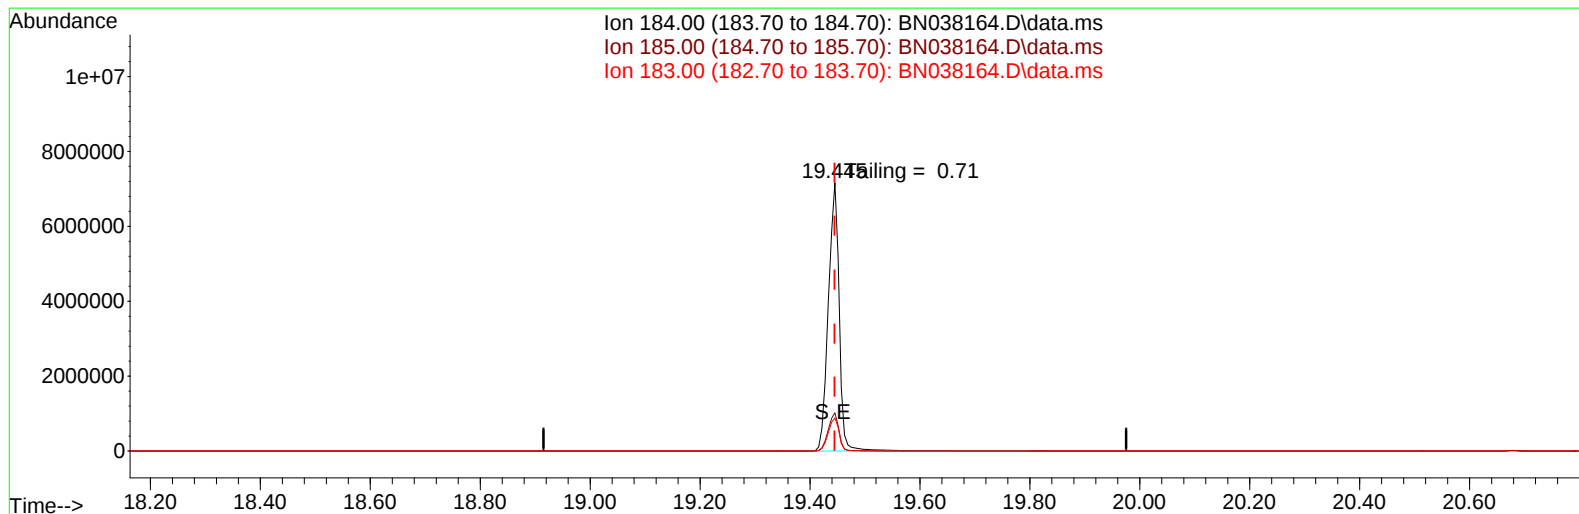

TIC: BN038164.D\data.ms

(77) Benzidine

19.445min (0.000) 4251.91 ng m

response 9910482

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	12.38
0.00	0.00	0.00