

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110821\
 Data File : BN017337.D
 Acq On : 08 Nov 2021 16:31
 Operator : CG/JU
 Sample : M4412-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG365

Quant Time: Nov 08 17:00:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 11:43:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.515	152	5156	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	20731	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	12962	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.919	188	27903	0.400	ng/ul	0.00
17) Chrysene-d12	21.133	240	23422	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	24743	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	27243	4.752	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	10745	0.355	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	28072	0.457	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.962	178	3292	0.037	ng/ul#	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110821\
Data File : BN017337.D
Acq On : 08 Nov 2021 16:31
Operator : CG/JU
Sample : M4412-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG365

Quant Time: Nov 08 17:00:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 08 11:43:44 2021
Response via : Initial Calibration

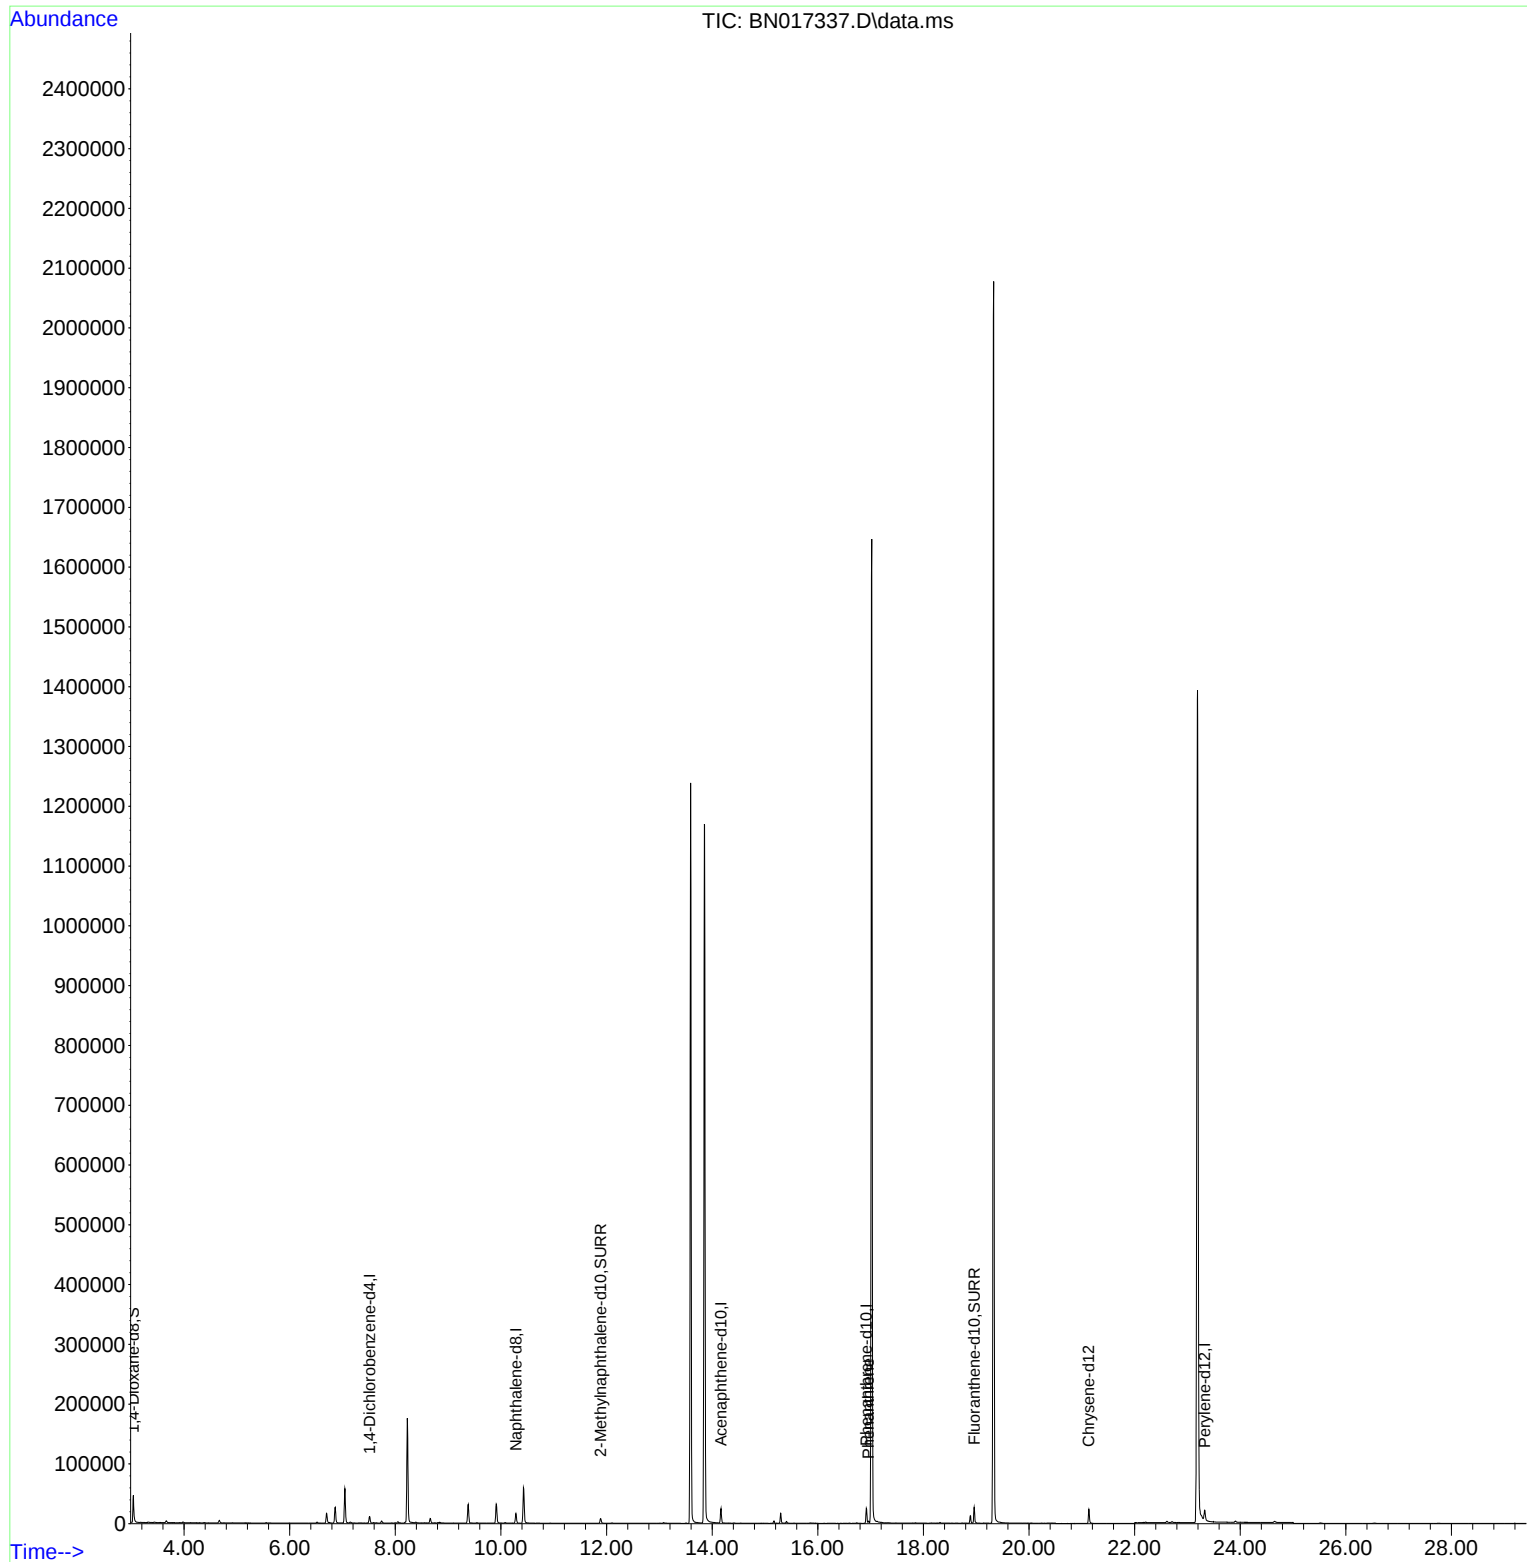

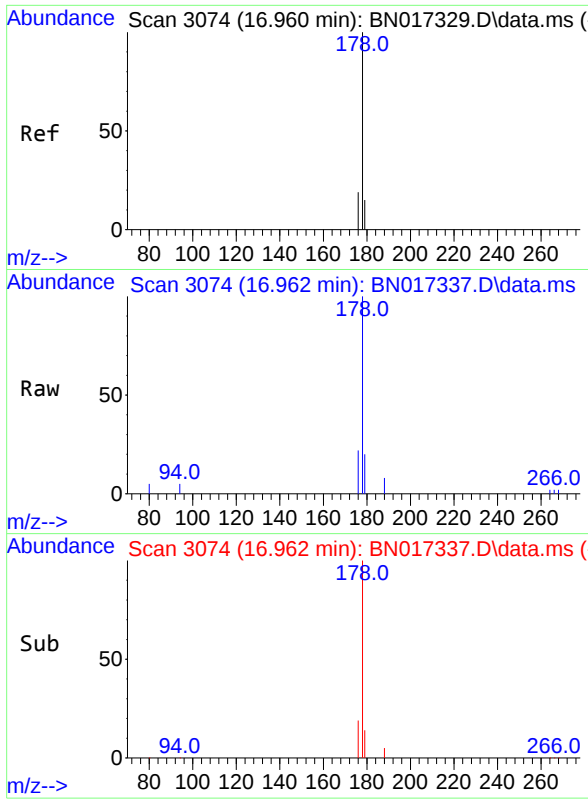

#15
Phenanthrene
Concen: 0.037 ng/ul
RT: 16.962 min Scan# 3074
Delta R.T. 0.001 min
Lab File: BN017337.D
Acq: 08 Nov 2021 16:31

Instrument :
BNA_N
ClientSampleId :
BG365

Tgt Ion:	178	Resp:	3292
Ion	Ratio	Lower	Upper
178	100		
179	19.8	12.6	19.0#
176	22.2	15.5	23.3

