
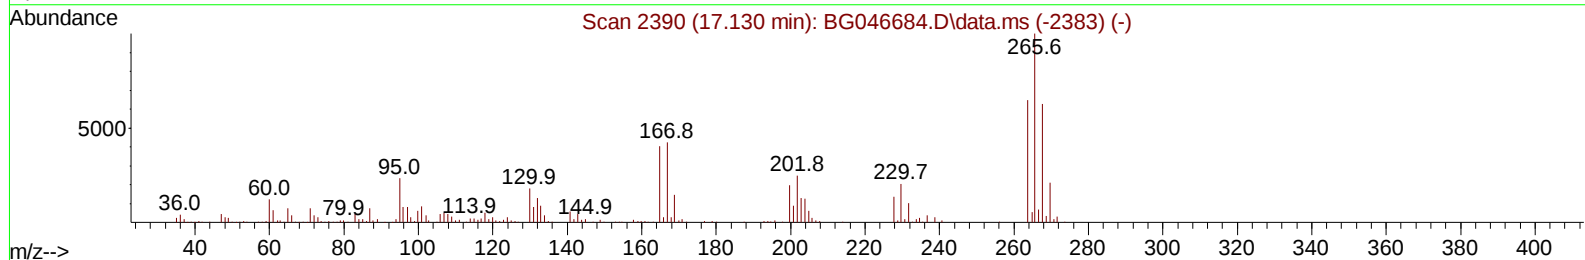
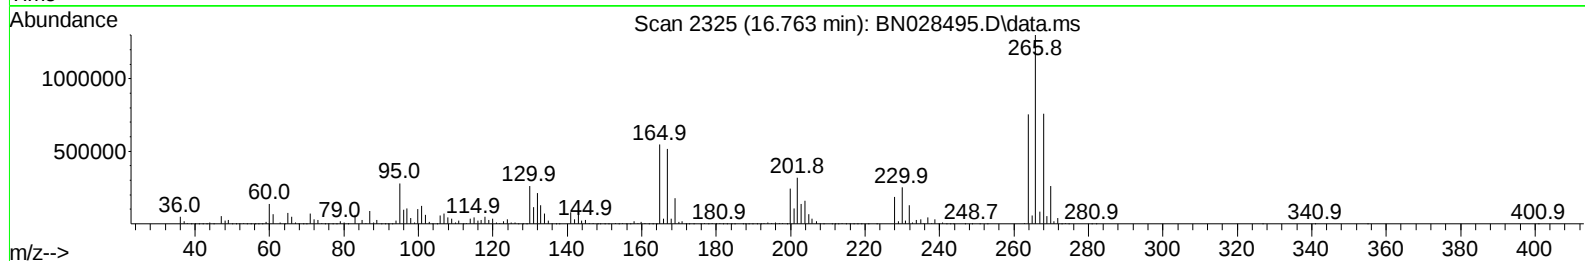


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
Data File : BN028495.D
Acq On : 08 Nov 2023 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 00:51:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 00:51:48 2023
Response via : Initial Calibration

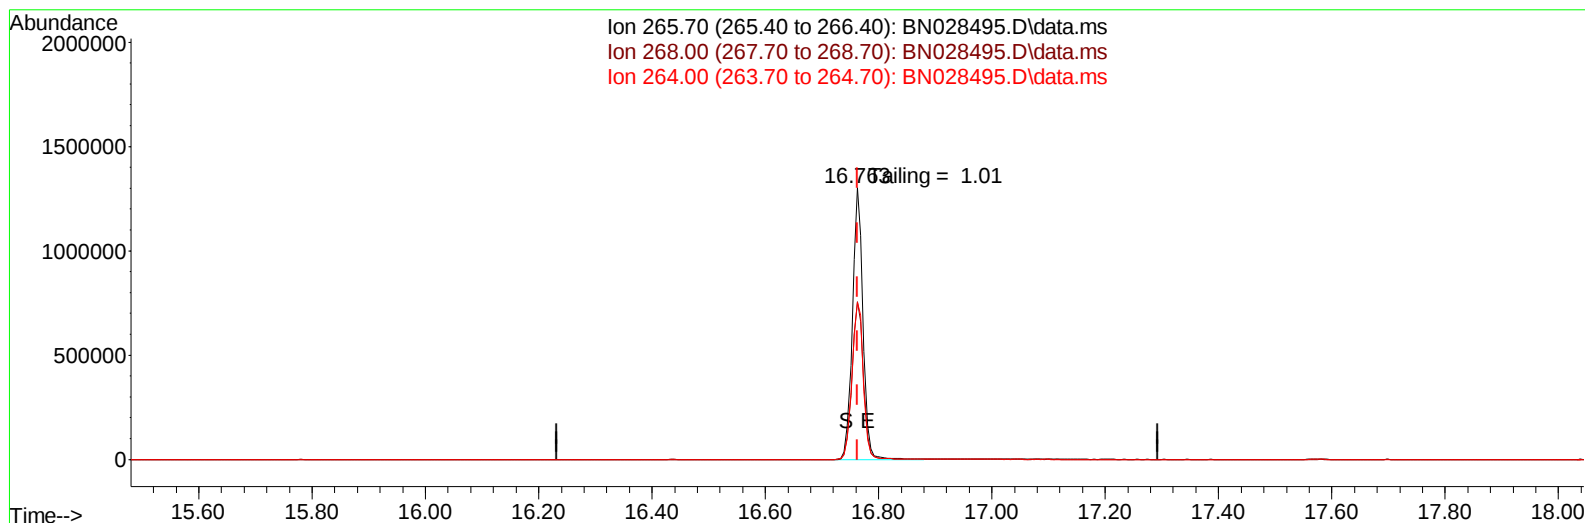

TIC: BN028495.D\data.ms

(70) Pentachlorophenol (C)




16.763min (0.000) 28770.22 ng

response 1698328

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.23
264.00	61.60	57.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
Data File : BN028495.D
Acq On : 08 Nov 2023 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 00:51:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 00:51:48 2023
Response via : Initial Calibration

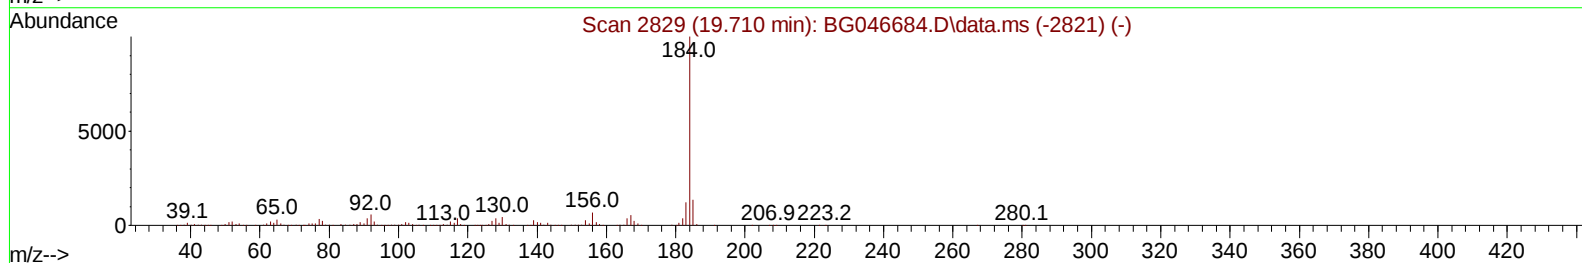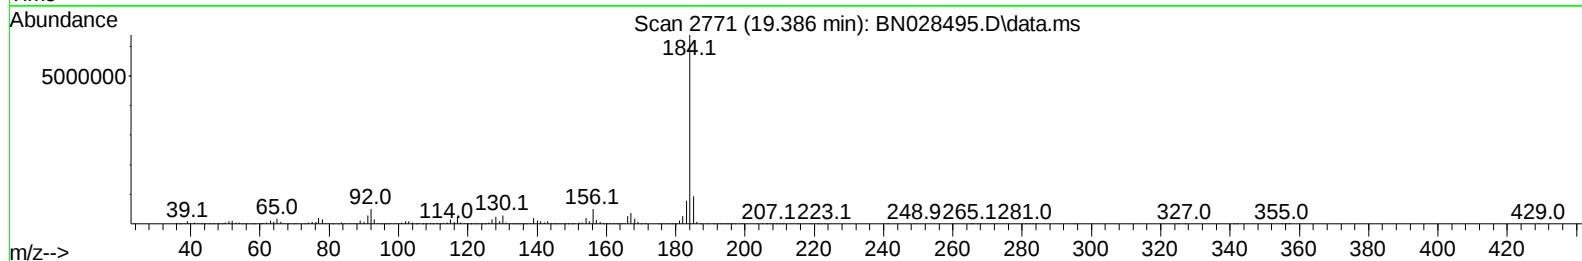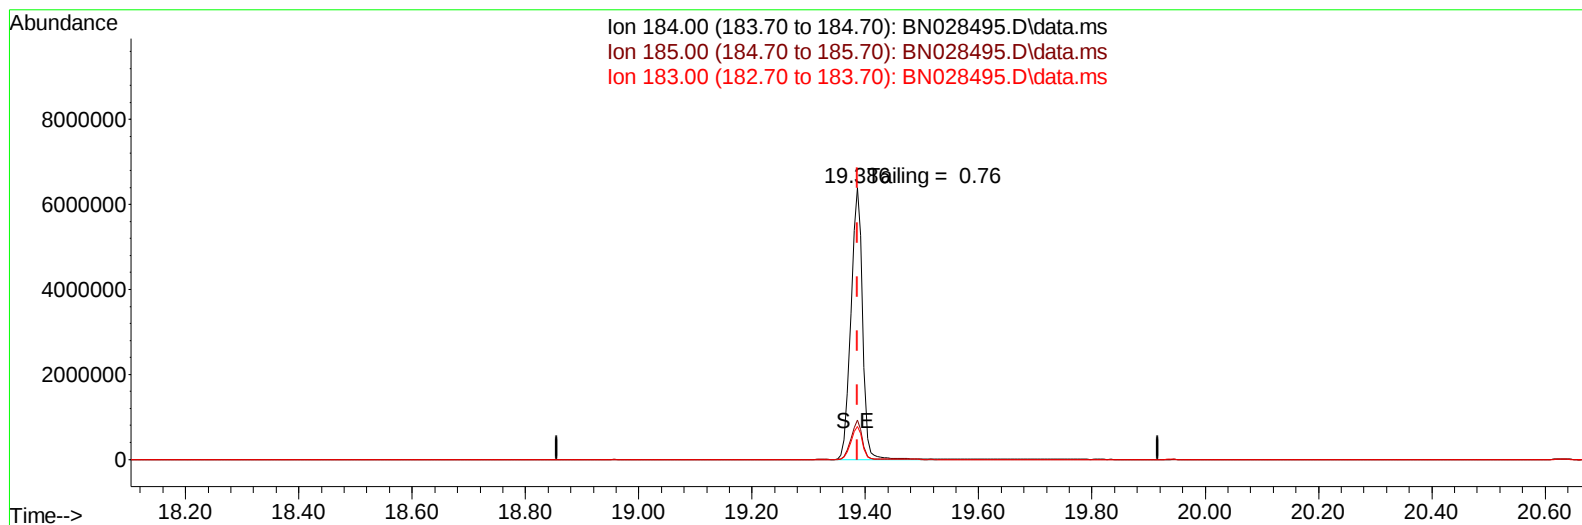

TIC: BN028495.D\data.ms

(77) Benzidine**19.386min (0.000) 2329309.91 ng****response 9190636**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	12.08
0.00	0.00	0.00