
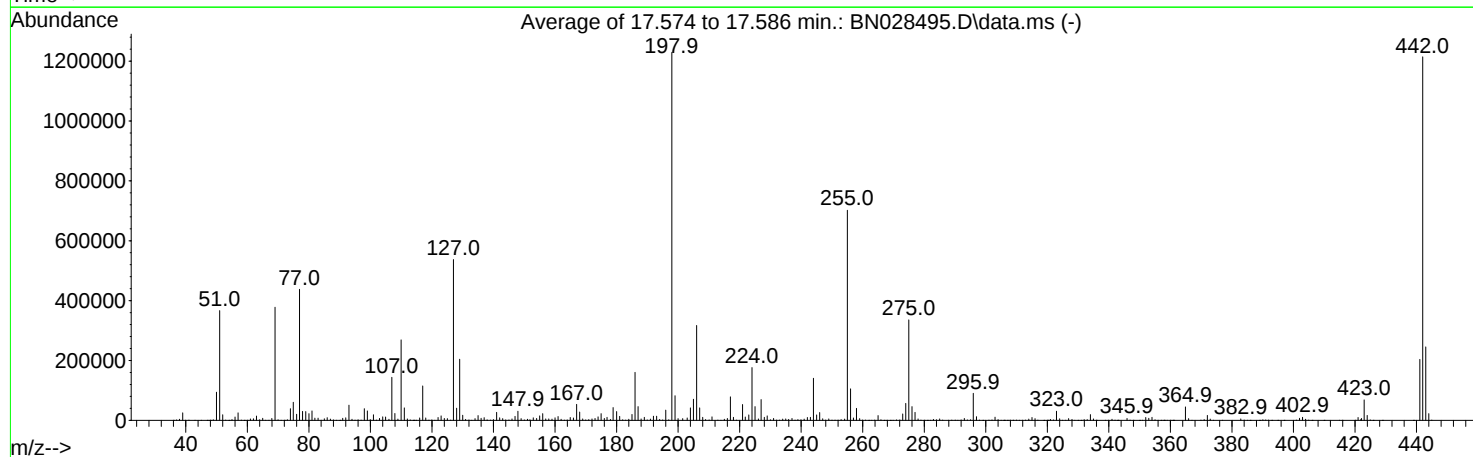


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
Data File : BN028495.D
Acq On : 08 Nov 2023 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 08 00:27:19 2023

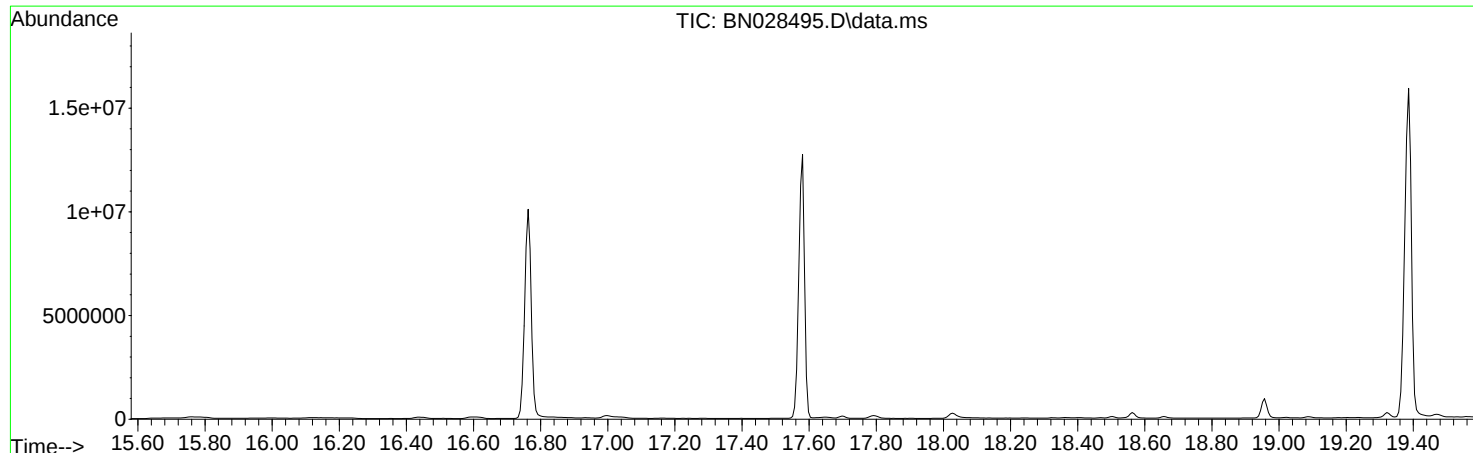




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	366883	PASS
68	69	0.00	2	1.6	6210	PASS
69	198	0.00	100	30.7	377760	PASS
70	69	0.00	2	0.6	2142	PASS
127	198	10	80	43.7	536960	PASS
197	198	0.00	2	0.2	2413	PASS
198	198	100	100	100.0	1228864	PASS
199	198	5	9	6.7	82571	PASS
275	198	10	60	27.3	335531	PASS
365	198	1	100	3.6	44819	PASS
441	198	0.01	100	16.6	203776	PASS
442	442	50	100	100.0	1214528	PASS
443	442	15	24	20.2	245397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
Data File : BN028495.D
Acq On : 08 Nov 2023 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 09 00:51:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 00:51:48 2023
Response via : Initial Calibration

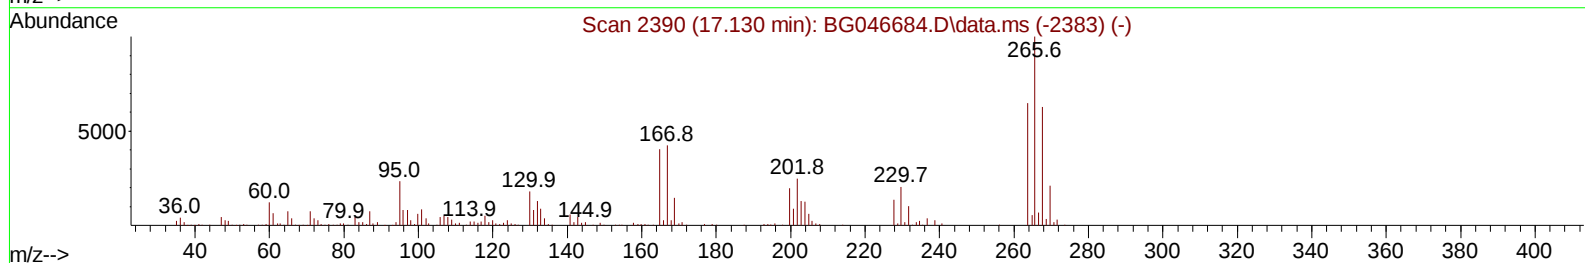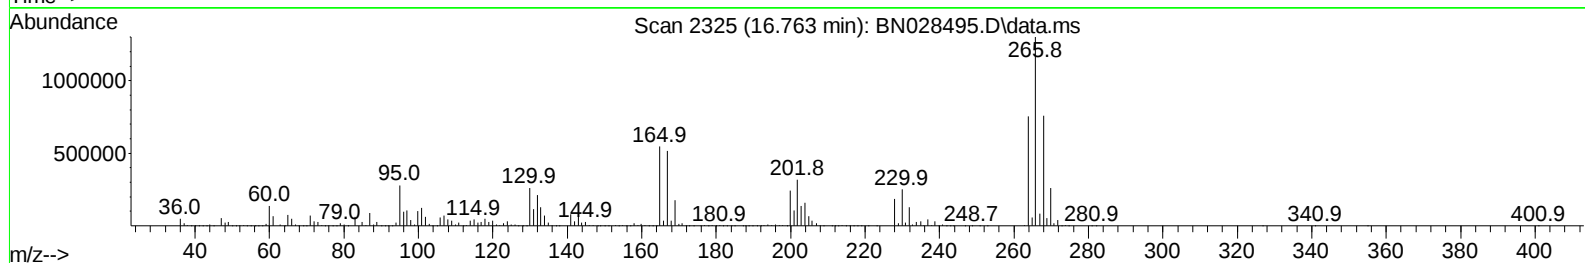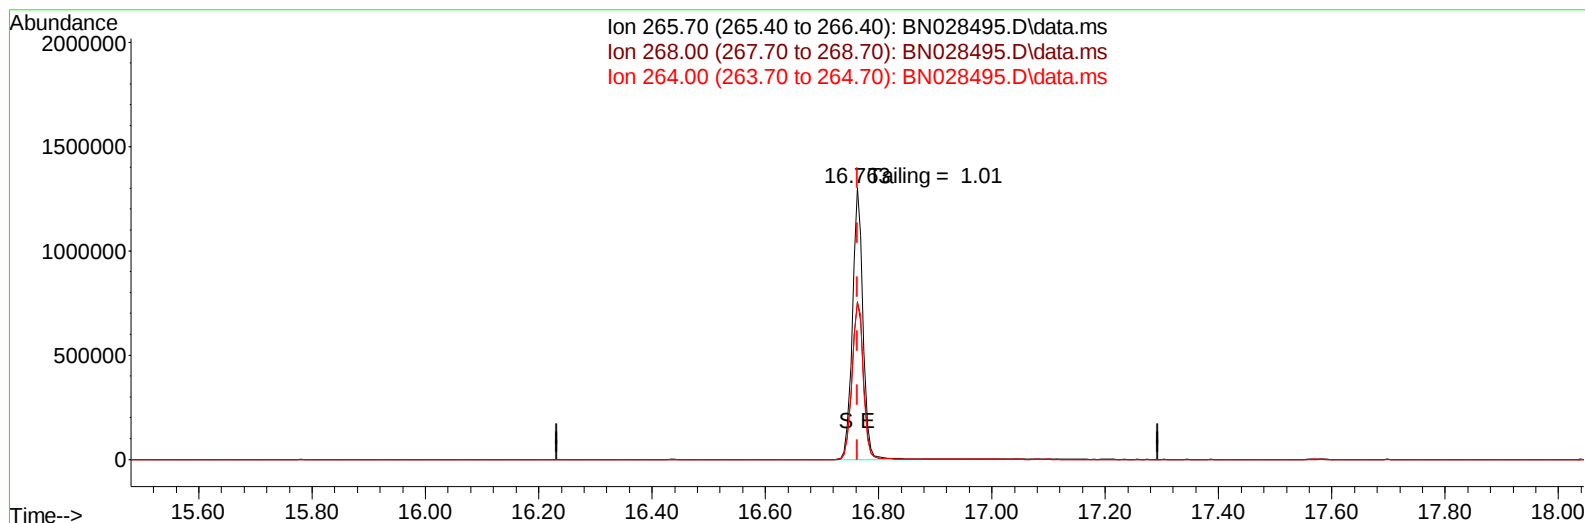

TIC: BN028495.D\data.ms

(70) Pentachlorophenol (C)

16.763min (0.000) 28770.22 ng




response 1698328

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.23
264.00	61.60	57.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
 Data File : BN028495.D
 Acq On : 08 Nov 2023 08:54
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 00:51:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 00:51:48 2023
 Response via : Initial Calibration

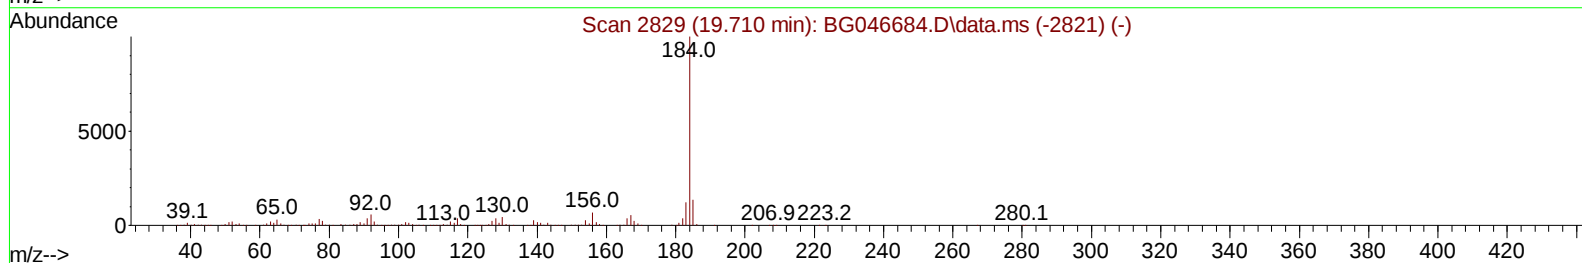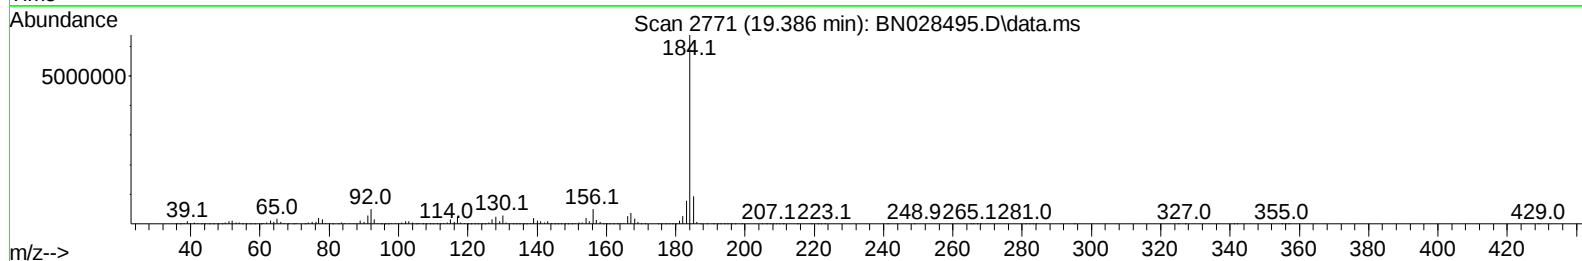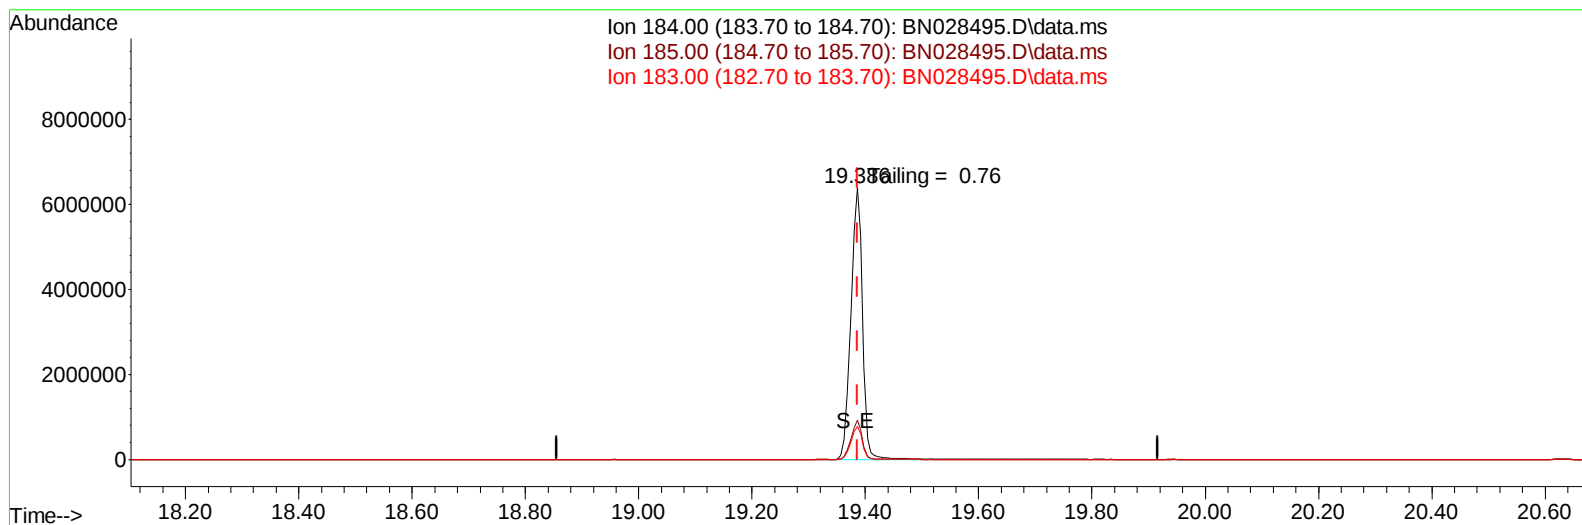

TIC: BN028495.D\data.ms

(77) Benzidine**19.386min (0.000) 2329309.91 ng****response 9190636**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/8/2023	BNA_N	<u>BN028495.D</u>
Compound Name	Response	Retention Time
DDT	4662179	20.633
DDD	47520	20.239
DDE	2230	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49750	4711929	1.06

Instrument :
BNA_N
ClientSampleId :
DFTPP