


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110823\
 Data File : BN028506.D
 Acq On : 08 Nov 2023 19:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 08 00:27:19 2023

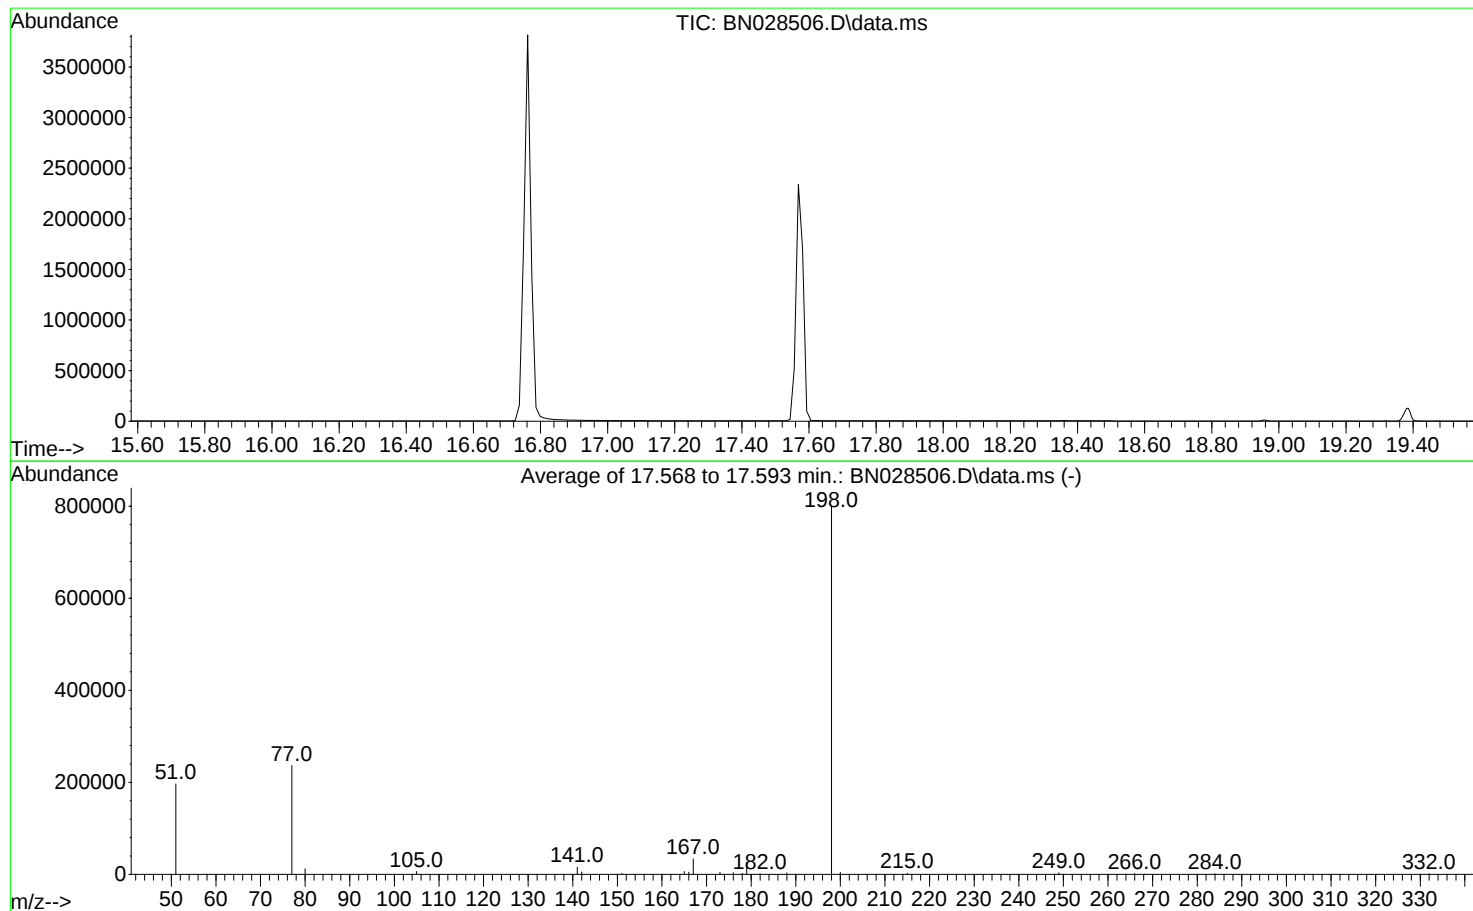

AutoFind: Scans 1768, 1769, 1770; Background Corrected with Scan 1762

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	196400	PASS
68.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
69	198	0.00	100	0.0	0	PASS
70.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
127	198	10	80	0.0	0	FAIL*
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	799351	PASS
199	198	5	9	0.0	0	FAIL*
275	198	10	60	0.0	0	FAIL*
365	198	1	100	0.0	0	FAIL*
441	198	0.01	100	0.0	0	FAIL*
442.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				
443.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				