
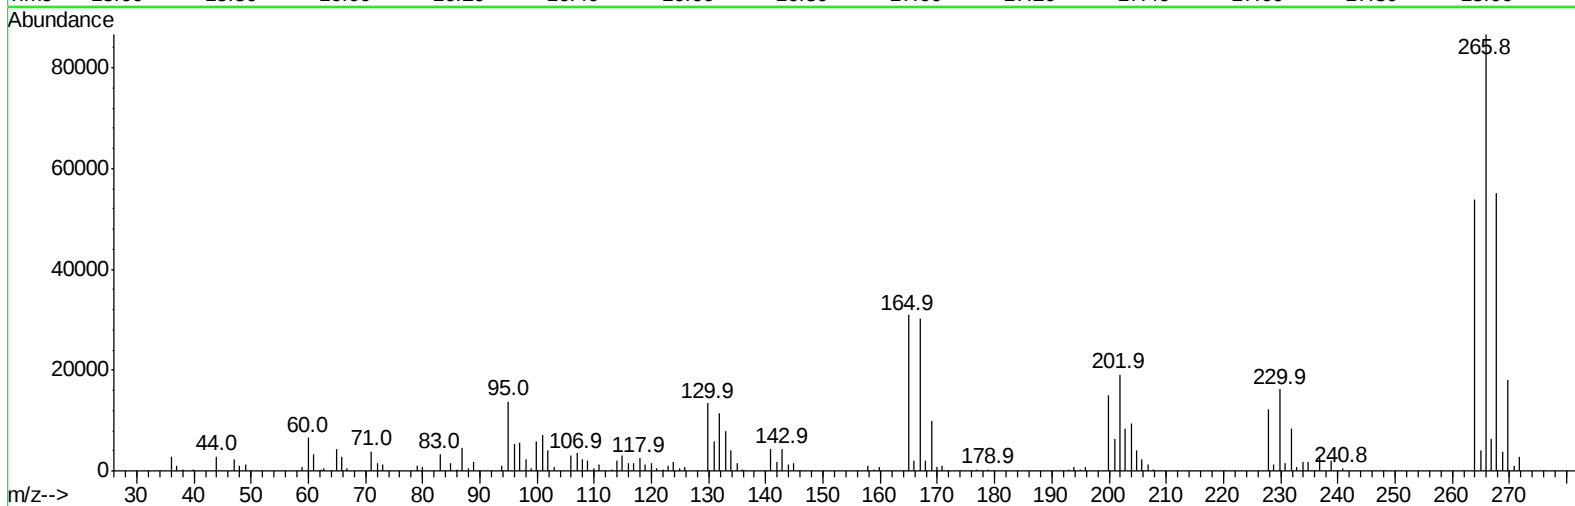


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003469.D
Acq On : 09 Nov 2018 12:41
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 04:47:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

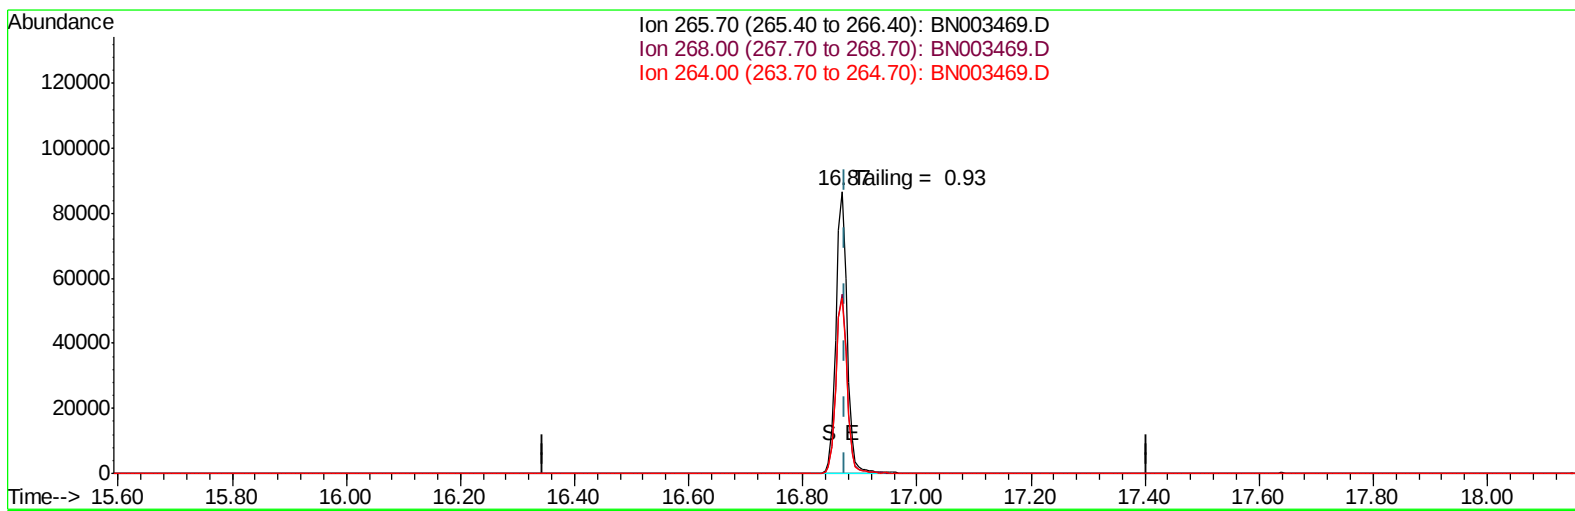

TIC: BN003469.D

(70) Pentachlorophenol (C)



16.869min (-0.006) 34436.01ng

response 116630

Ion	Exp%	Act%
265.70	100	100
268.00	65.60	63.52
264.00	62.90	62.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003469.D
Acq On : 09 Nov 2018 12:41
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 04:47:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

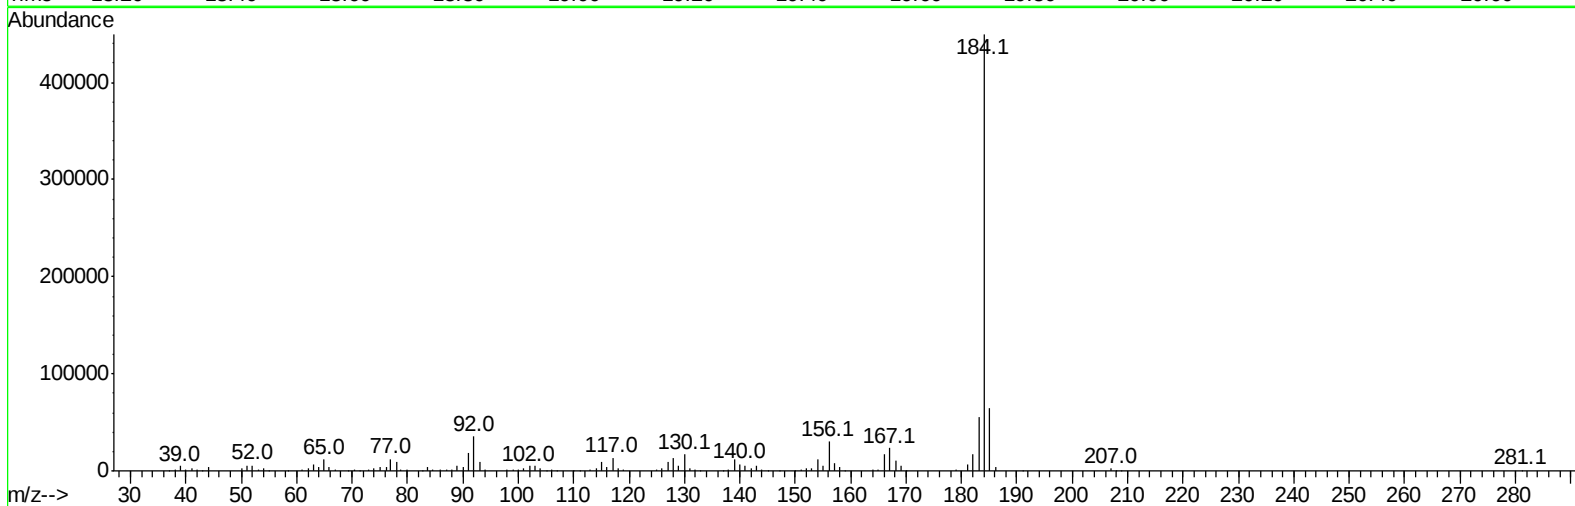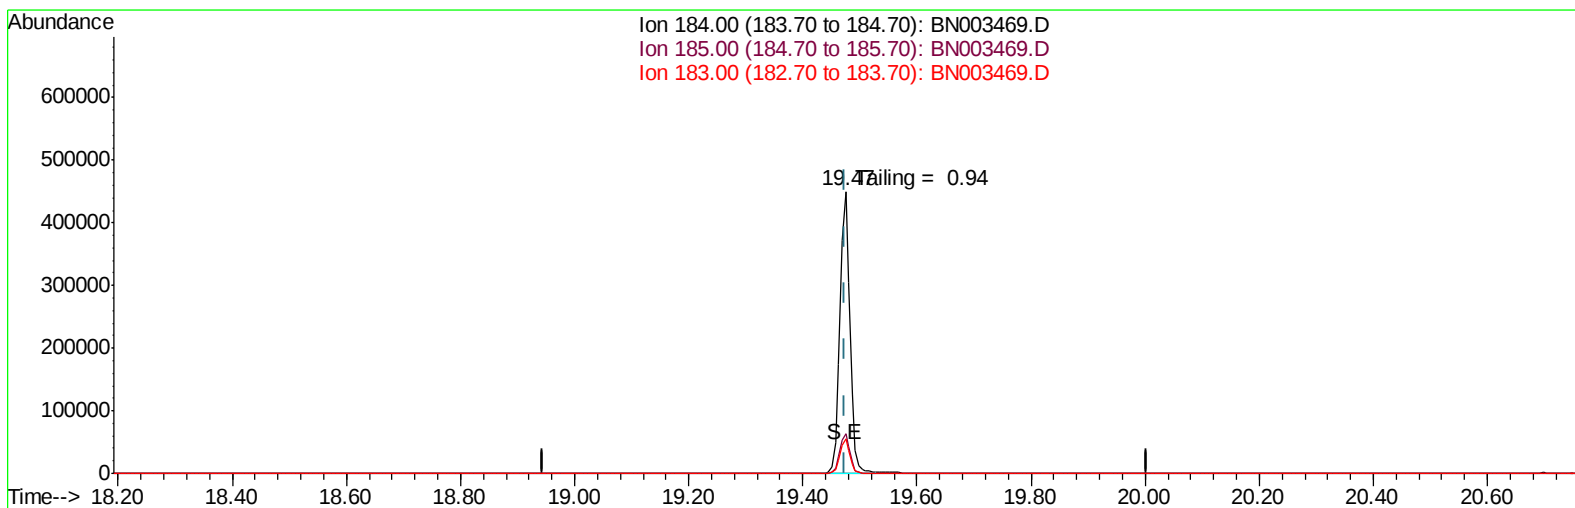

TIC: BN003469.D

(77) Benzidine

19.474min (0.000) 1696.31ng

response 555496

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.33
183.00	11.70	12.30
0.00	0.00	0.00