
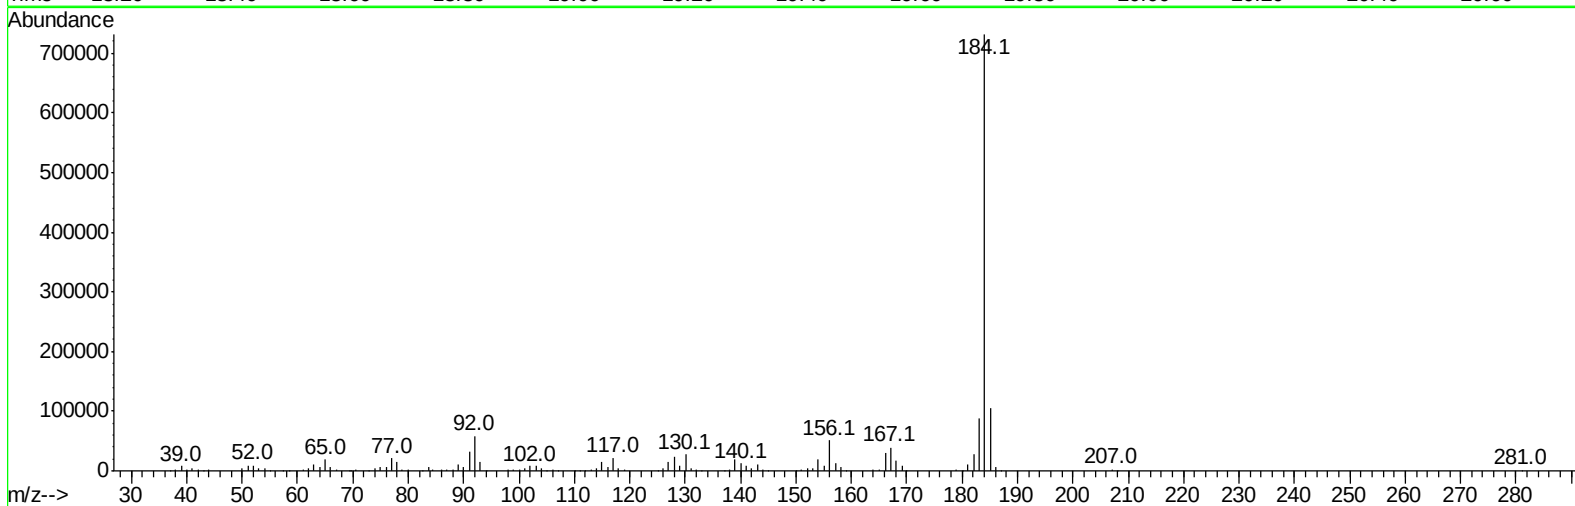


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
 Data File : BN003487.D
 Acq On : 10 Nov 2018 00:02
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 04:48:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration

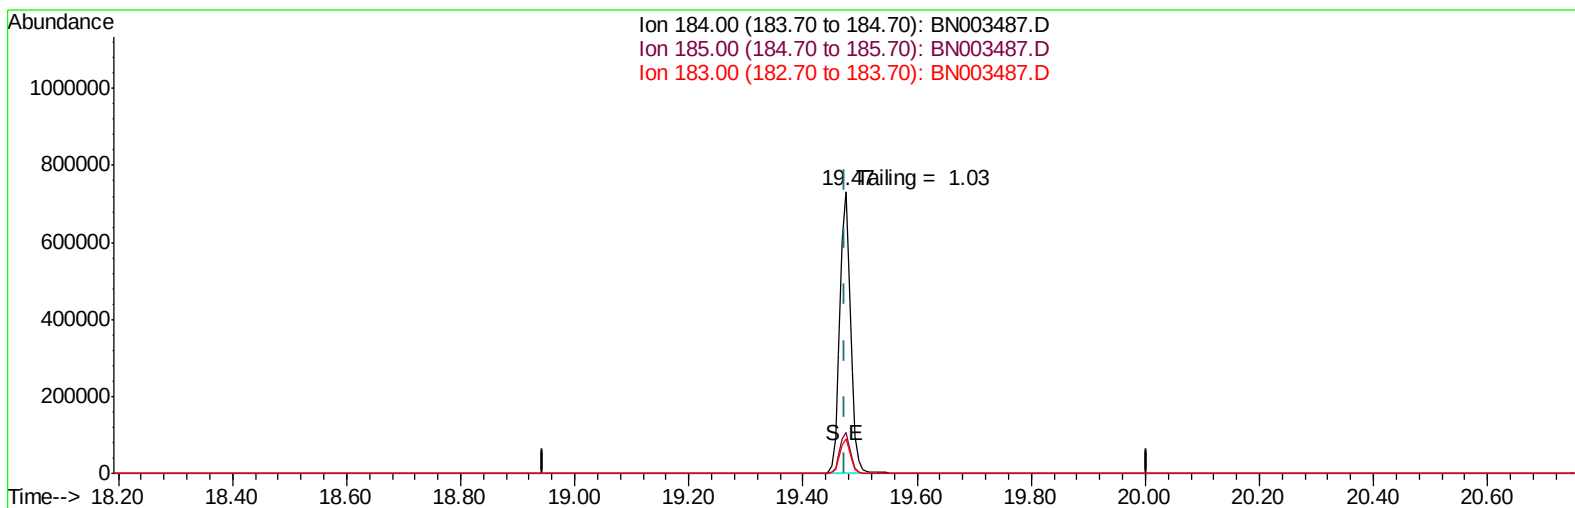

TIC: BN003487.D

(77) Benzidine



19.474min (-0.000) 0.00ng

response 969879

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.40
183.00	11.70	12.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003487.D
Acq On : 10 Nov 2018 00:02
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 04:48:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

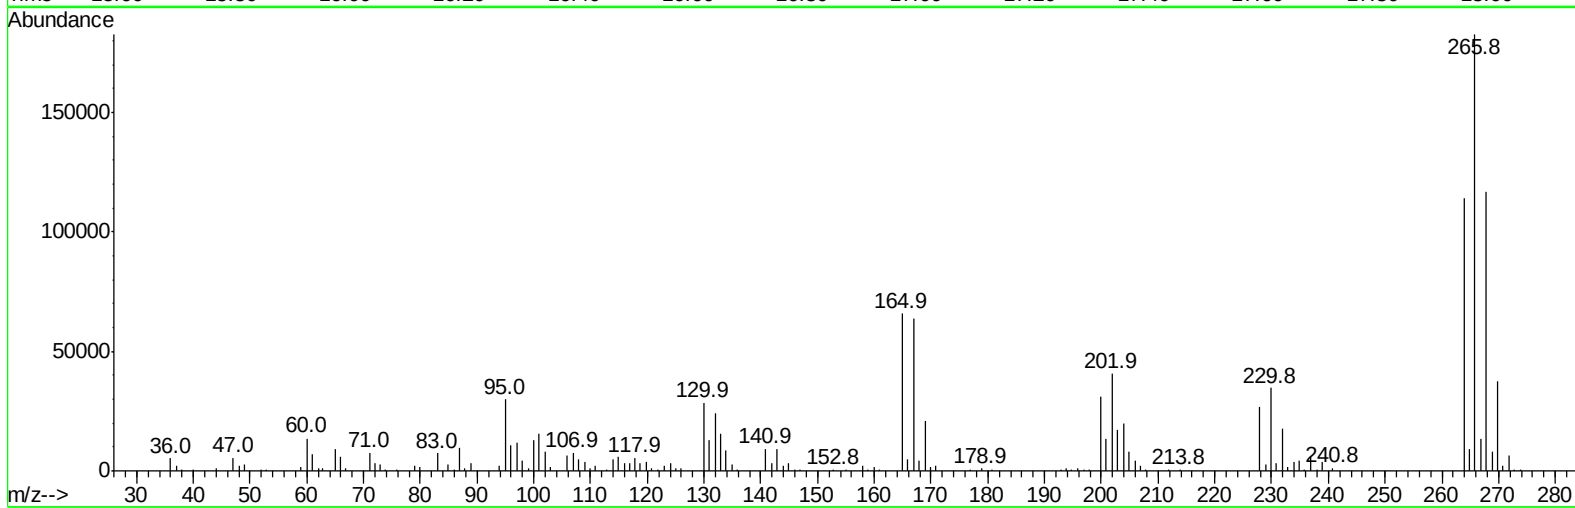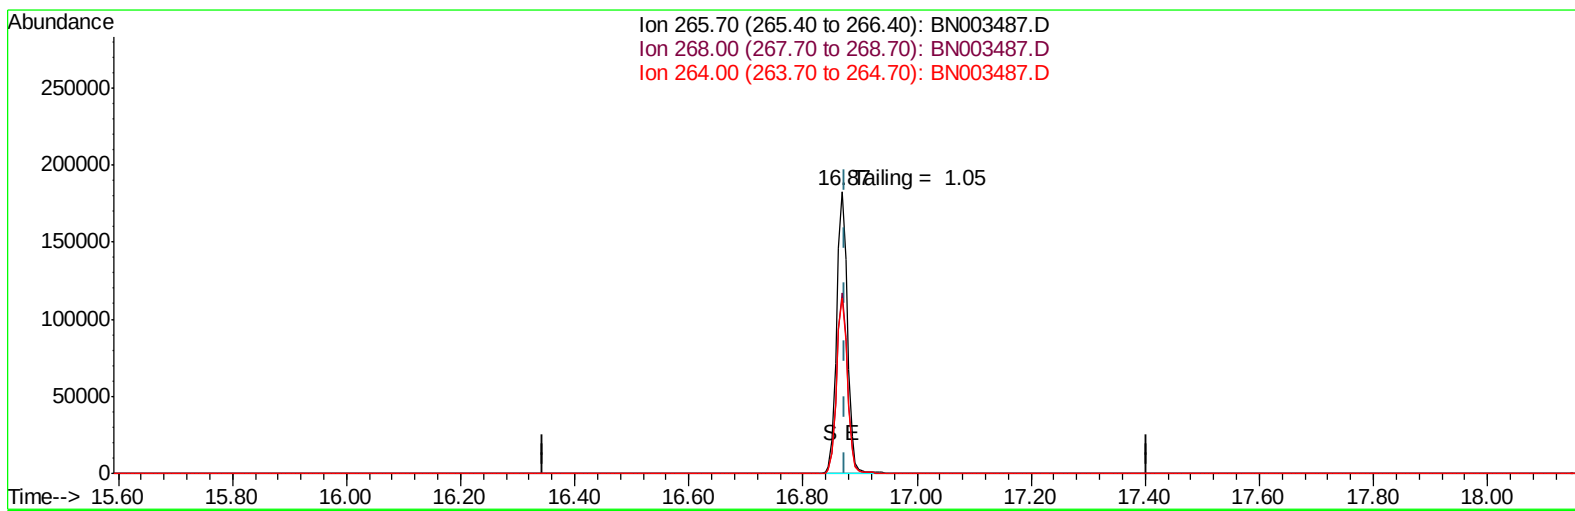

TIC: BN003487.D

(70) Pentachlorophenol (C)

16.868min (-0.006) 41922.51ng

response 238130

Ion	Exp%	Act%
265.70	100	100
268.00	65.60	63.91
264.00	62.90	62.38
0.00	0.00	0.00