

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
 Data File : BN003481.D
 Acq On : 09 Nov 2018 20:32
 Operator : MJ/SJ
 Sample : J5860-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EP2-FD-01-1118

Quant Time: Nov 12 04:01:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	96545	20.00	ng	0.00
21) Naphthalene-d8	10.65	136	412373	20.00	ng	0.00
39) Acenaphthene-d10	14.49	164	248104	20.00	ng	0.00
64) Phenanthrene-d10	17.23	188	554666	20.00	ng	0.00
76) Chrysene-d12	21.40	240	458227	20.00	ng	0.00
87) Perylene-d12	23.72	264	440922	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	784618	141.55	ng	0.00
7) Phenol-d6	7.01	99	1072123	136.02	ng	0.00
23) Nitrobenzene-d5	9.02	82	613263	85.29	ng	0.00
42) 2,4,6-Tribromophenol	15.97	330	525421	157.27	ng	0.00
45) 2-Fluorobiphenyl	13.10	172	1427718	78.06	ng	0.00
79) Terphenyl-d14	19.85	244	2081997	97.17	ng	0.00
Target Compounds						
10) Phenol	7.03	94	79847	9.600	ng	95
50) Dimethylphthalate	13.93	163	245481	12.237	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003481.D
Acq On : 09 Nov 2018 20:32
Operator : MJ/SJ
Sample : J5860-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EP2-FD-01-1118

Quant Time: Nov 12 04:01:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

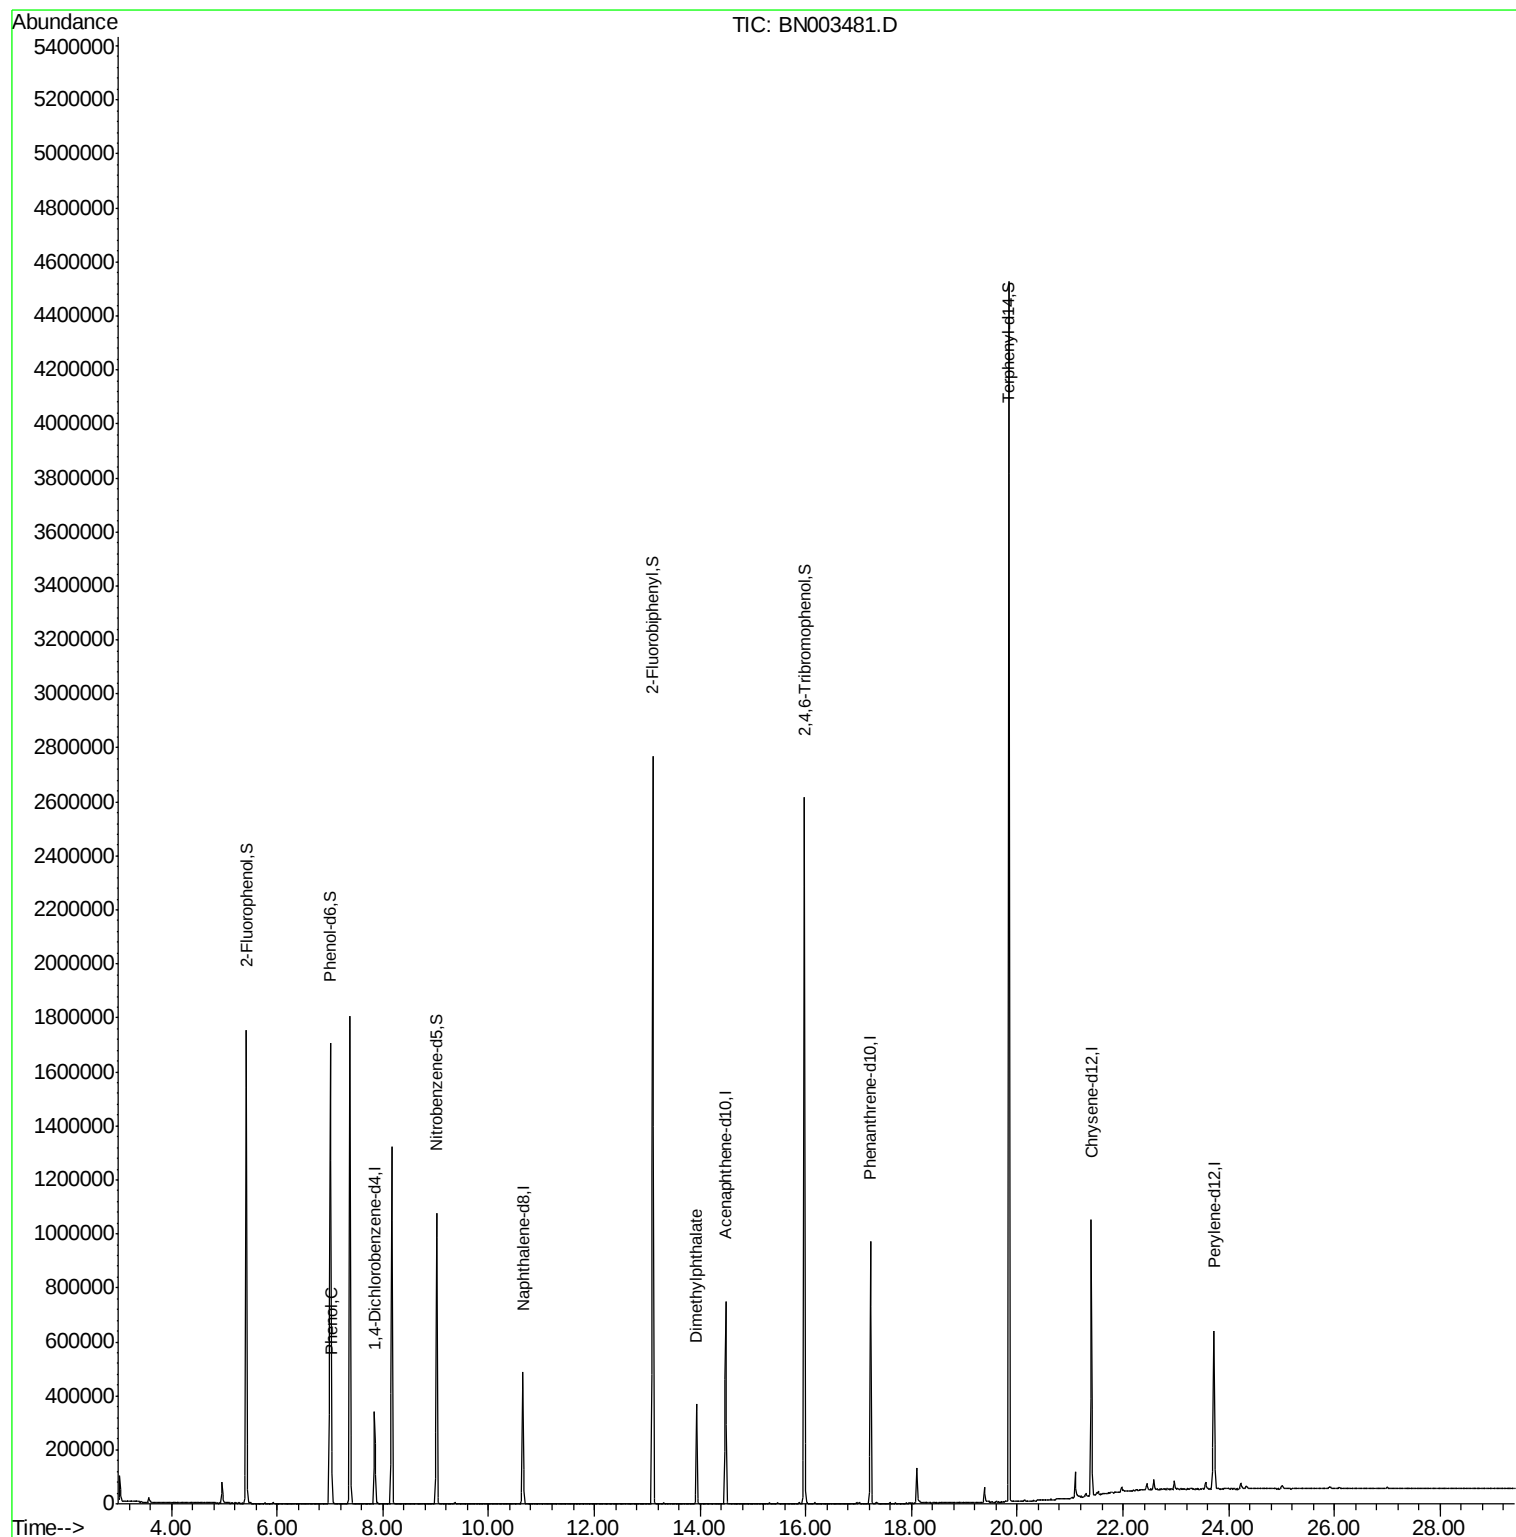

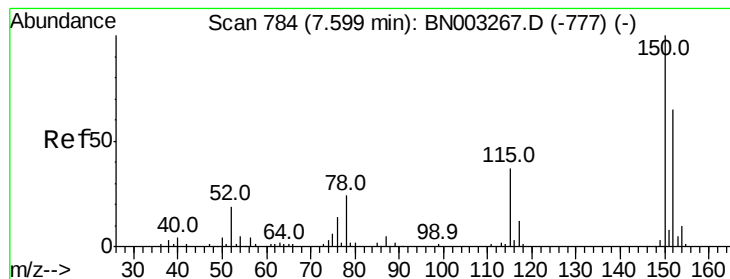


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.85 min Scan# 826
 Delta R.T. -0.01 min
 Lab File: BN003481.D
 Acq: 09 Nov 2018 20:32

Instrument :
 BNA_N
 ClientSampleId :
 EP2-FD-01-1118

Tot Ion:152 Resp: 96545
 Ion Ratio Lower Upper
 152 100
 150 157.8 123.8 185.8
 115 59.1 45.9 68.9

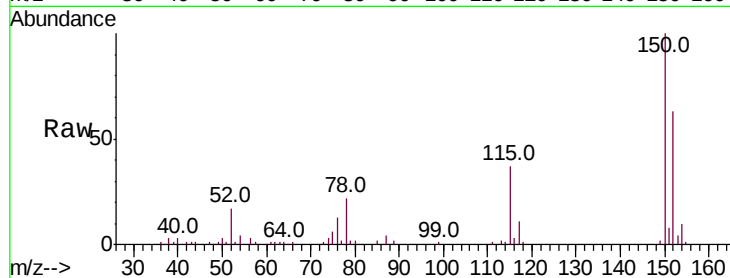


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

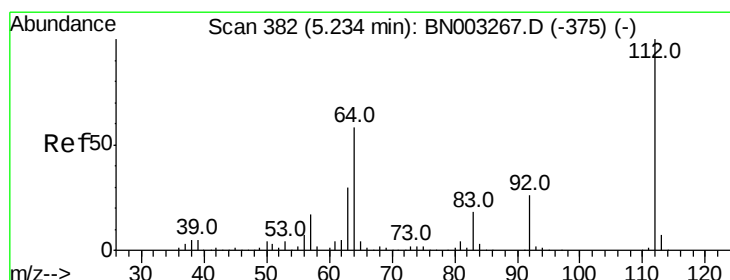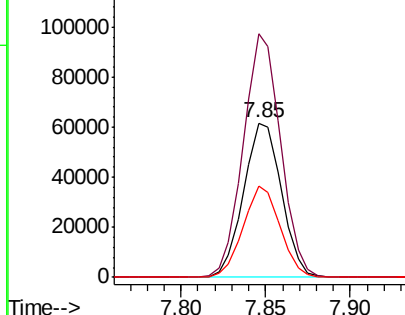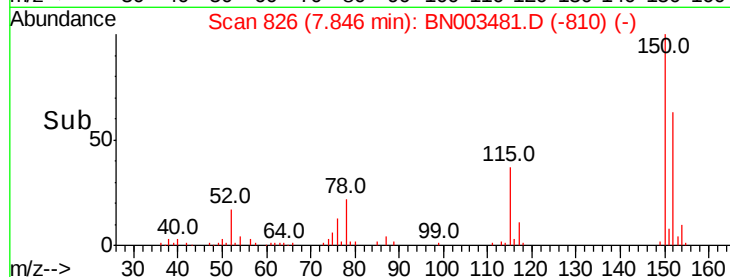



#5


2-Fluorophenol
 Concen: 141.551 ng
 RT: 5.42 min Scan# 413
 Delta R.T. 0.01 min
 Lab File: BN003481.D
 Acq: 09 Nov 2018 20:32

Tgt Ion:112 Resp: 784618
 Ion Ratio Lower Upper
 112 100
 64 51.8 46.6 69.8
 63 25.8 23.8 35.8

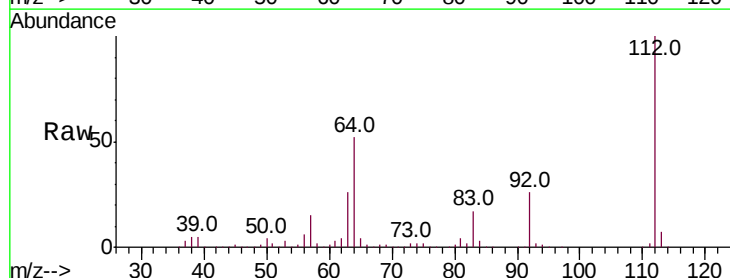

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BNC
 Ion 63.00 (62.70 to 63.70): BNC

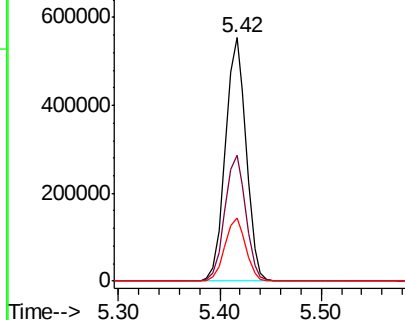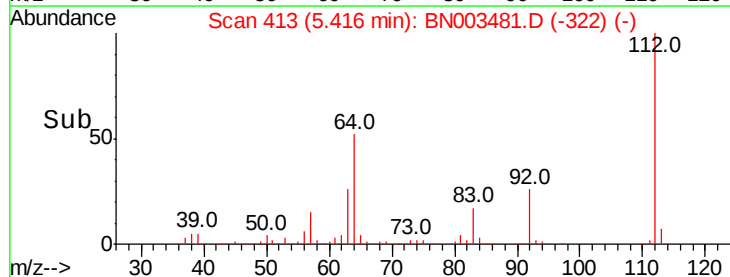

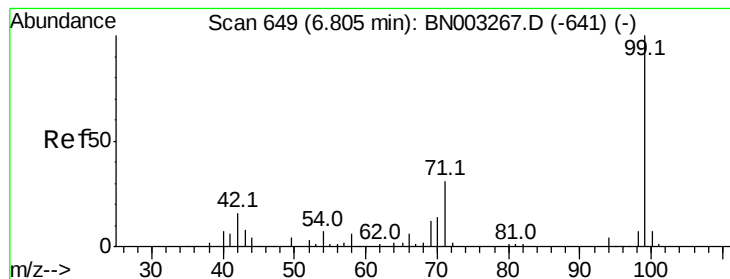

#7

Phenol-d6

Concen: 136.024 ng

RT: 7.01 min Scan# 684

Delta R.T. 0.00 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32

Instrument :

BNA_N

ClientSampleId :

EP2-FD-01-1118


Tot Ion: 99 Resp: 1072123

Ion Ratio Lower Upper




99 100

42 14.5 13.0 19.6

71 30.0 24.5 36.7

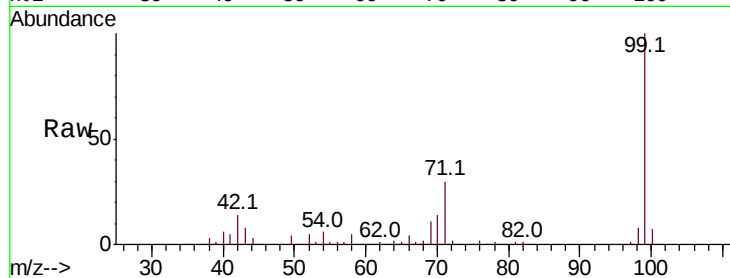

Abundance Ion 99.00 (98.70 to 99.70): BNC
Ion 42.00 (41.70 to 42.70): BNC
Ion 71.00 (70.70 to 71.70): BNC

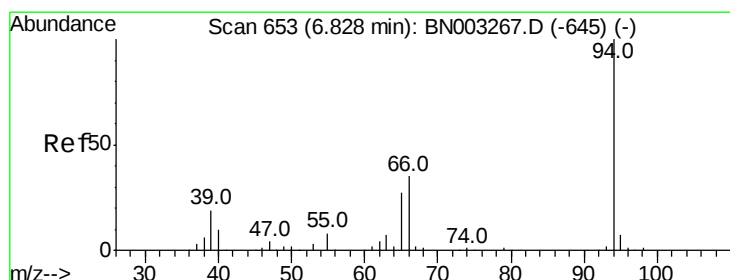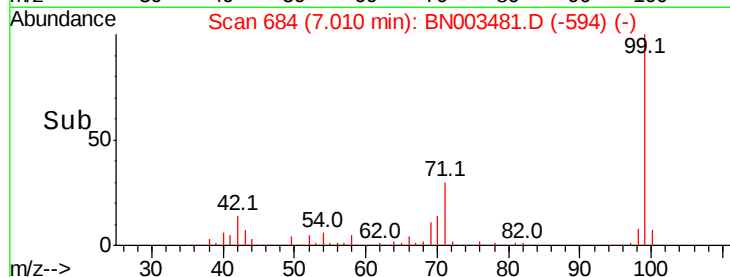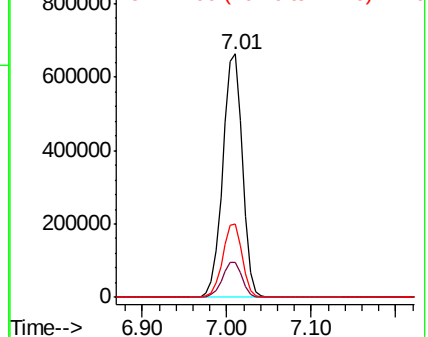

#10

Phenol

Concen: 9.600 ng

RT: 7.03 min Scan# 688

Delta R.T. 0.00 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32


Tgt Ion: 94 Resp: 79847

Ion Ratio Lower Upper



94 100


65 25.1 7.7 47.7

66 32.9 15.8 55.8

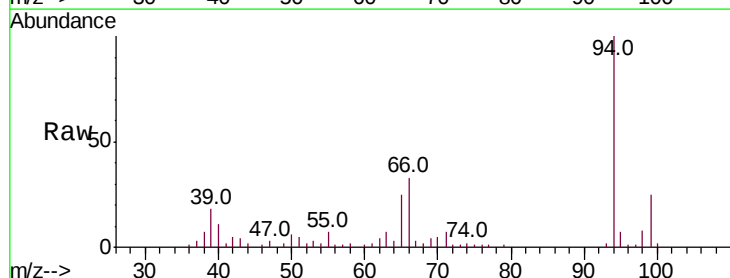

Abundance Ion 94.00 (93.70 to 94.70): BNC
Ion 65.00 (64.70 to 65.70): BNC
Ion 66.00 (65.70 to 66.70): BNC

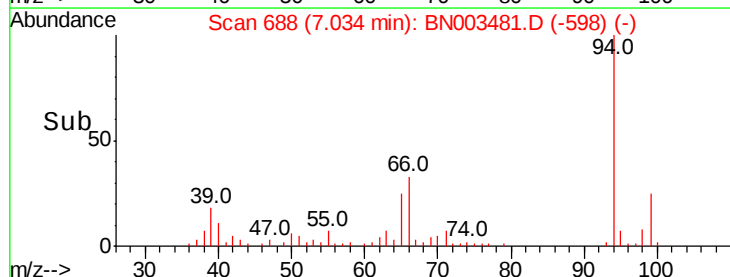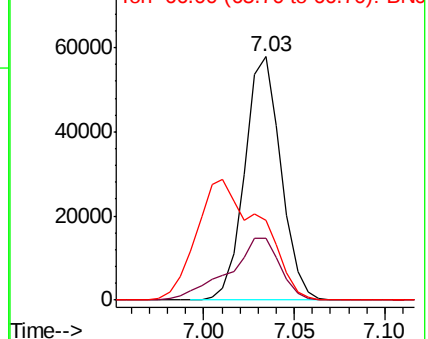

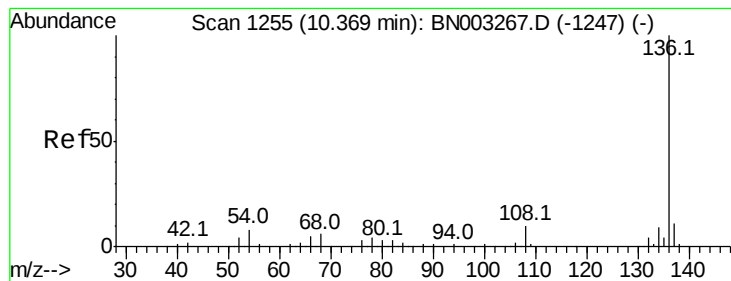

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.65 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32

Instrument :

BNA_N

ClientSampleId :

EP2-FD-01-1118

Tot Ion:136 Resp: 412373


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 7.2 6.6 10.0

68 6.2 4.6 7.0



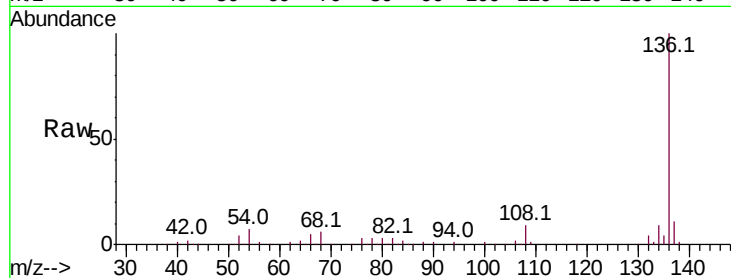


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

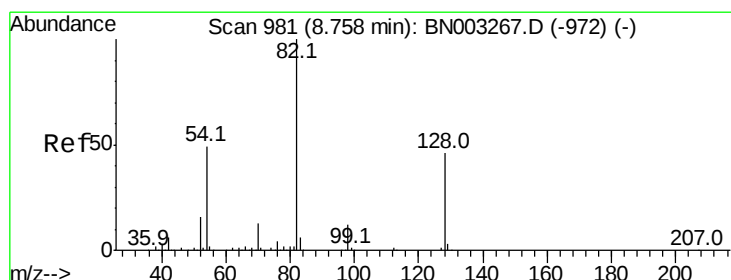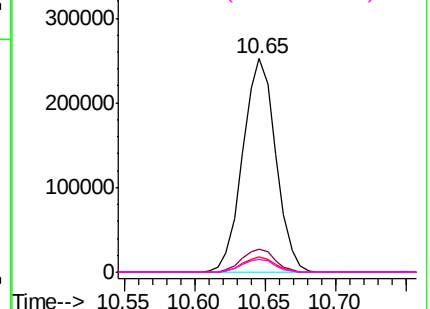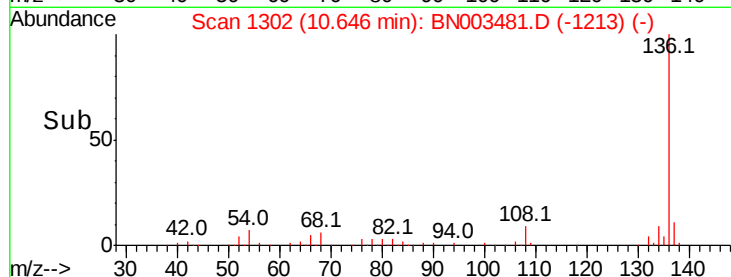

#23

Nitrobenzene-d5

Concen: 85.287 ng

RT: 9.02 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32


Tgt Ion: 82 Resp: 613263

Ion Ratio Lower Upper

82 100

128 49.9 37.1 55.7



54 45.4 39.4 59.2

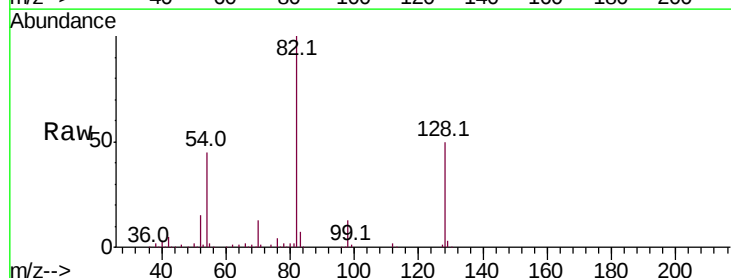


Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

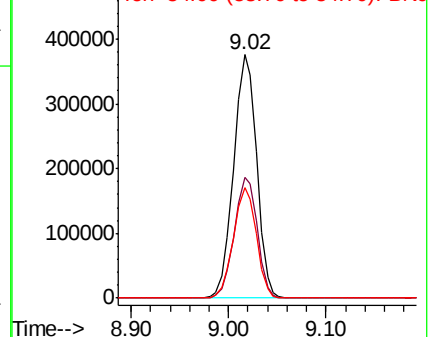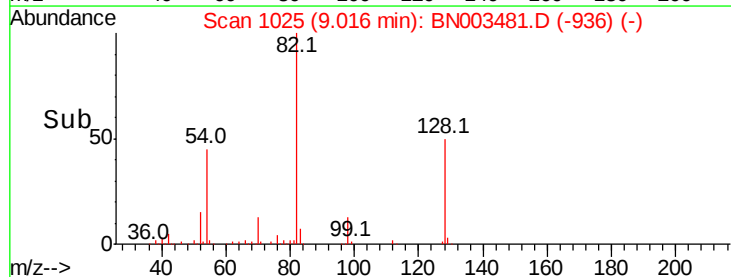

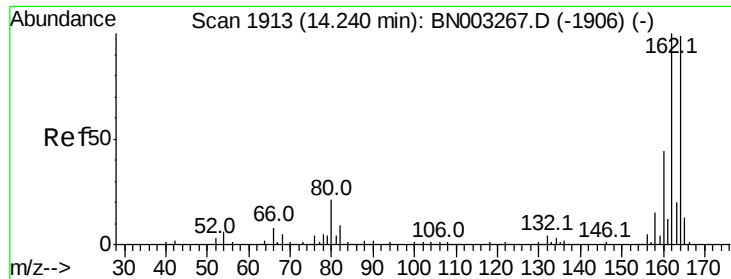

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.49 min Scan# 1955

Delta R.T. 0.00 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32

Instrument :

BNA_N

ClientSampleId :

EP2-FD-01-1118


Tot Ion:164 Resp: 248104

Ion Ratio Lower Upper

164 100

162 102.1 80.8 121.2




160 45.7 35.5 53.3

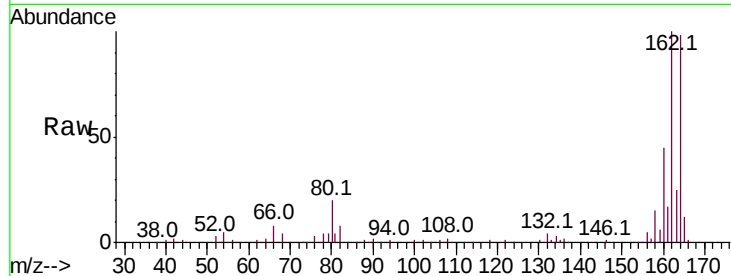

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

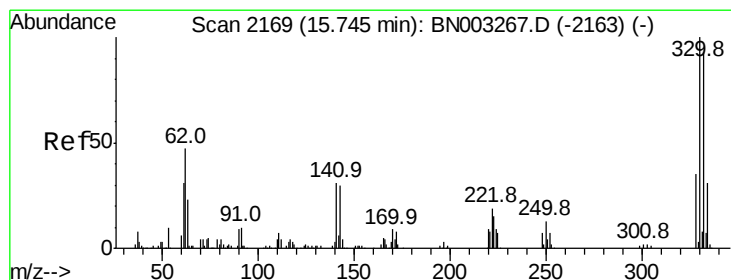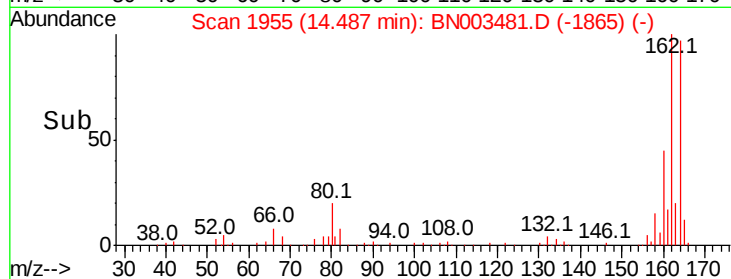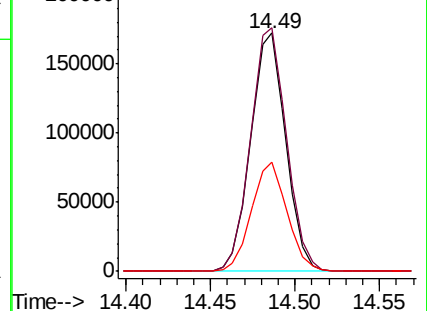

#42

2,4,6-Tribromophenol

Concen: 157.274 ng

RT: 15.97 min Scan# 2208

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32


Tgt Ion:330 Resp: 525421

Ion Ratio Lower Upper

330 100

332 96.4 76.6 114.8



141 27.1 24.5 36.7

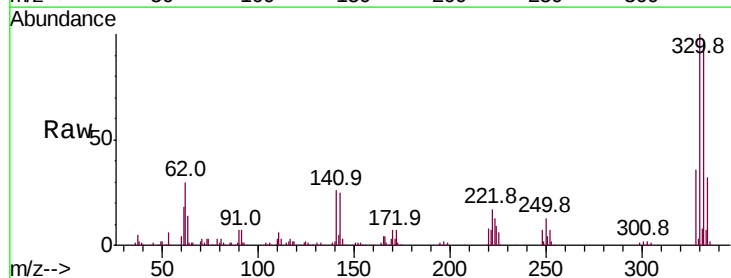


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

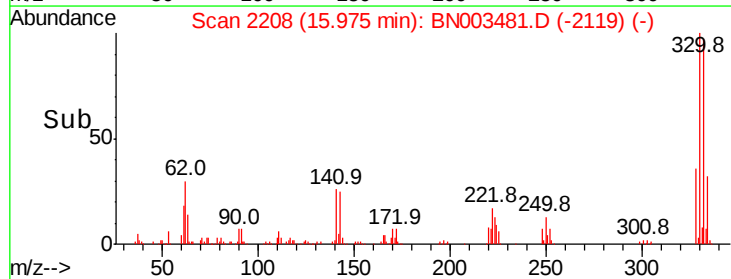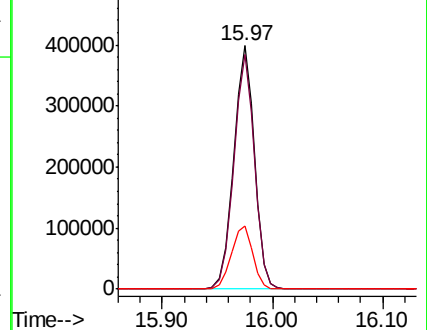




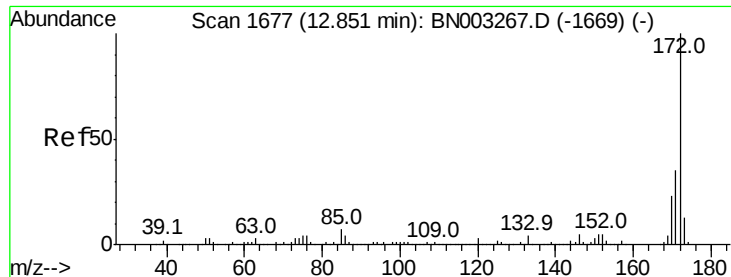


#45
 2-Fluorobiphenyl
 Concen: 78.056 ng
 RT: 13.10 min Scan# 1720
 Delta R.T. -0.01 min
 Lab File: BN003481.D
 Acq: 09 Nov 2018 20:32

Instrument :
 BNA_N
 ClientSampleId :
 EP2-FD-01-1118

Tot Ion:172 Resp: 1427718




Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.2	42.4
170	23.6	18.4	27.6

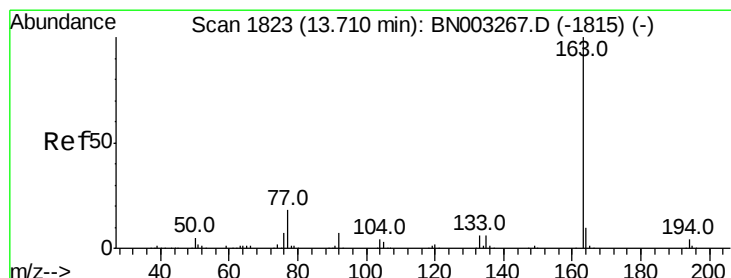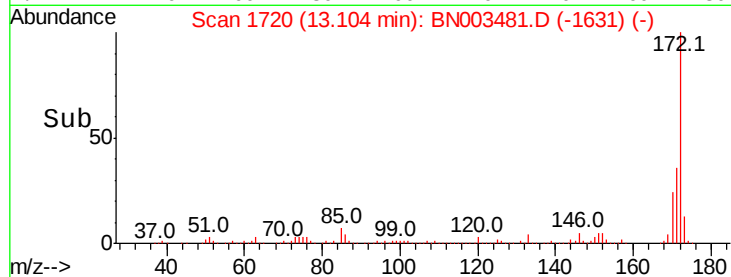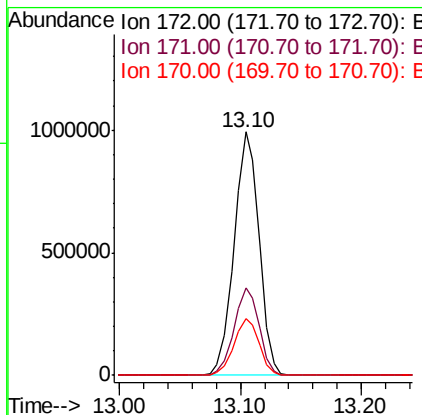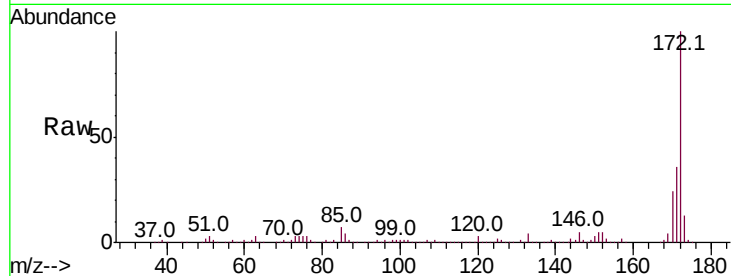


#50
 Dimethylphthalate
 Concen: 12.237 ng
 RT: 13.93 min Scan# 1861
 Delta R.T. -0.02 min
 Lab File: BN003481.D
 Acq: 09 Nov 2018 20:32

Tgt Ion:163 Resp: 245481

Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.2
164	10.4	7.9	11.9

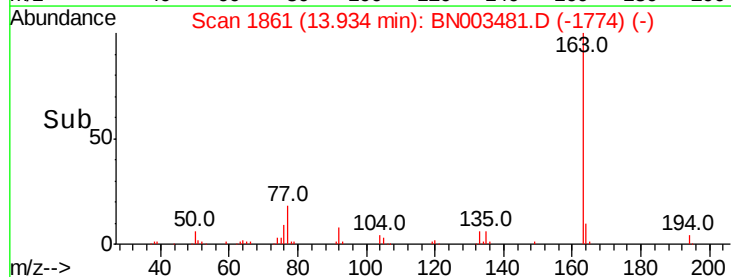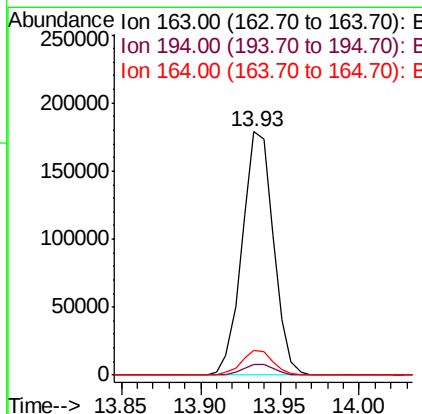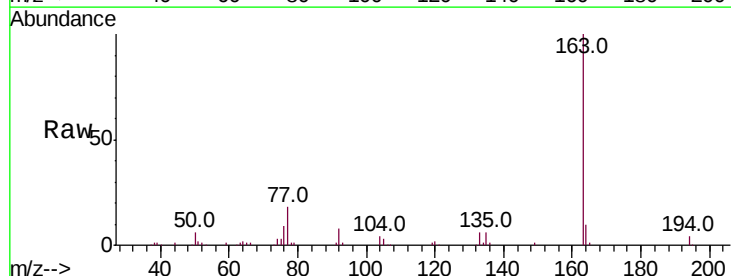

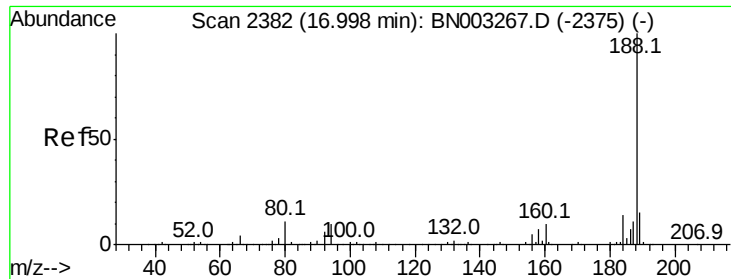

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.23 min Scan# 2421

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32

Instrument :

BNA_N

ClientSampleId :

EP2-FD-01-1118


Tot Ion:188 Resp: 554666

Ion Ratio Lower Upper

188 100

94 9.6 8.1 12.1




80 9.9 8.6 13.0

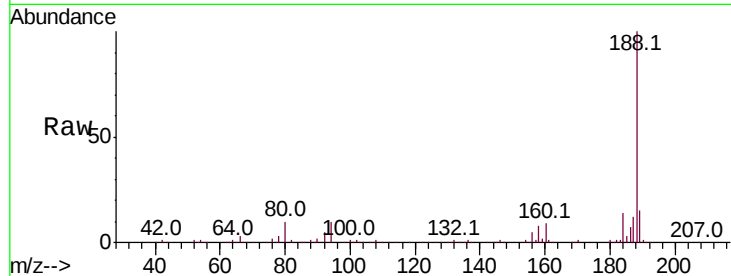

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

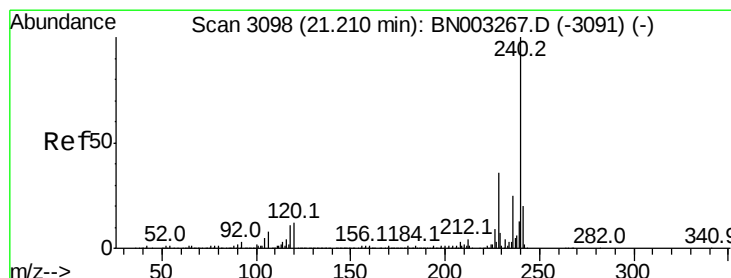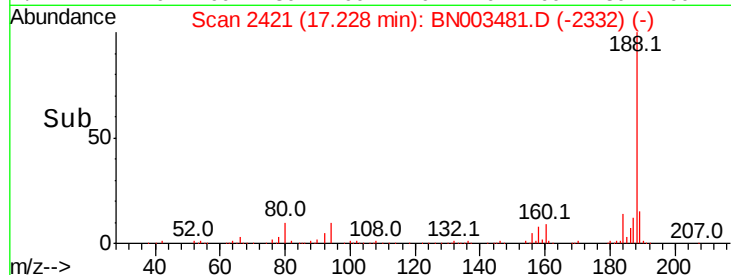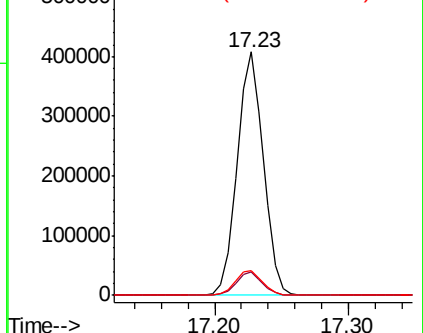

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.40 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32


Tgt Ion:240 Resp: 458227

Ion Ratio Lower Upper

240 100

120 11.4 9.4 14.0



236 25.8 20.3 30.5

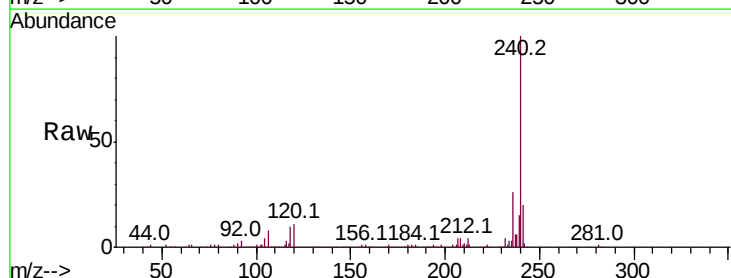


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

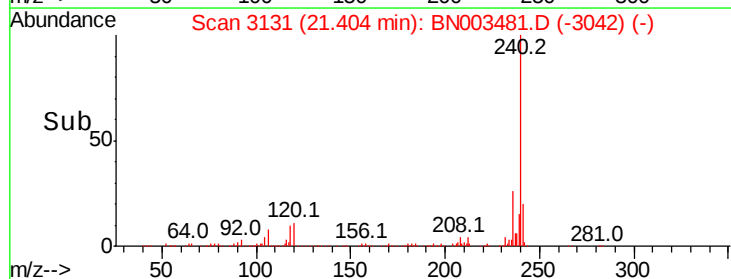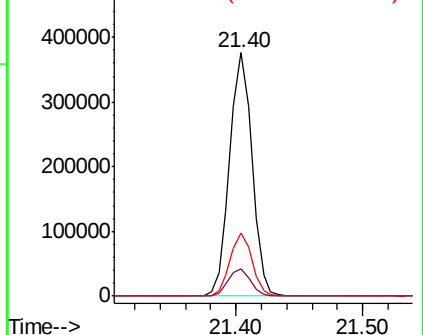

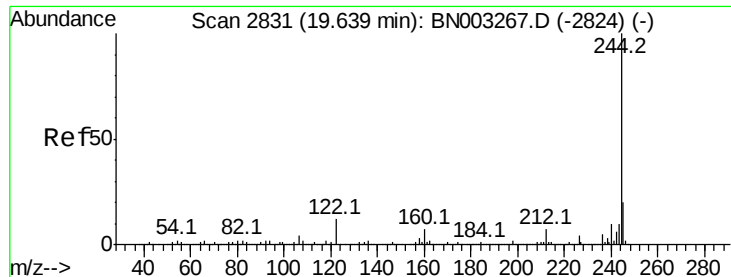

#79

Terphenyl-d14

Concen: 97.167 ng

RT: 19.85 min Scan# 2866

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32

Instrument :

BNA_N

ClientSampleId :

EP2-FD-01-1118


Tot Ion:244 Resp: 2081997

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 10.9 9.4 14.2

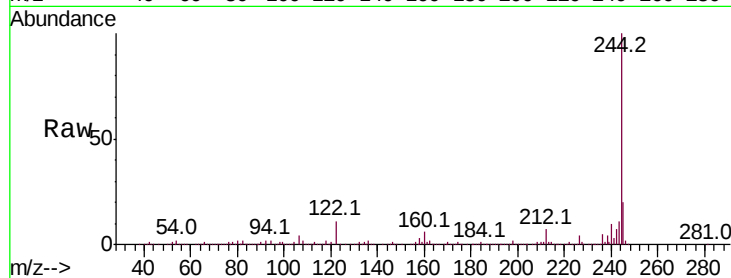

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

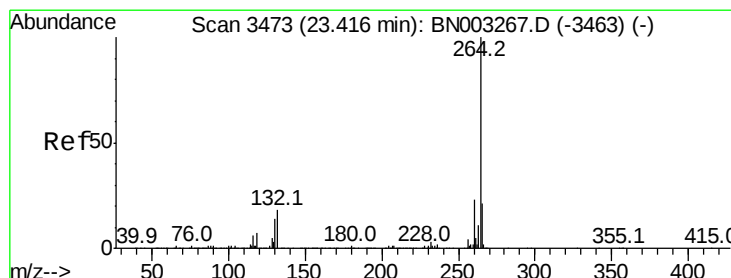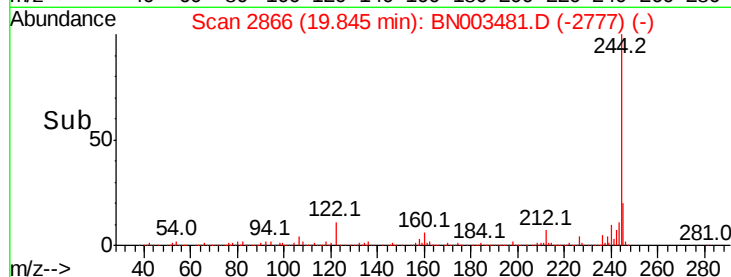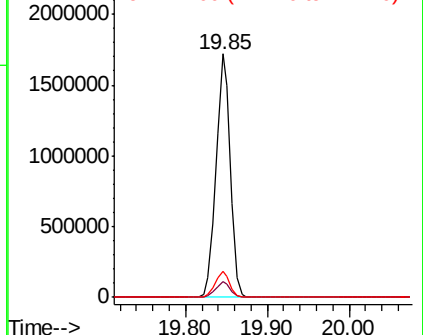

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.72 min Scan# 3525

Delta R.T. -0.01 min

Lab File: BN003481.D

Acq: 09 Nov 2018 20:32


Tgt Ion:264 Resp: 440922

Ion Ratio Lower Upper

264 100

260 24.1 18.5 27.7

265 21.7 16.6 25.0

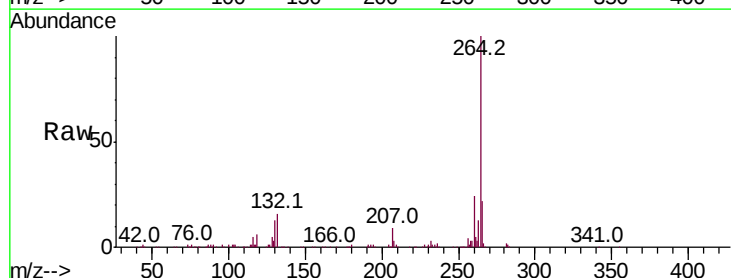

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

