

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
 Data File : BN003492.D
 Acq On : 10 Nov 2018 02:59
 Operator : MJ/SJ
 Sample : J5881-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 110718-TIPC-F-D-B

Quant Time: Nov 12 04:31:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	87953	20.00	ng	0.00
21) Naphthalene-d8	10.65	136	394294	20.00	ng	0.00
39) Acenaphthene-d10	14.48	164	238812	20.00	ng	0.00
64) Phenanthrene-d10	17.23	188	519775	20.00	ng	0.00
76) Chrysene-d12	21.40	240	416579	20.00	ng	0.00
87) Perylene-d12	23.72	264	414428	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	203936	40.39	ng	0.00
7) Phenol-d6	7.00	99	161444	22.48	ng	-0.01
23) Nitrobenzene-d5	9.02	82	620763	90.29	ng	0.00
42) 2,4,6-Tribromophenol	15.97	330	343083	106.69	ng	0.00
45) 2-Fluorobiphenyl	13.10	172	1763880	100.19	ng	0.00
79) Terphenyl-d14	19.85	244	1953344	100.28	ng	0.00
Target Compounds						
10) Phenol	7.03	94	16924	2.233	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003492.D
Acq On : 10 Nov 2018 02:59
Operator : MJ/SJ
Sample : J5881-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-B

Quant Time: Nov 12 04:31:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

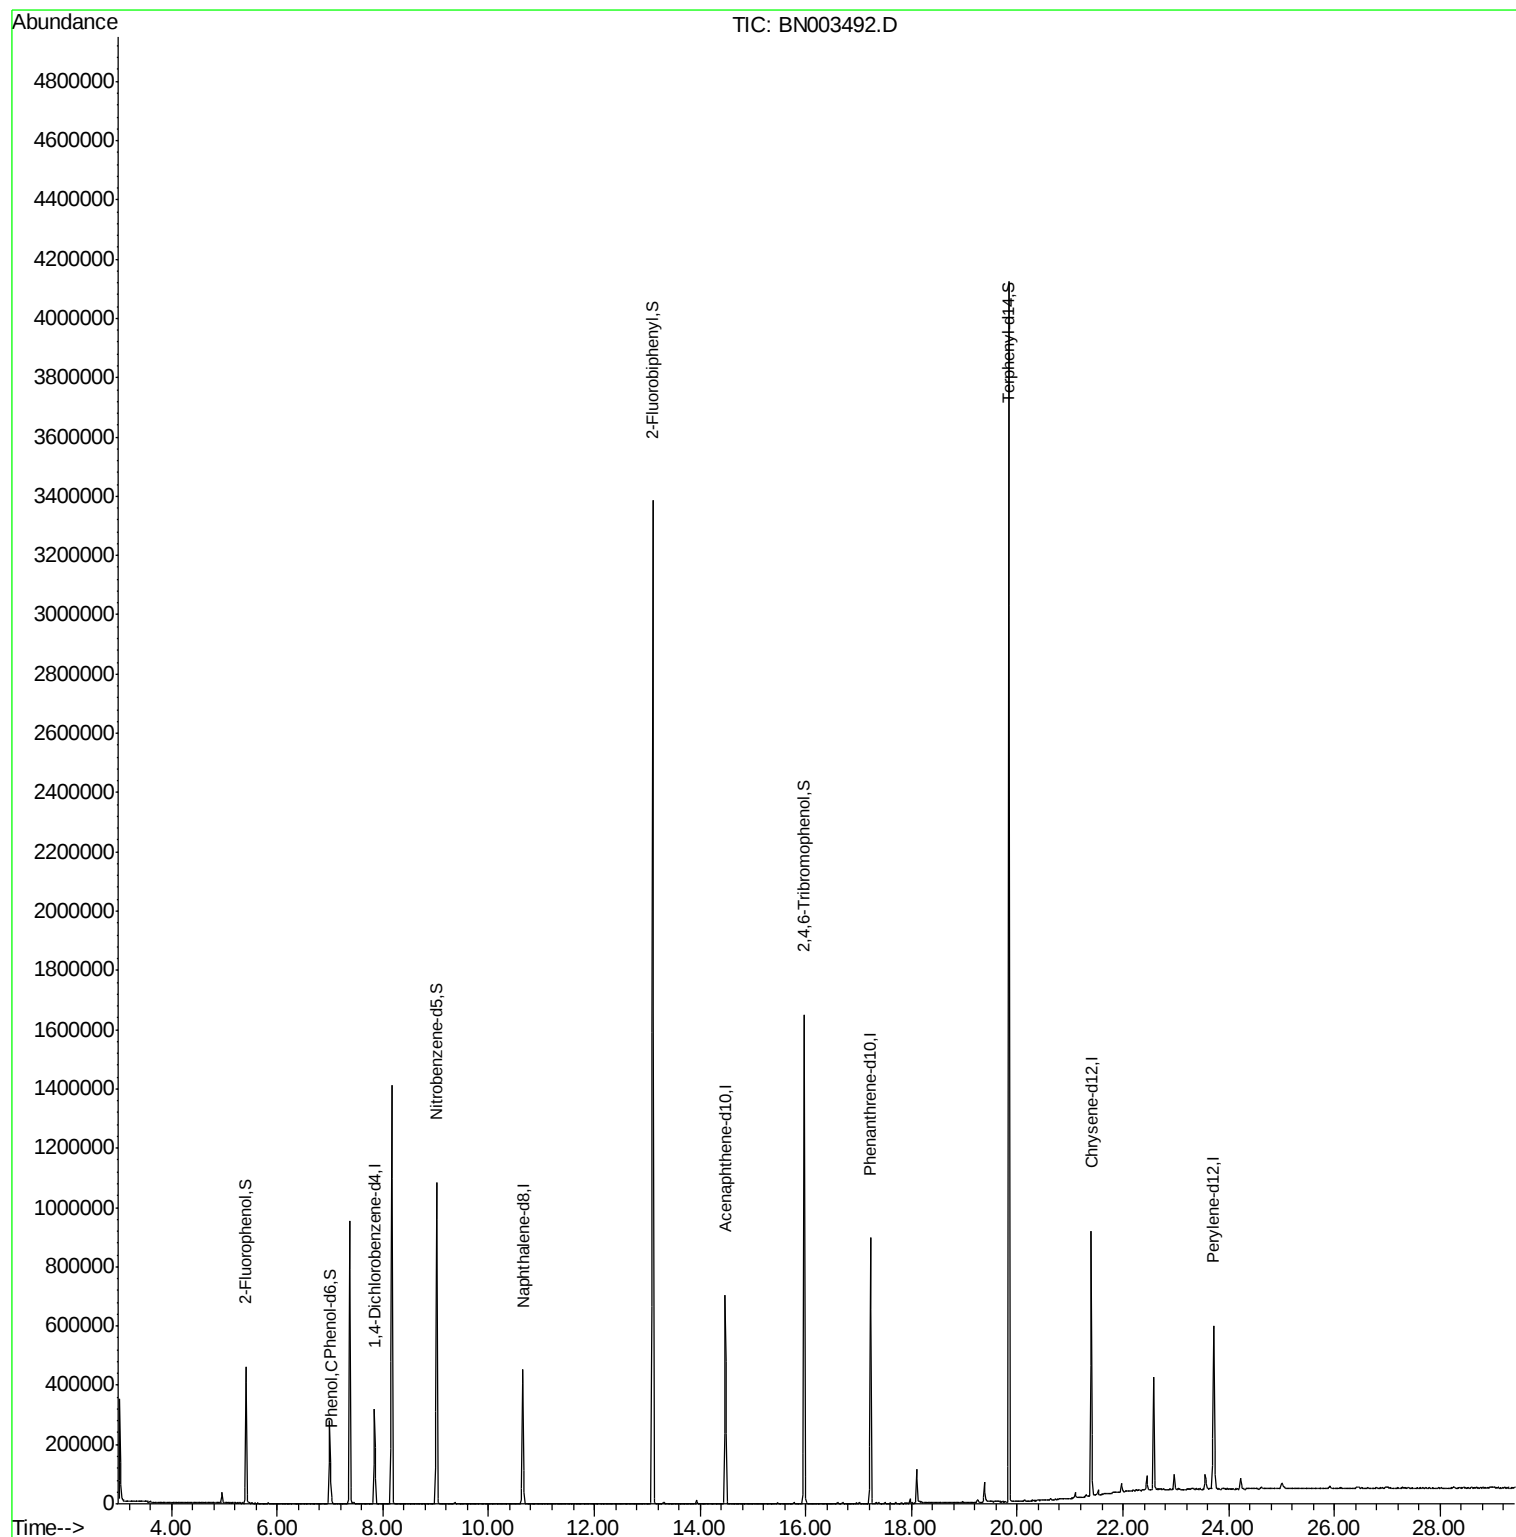

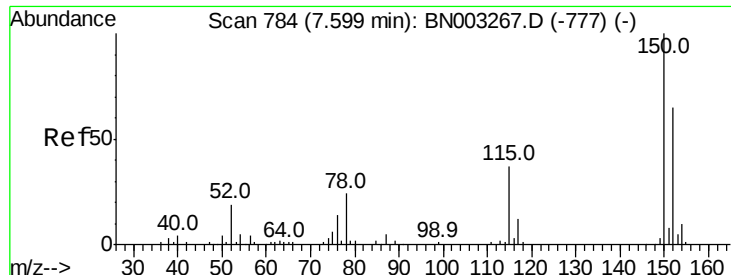


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.85 min Scan# 826
 Delta R.T. -0.01 min
 Lab File: BN003492.D
 Acq: 10 Nov 2018 02:59

Instrument :
 BNA_N
 ClientSampleId :
 110718-TIPC-F-D-B

Tot Ion:152 Resp: 87953
 Ion Ratio Lower Upper
 152 100
 150 155.5 123.8 185.8
 115 58.2 45.9 68.9

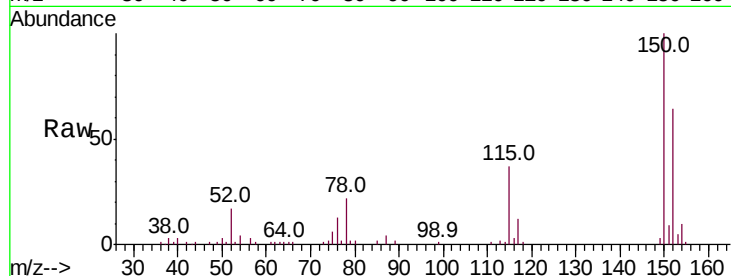


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

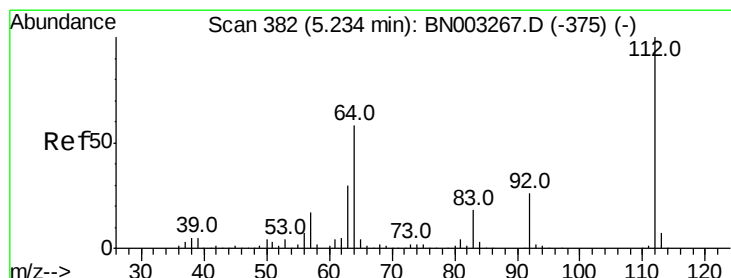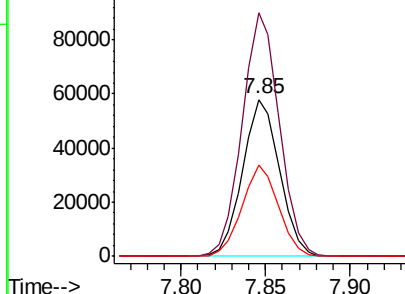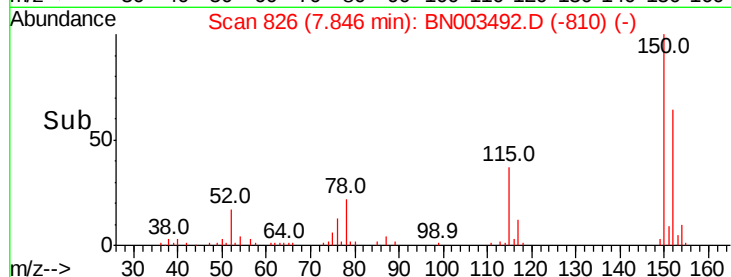



#5


2-Fluorophenol
 Concen: 40.386 ng
 RT: 5.41 min Scan# 412
 Delta R.T. 0.00 min
 Lab File: BN003492.D
 Acq: 10 Nov 2018 02:59

Tgt Ion:112 Resp: 203936
 Ion Ratio Lower Upper
 112 100
 64 53.4 46.6 69.8
 63 26.4 23.8 35.8

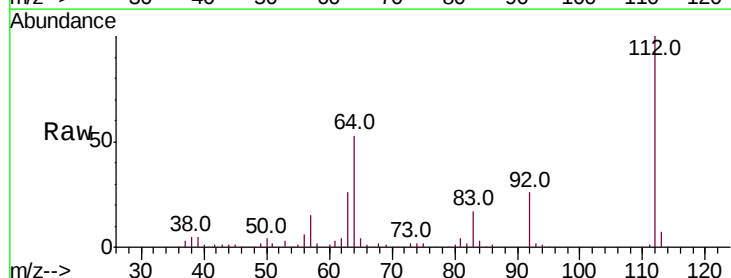

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BNC
 Ion 63.00 (62.70 to 63.70): BNC

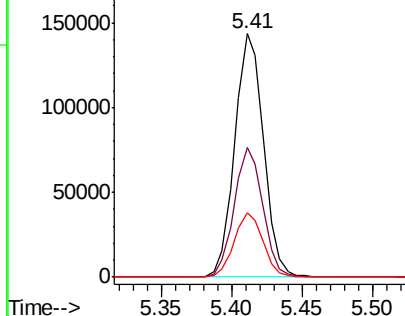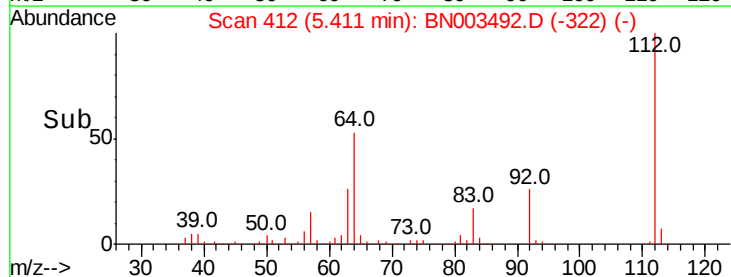

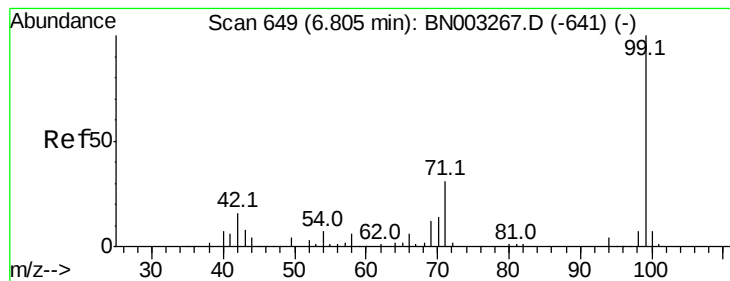

#7

Phenol-d6

Concen: 22.484 ng

RT: 7.00 min Scan# 682

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-B


Tot Ion: 99 Resp: 161444

Ion Ratio Lower Upper




99 100

42 14.7 13.0 19.6

71 29.7 24.5 36.7

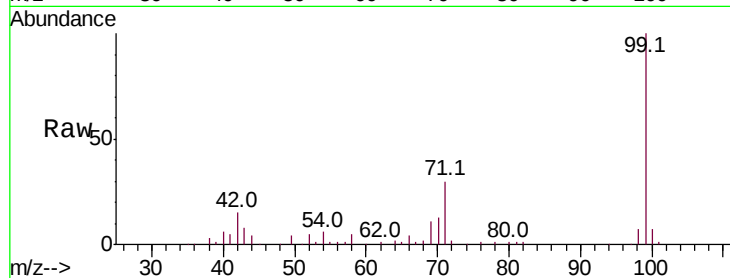

Abundance Ion 99.00 (98.70 to 99.70): BN0
Ion 42.00 (41.70 to 42.70): BN0
Ion 71.00 (70.70 to 71.70): BN0

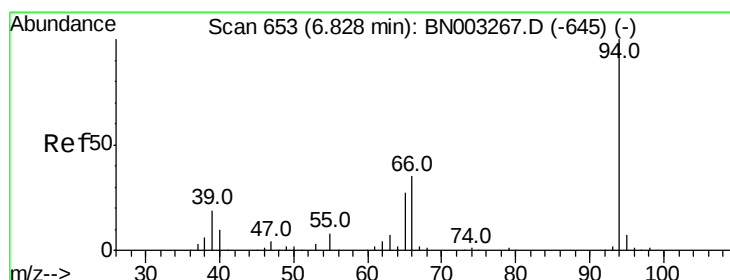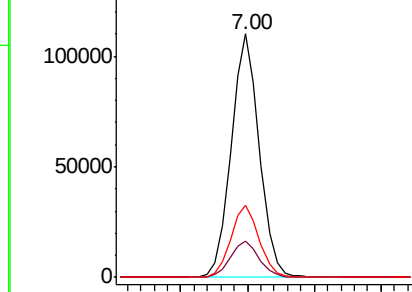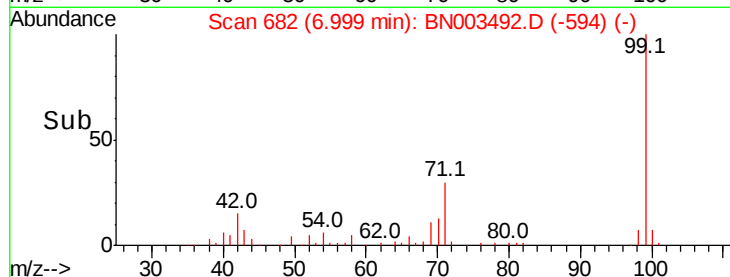

#10

Phenol

Concen: 2.233 ng

RT: 7.03 min Scan# 687

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59


Tgt Ion: 94 Resp: 16924

Ion Ratio Lower Upper



94 100


65 26.6 7.7 47.7

66 33.7 15.8 55.8

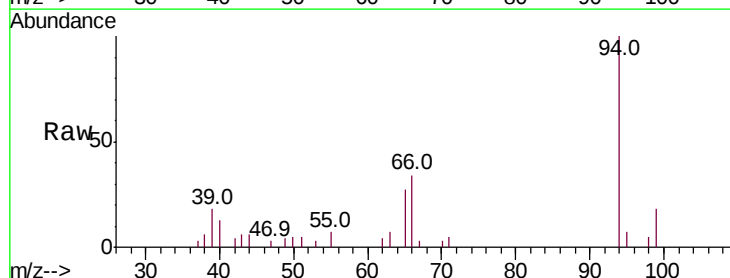

Abundance Ion 94.00 (93.70 to 94.70): BN0
Ion 65.00 (64.70 to 65.70): BN0
Ion 66.00 (65.70 to 66.70): BN0

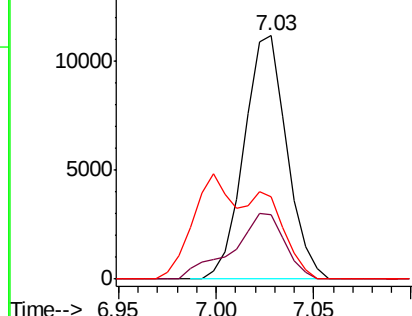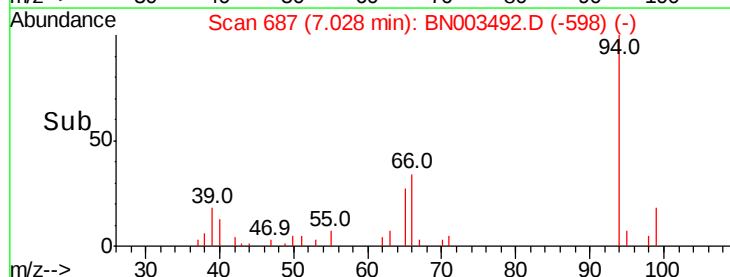


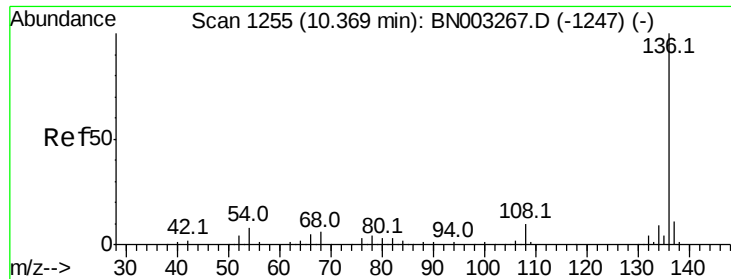




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.65 min Scan# 1302
Delta R.T. -0.01 min
Lab File: BN003492.D
Acq: 10 Nov 2018 02:59

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-B

Tot Ion:	136	Resp:	394294
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	7.1	6.6	10.0
68	6.0	4.6	7.0

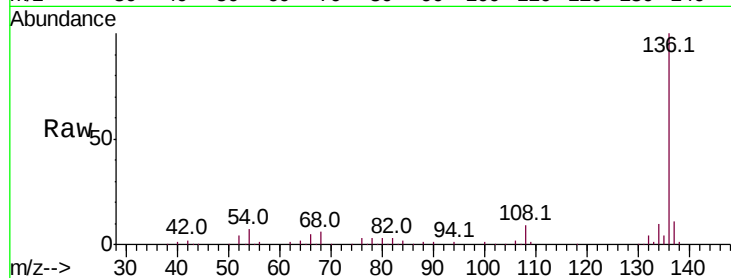


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BNC
Ion 68.00 (67.70 to 68.70): BNC

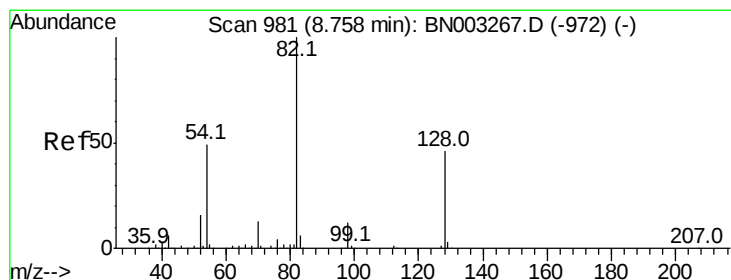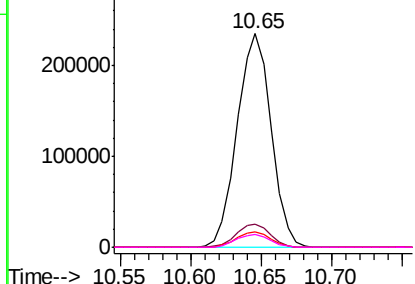
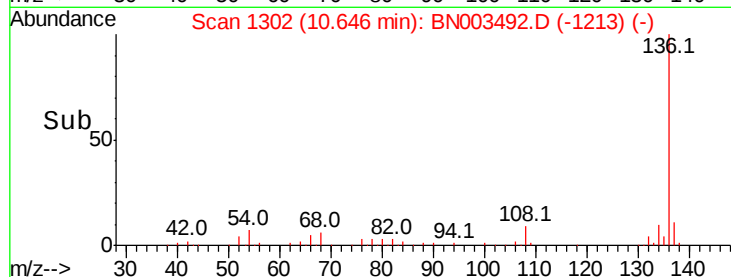



#23
Nitrobenzene-d5
Concen: 90.289 ng
RT: 9.02 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BN003492.D
Acq: 10 Nov 2018 02:59

Tgt Ion:	82	Resp:	620763
Ion	Ratio	Lower	Upper
82	100		
128	50.3	37.1	55.7
54	45.0	39.4	59.2

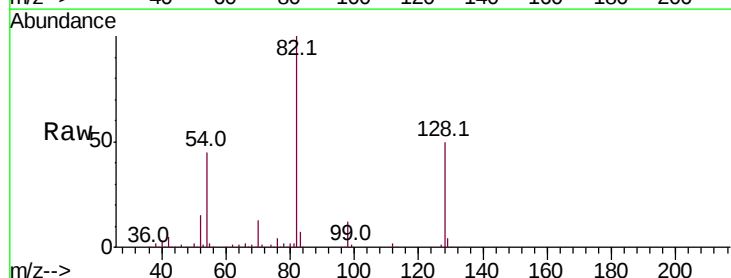

Abundance Ion 82.00 (81.70 to 82.70): BNC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BNC

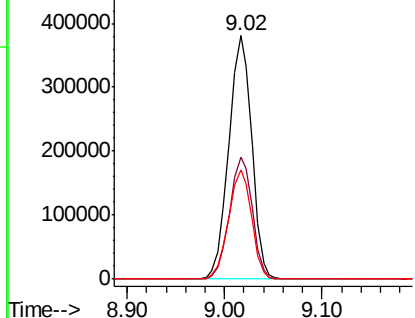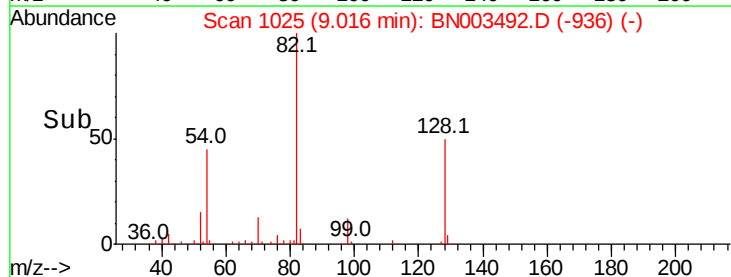

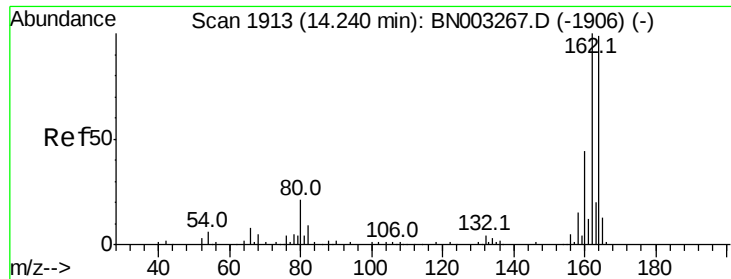

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.48 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-B


Tot Ion:164 Resp: 238812

Ion Ratio Lower Upper

164 100

162 100.7 80.8 121.2




160 44.2 35.5 53.3

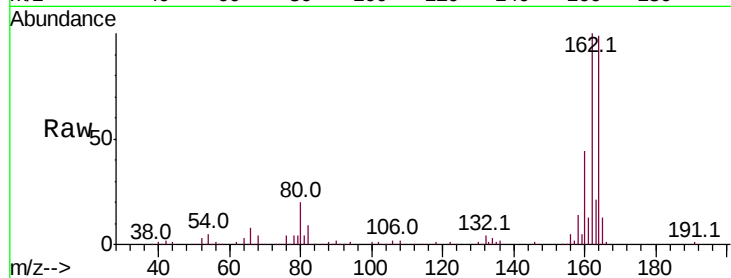

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

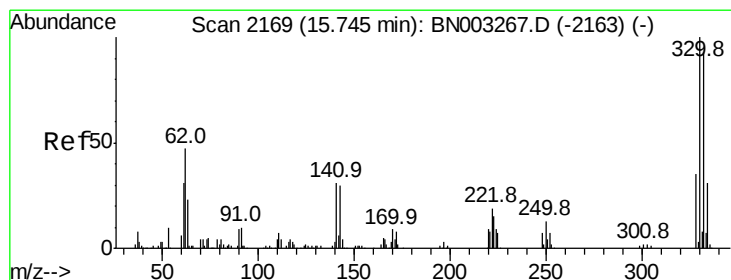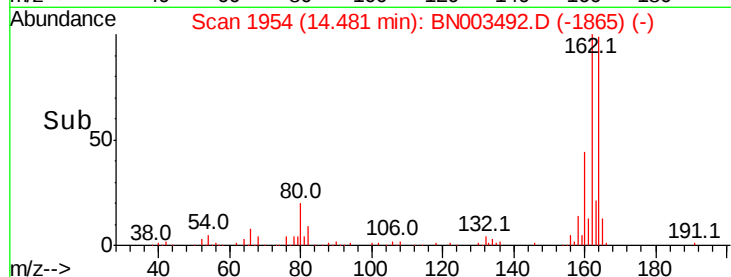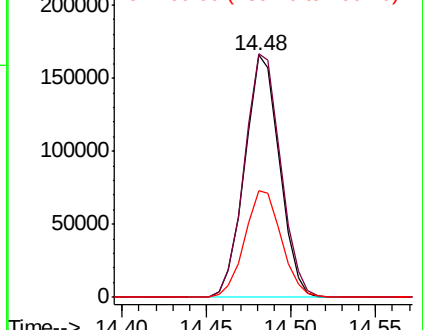

#42

2,4,6-Tribromophenol

Concen: 106.691 ng

RT: 15.97 min Scan# 2208

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59


Tgt Ion:330 Resp: 343083

Ion Ratio Lower Upper

330 100

332 96.7 76.6 114.8



141 27.0 24.5 36.7

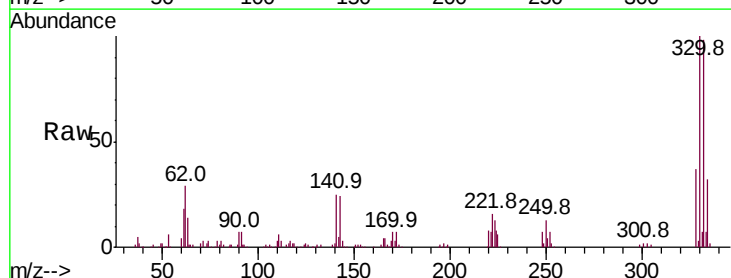


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

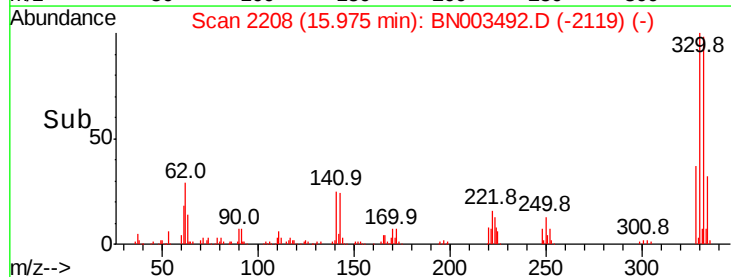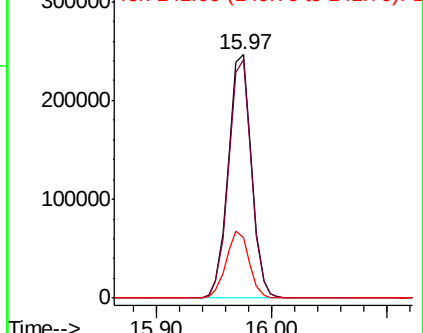




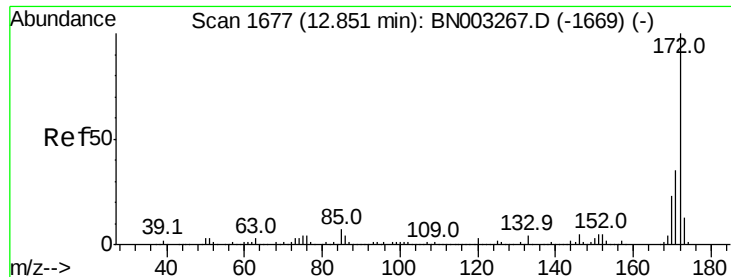


#45
 2-Fluorobiphenyl
 Concen: 100.186 ng
 RT: 13.10 min Scan# 1720
 Delta R.T. -0.01 min
 Lab File: BN003492.D
 Acq: 10 Nov 2018 02:59

Instrument :
 BNA_N
 ClientSampleId :
 110718-TIPC-F-D-B

Tot Ion:172 Resp: 1763880




Ion	Ratio	Lower	Upper
172	100		
171	36.3	28.2	42.4
170	23.5	18.4	27.6

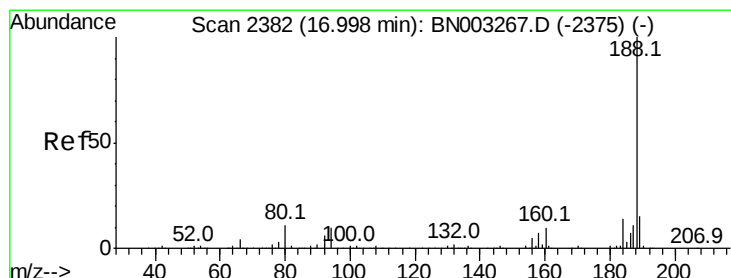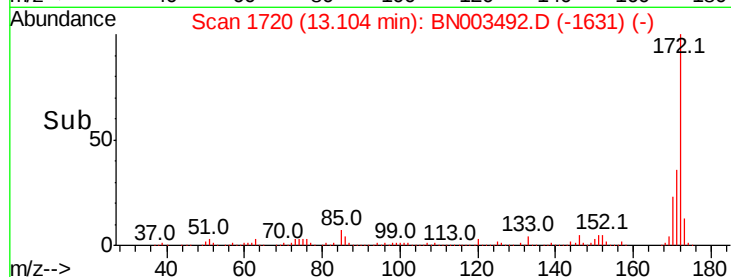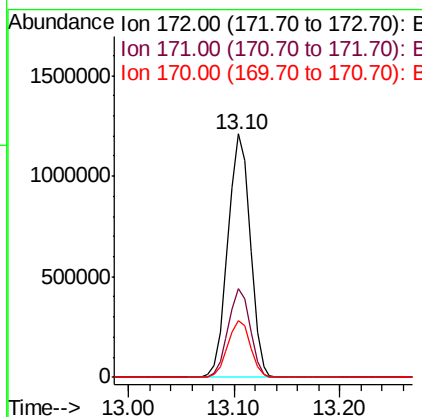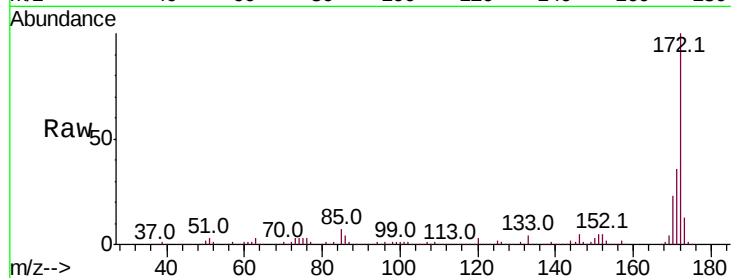


#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.23 min Scan# 2421
 Delta R.T. -0.01 min
 Lab File: BN003492.D
 Acq: 10 Nov 2018 02:59

Tgt Ion:188 Resp: 519775

Ion	Ratio	Lower	Upper
188	100		
94	9.4	8.1	12.1
80	10.3	8.6	13.0

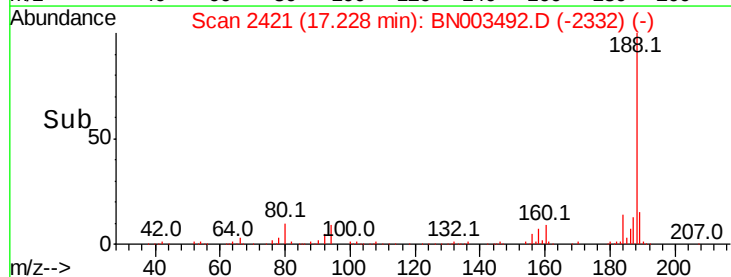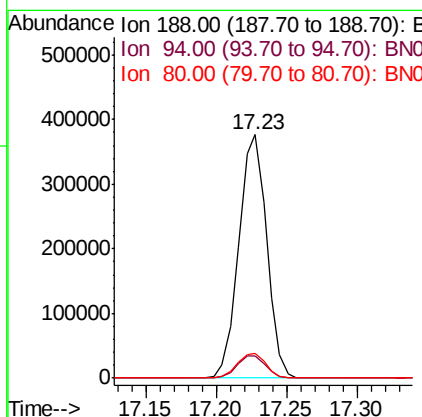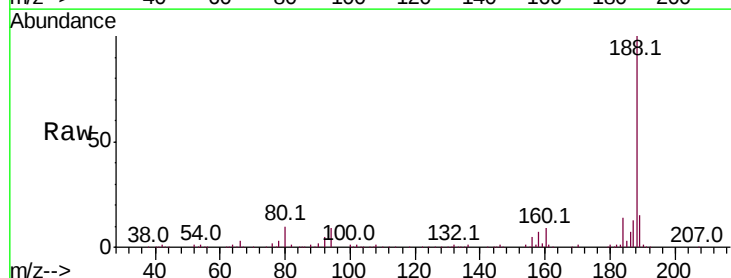

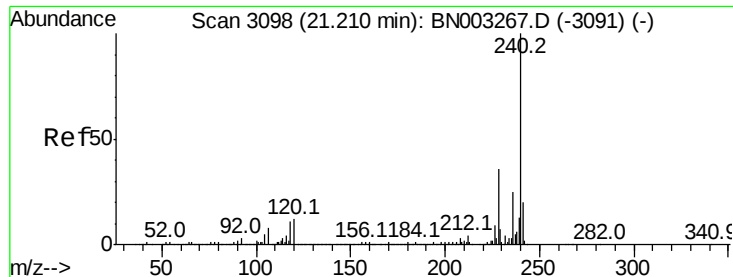

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.40 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-B


Tot Ion:240 Resp: 416579

Ion Ratio Lower Upper

240 100

120 10.5 9.4 14.0




236 26.1 20.3 30.5

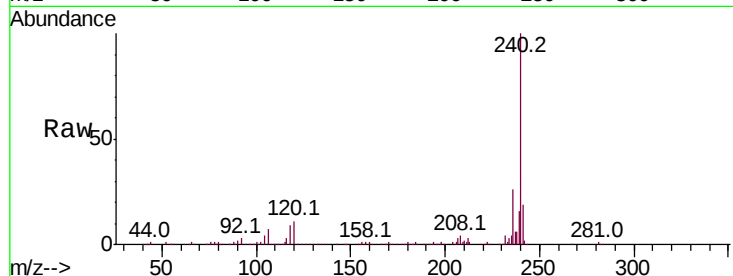

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

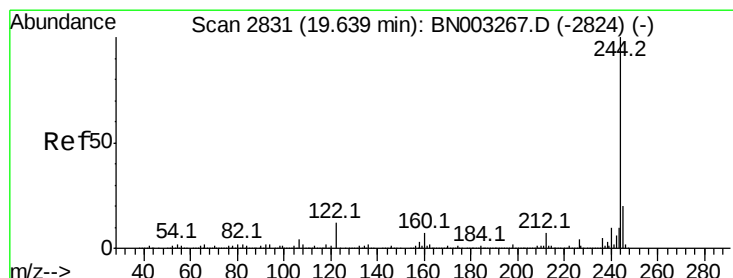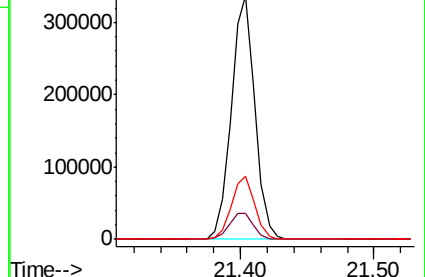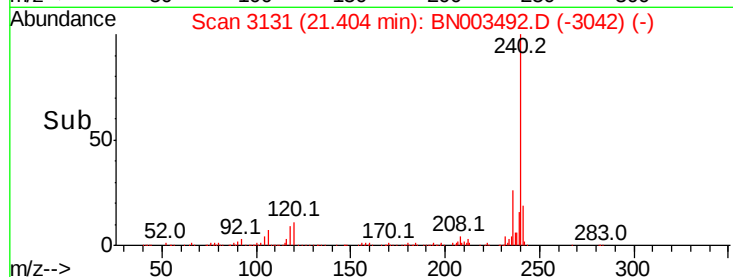

#79

Terphenyl-d14

Concen: 100.277 ng

RT: 19.85 min Scan# 2866

Delta R.T. -0.01 min

Lab File: BN003492.D

Acq: 10 Nov 2018 02:59


Tgt Ion:244 Resp: 1953344

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0



122 10.4 9.4 14.2

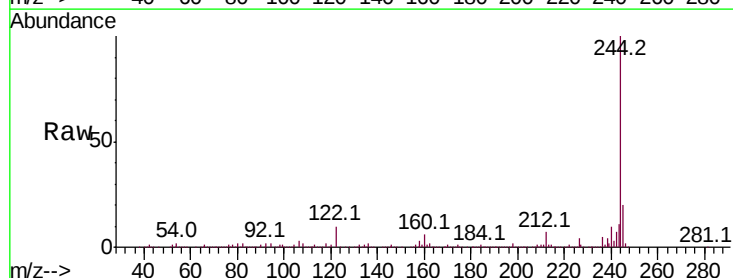


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

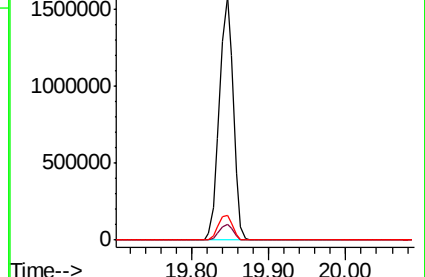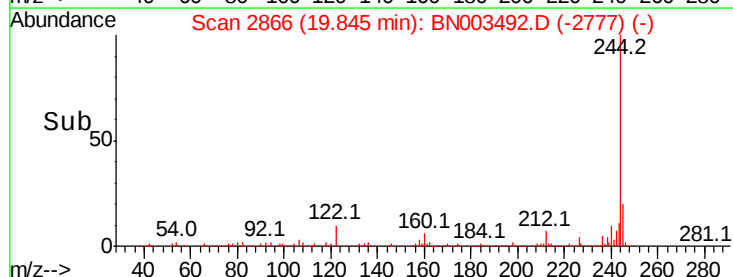


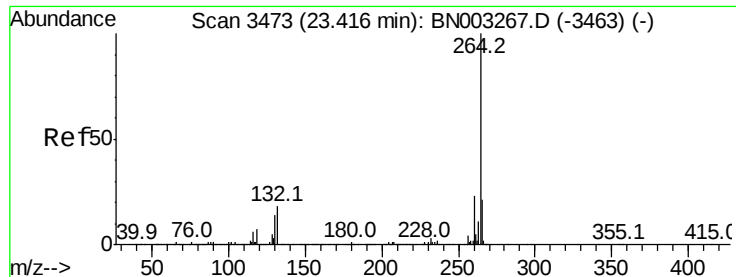

#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.72 min Scan# 3524
Delta R.T. -0.01 min
Lab File: BN003492.D
Acq: 10 Nov 2018 02:59

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	18.5	27.7
265	21.7	16.6	25.0

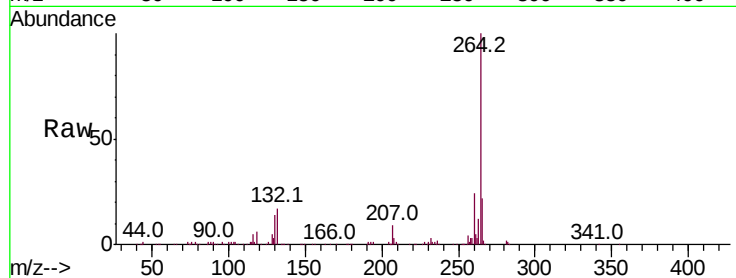

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

