

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
 Data File : BN003493.D
 Acq On : 10 Nov 2018 03:34
 Operator : MJ/SJ
 Sample : J5881-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 110718-TIPC-F-D-S

Quant Time: Nov 12 04:33:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 07 08:25:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	97025	20.00	ng	0.00
21) Naphthalene-d8	10.65	136	434348	20.00	ng	0.00
39) Acenaphthene-d10	14.48	164	261464	20.00	ng	0.00
64) Phenanthrene-d10	17.23	188	580799	20.00	ng	0.00
76) Chrysene-d12	21.40	240	473597	20.00	ng	0.00
87) Perylene-d12	23.72	264	460173	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	225113	40.41	ng	0.00
7) Phenol-d6	7.00	99	176560	22.29	ng	-0.01
23) Nitrobenzene-d5	9.02	82	664034	87.68	ng	0.00
42) 2,4,6-Tribromophenol	15.97	330	376206	106.86	ng	-0.01
45) 2-Fluorobiphenyl	13.10	172	1858929	96.44	ng	0.00
79) Terphenyl-d14	19.85	244	2166701	97.84	ng	0.00
Target Compounds						
10) Phenol	7.03	94	57532	6.883	ng	93
50) Dimethylphthalate	13.93	163	64267	3.040	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN110918\
Data File : BN003493.D
Acq On : 10 Nov 2018 03:34
Operator : MJ/SJ
Sample : J5881-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-S

Quant Time: Nov 12 04:33:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN102418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 07 08:25:32 2018
Response via : Initial Calibration

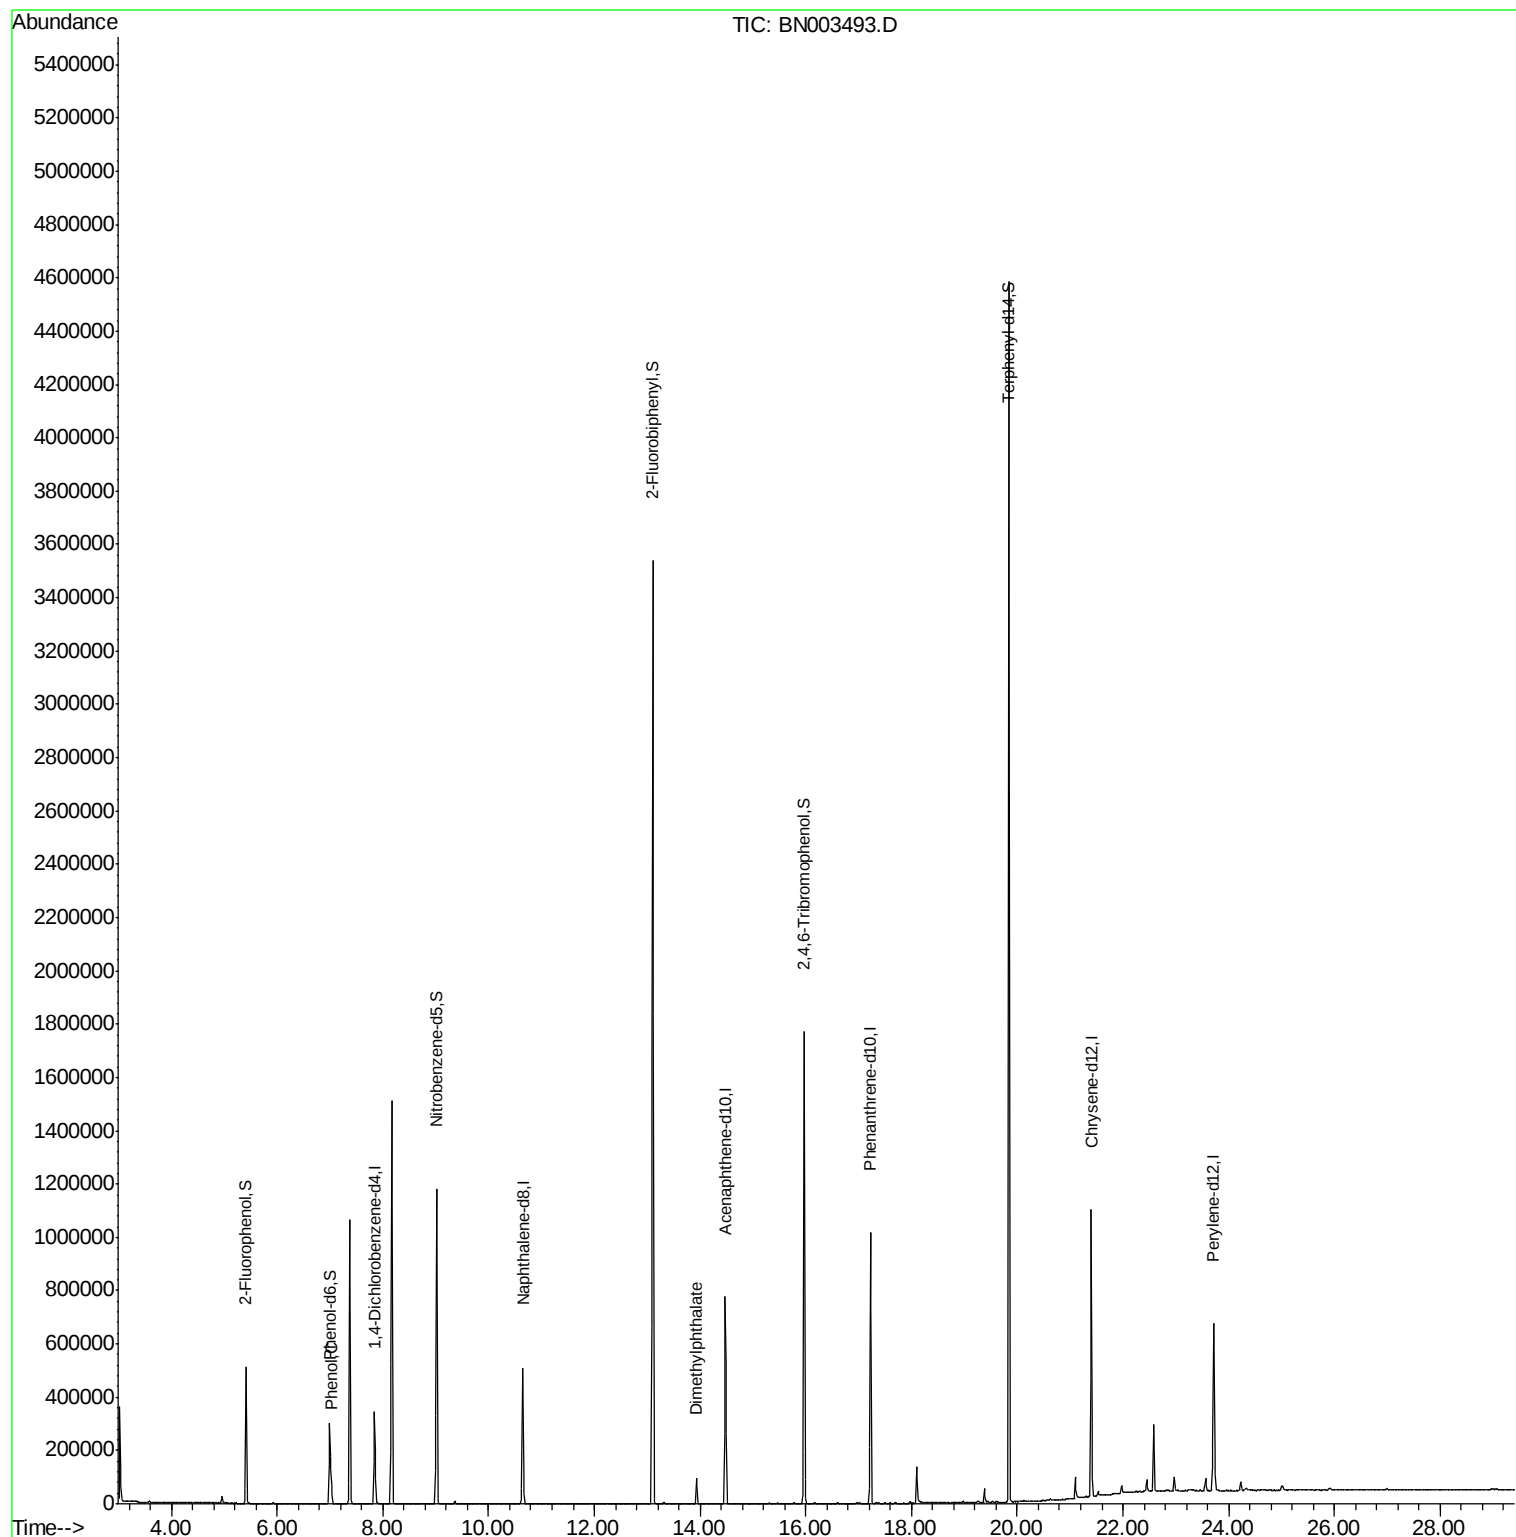

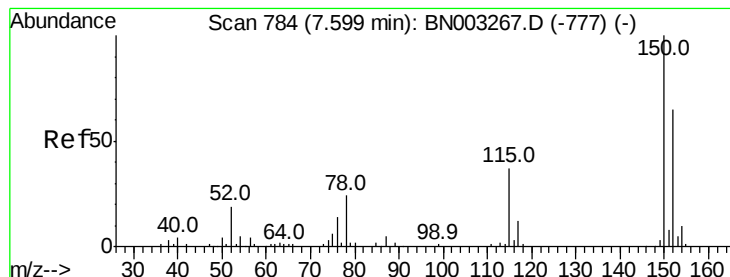


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.85 min Scan# 826
Delta R.T. -0.01 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-S

Tot Ion:152 Resp: 97025
Ion Ratio Lower Upper
152 100
150 153.7 123.8 185.8
115 57.0 45.9 68.9

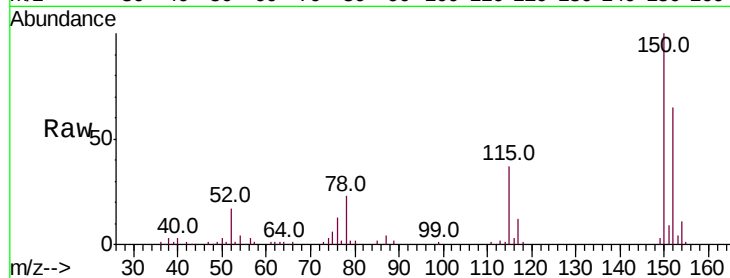


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

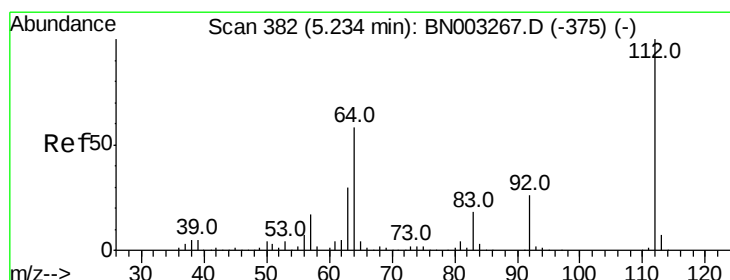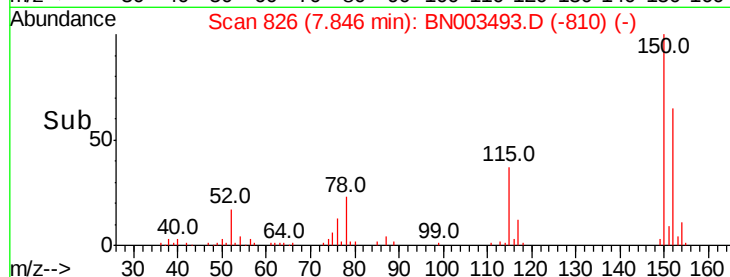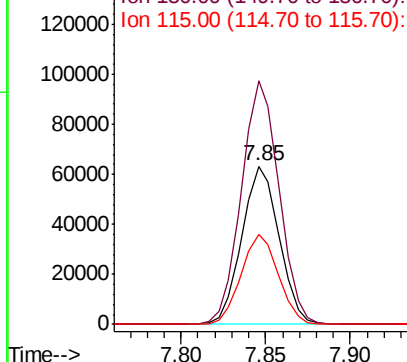



#5


2-Fluorophenol
Concen: 40.411 ng
RT: 5.41 min Scan# 412
Delta R.T. 0.00 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Tgt Ion:112 Resp: 225113
Ion Ratio Lower Upper
112 100
64 53.4 46.6 69.8
63 26.5 23.8 35.8

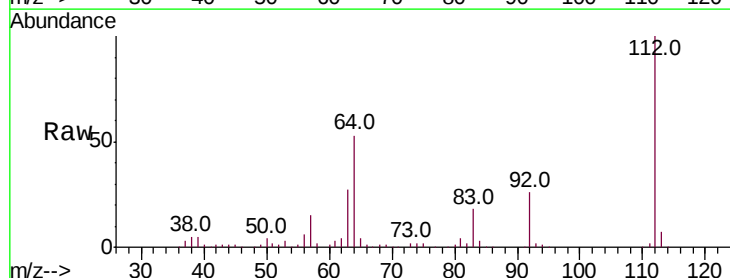

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

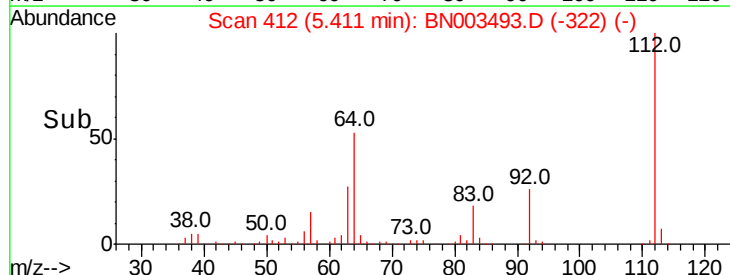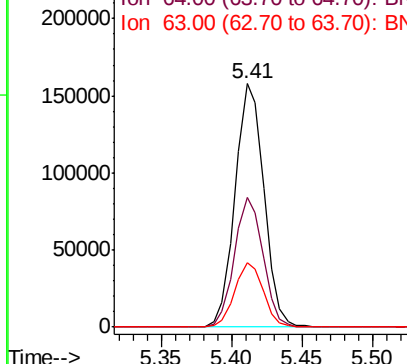

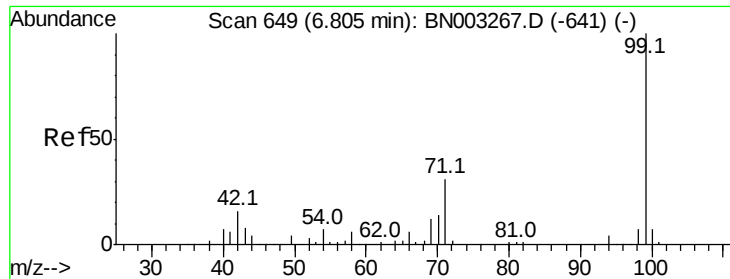

#7

Phenol-d6

Concen: 22.290 ng

RT: 7.00 min Scan# 682

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-S


Tot Ion: 99 Resp: 176560

Ion Ratio Lower Upper




99 100

42 15.1 13.0 19.6

71 29.8 24.5 36.7

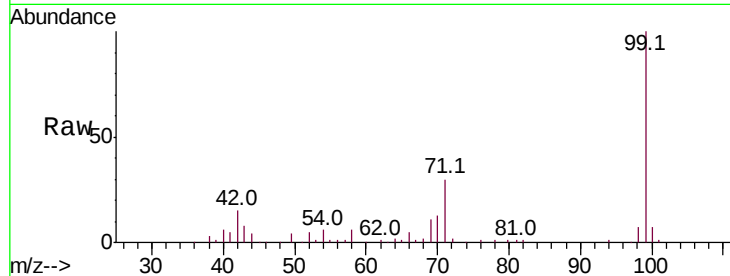

Abundance Ion 99.00 (98.70 to 99.70): BN0
Ion 42.00 (41.70 to 42.70): BN0
Ion 71.00 (70.70 to 71.70): BN0

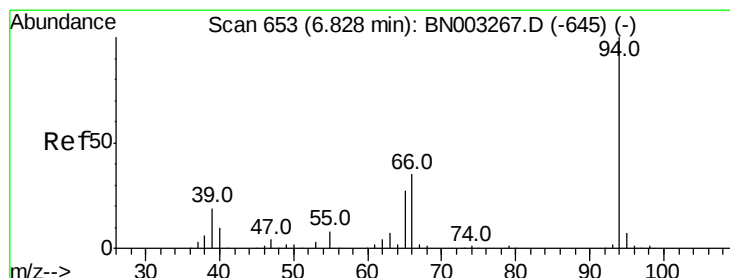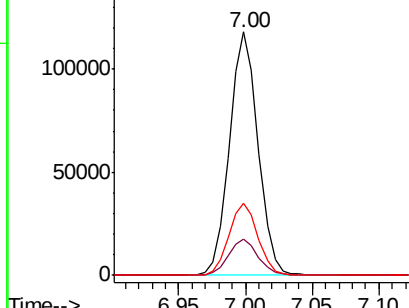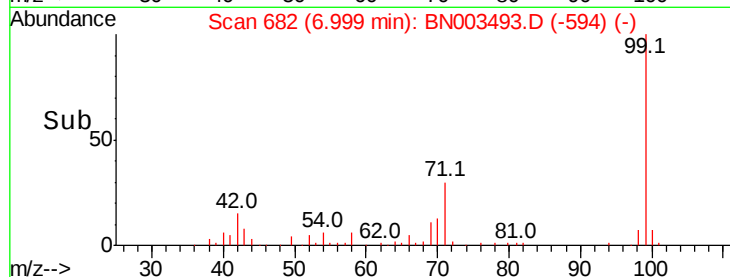

#10

Phenol

Concen: 6.883 ng

RT: 7.03 min Scan# 687

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34


Tgt Ion: 94 Resp: 57532

Ion Ratio Lower Upper



94 100


65 24.4 7.7 47.7

66 31.8 15.8 55.8

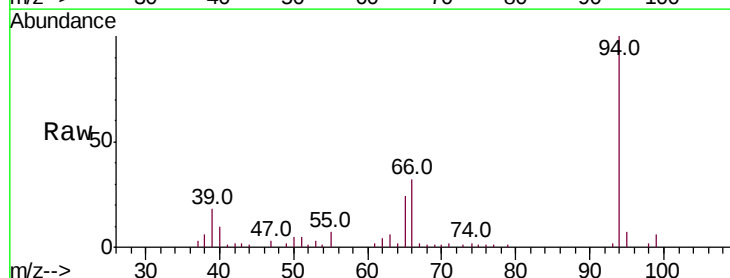

Abundance Ion 94.00 (93.70 to 94.70): BN0
Ion 65.00 (64.70 to 65.70): BN0
Ion 66.00 (65.70 to 66.70): BN0

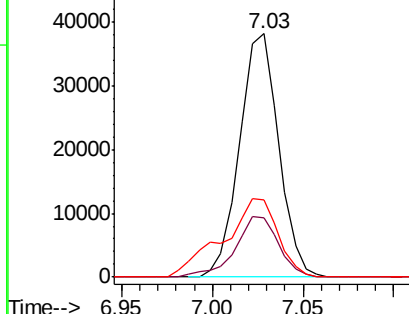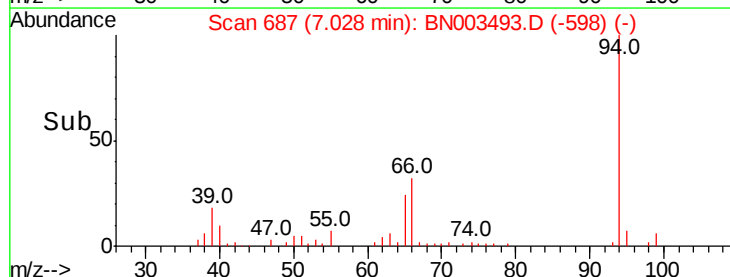


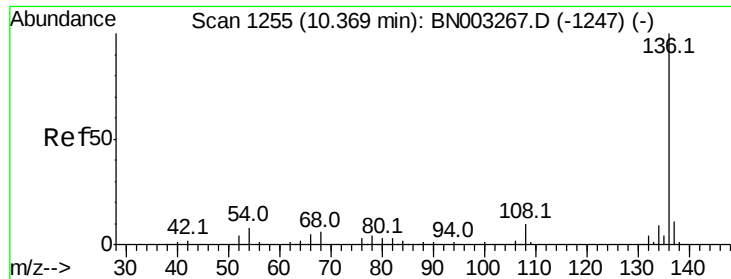

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.65 min Scan# 1302
Delta R.T. -0.01 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-S

Tot Ion:	136	Resp:	434348
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.7	13.1
54	7.0	6.6	10.0
68	6.1	4.6	7.0

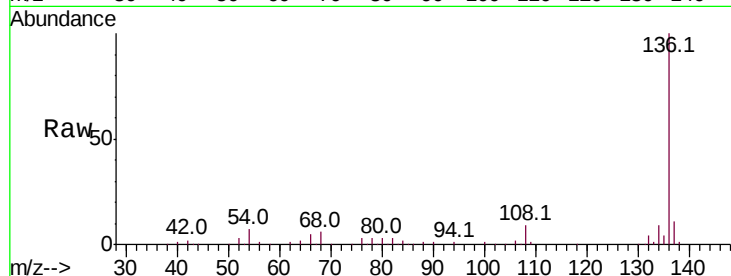




Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

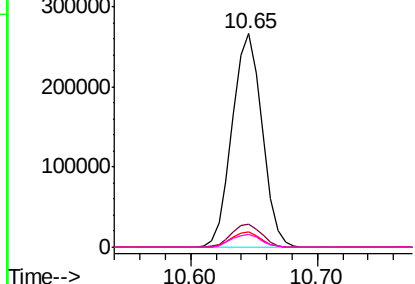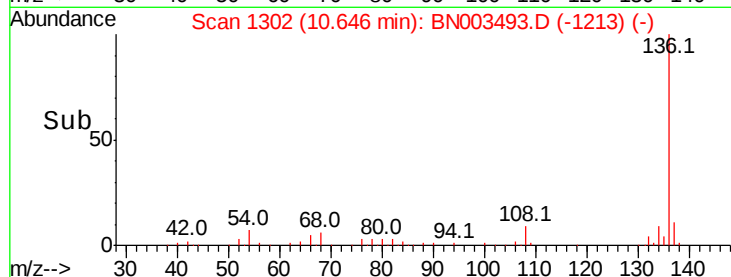

#23
Nitrobenzene-d5
Concen: 87.676 ng
RT: 9.02 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Tgt Ion:	82	Resp:	664034
Ion	Ratio	Lower	Upper
82	100		
128	50.3	37.1	55.7
54	45.4	39.4	59.2






Abundance

Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

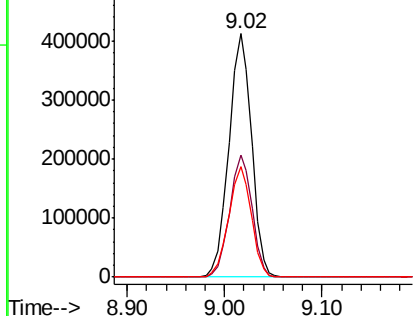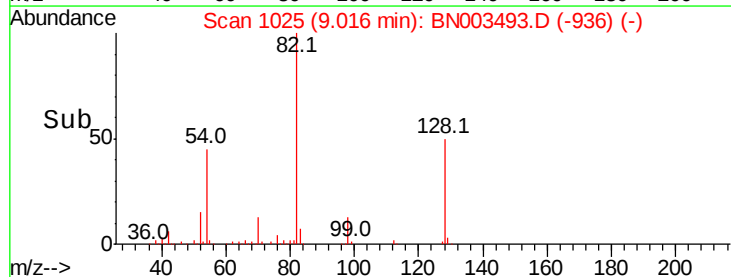

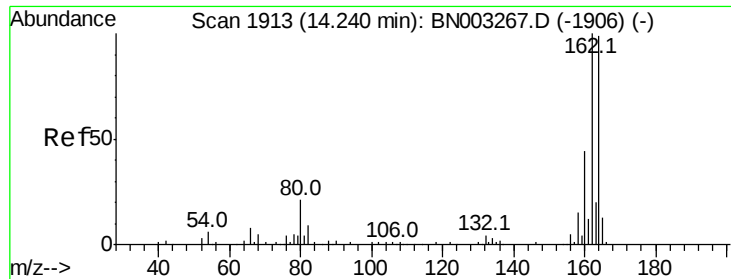

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.48 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-S


Tot Ion:164 Resp: 261464

Ion Ratio Lower Upper

164 100

162 100.6 80.8 121.2




160 44.9 35.5 53.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

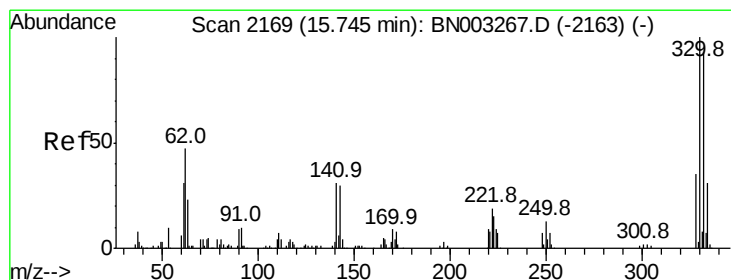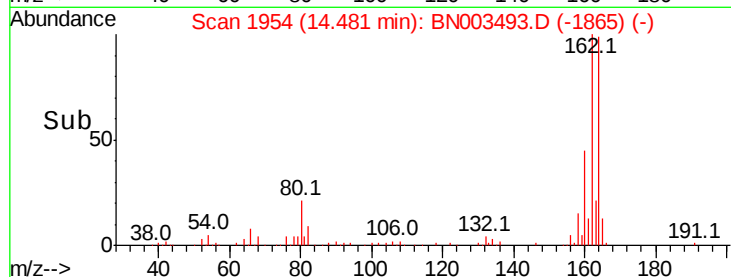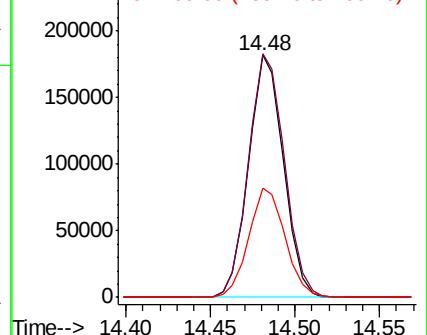

#42

2,4,6-Tribromophenol

Concen: 106.855 ng

RT: 15.97 min Scan# 2207

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34


Tgt Ion:330 Resp: 376206

Ion Ratio Lower Upper

330 100

332 96.0 76.6 114.8



141 27.0 24.5 36.7

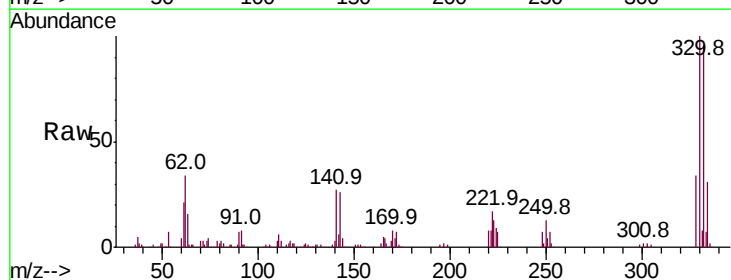


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

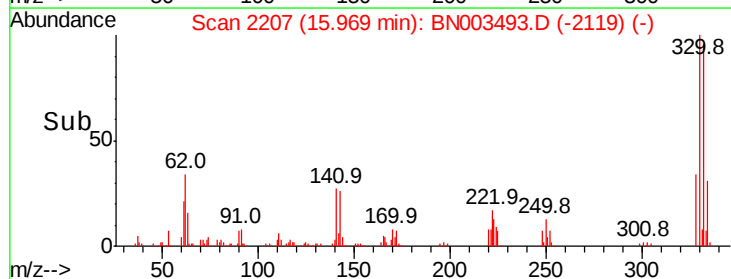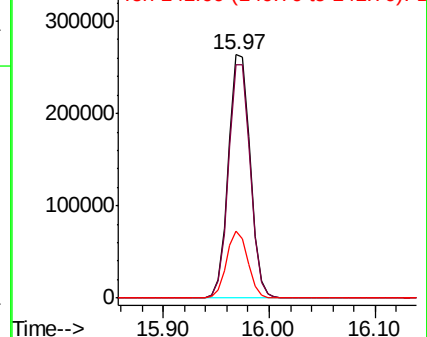


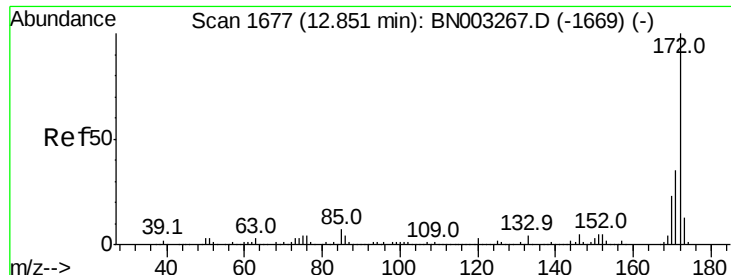




#45
2-Fluorobiphenyl
Concen: 96.438 ng
RT: 13.10 min Scan# 1720
Delta R.T. -0.01 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Instrument :
BNA_N
ClientSampleId :
110718-TIPC-F-D-S

Tot Ion:172 Resp: 1858929
Ion Ratio Lower Upper
172 100
171 36.8 28.2 42.4
170 23.6 18.4 27.6

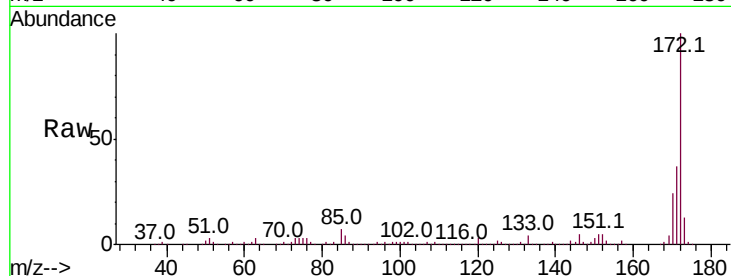


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

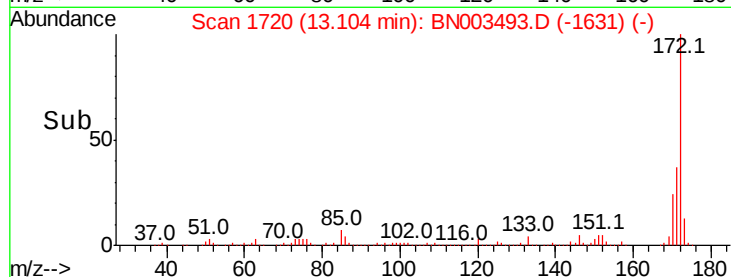
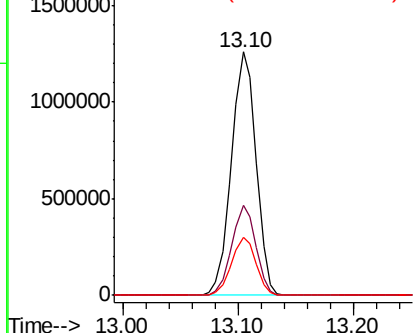



#50
Dimethylphthalate
Concen: 3.040 ng
RT: 13.93 min Scan# 1861
Delta R.T. -0.02 min
Lab File: BN003493.D
Acq: 10 Nov 2018 03:34

Tgt Ion:163 Resp: 64267
Ion Ratio Lower Upper
163 100
194 4.7 3.4 5.2
164 10.9 7.9 11.9



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

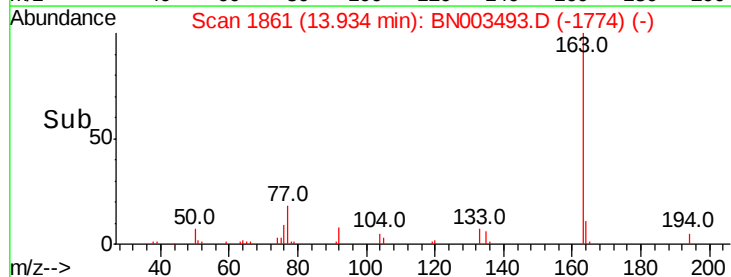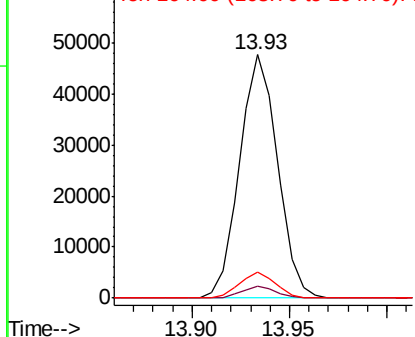

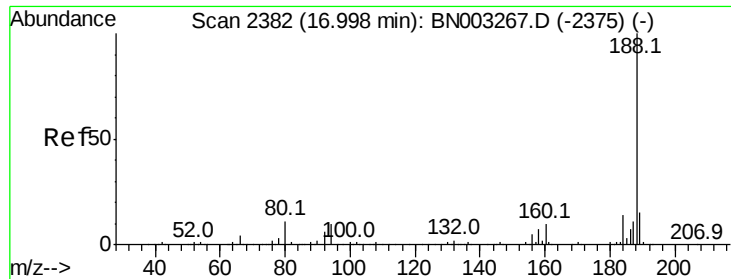

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.23 min Scan# 2421

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-S


Tot Ion:188 Resp: 580799

Ion Ratio Lower Upper

188 100

94 9.4 8.1 12.1




80 10.2 8.6 13.0

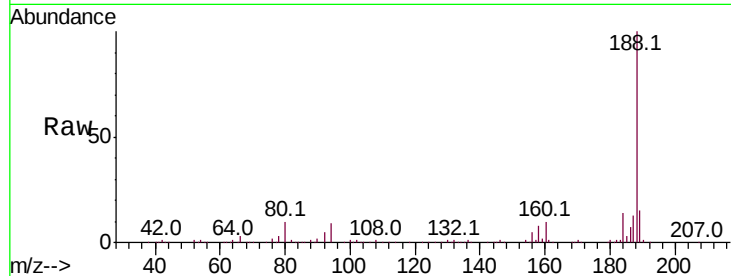

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

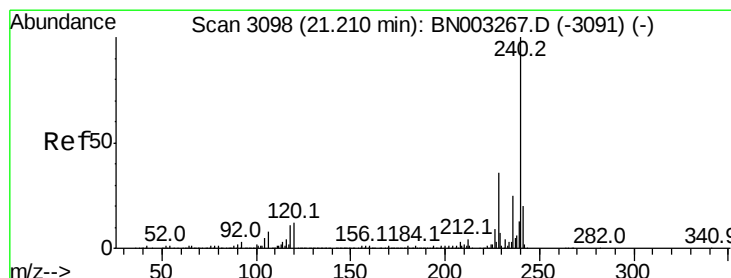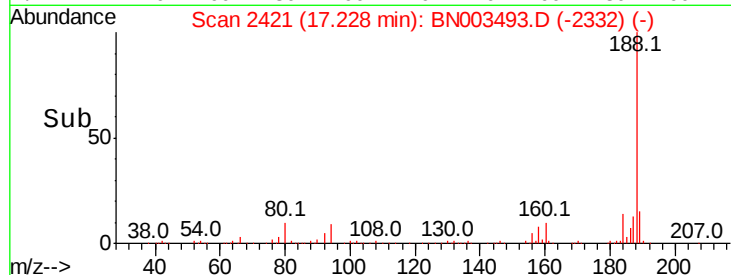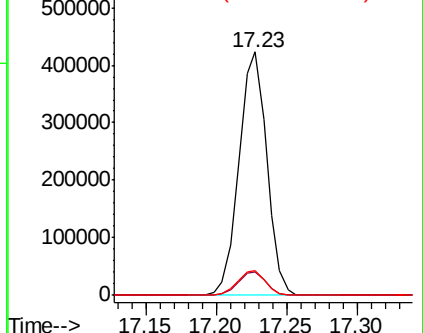

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.40 min Scan# 3131

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34


Tgt Ion:240 Resp: 473597

Ion Ratio Lower Upper

240 100

120 11.0 9.4 14.0



236 26.0 20.3 30.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

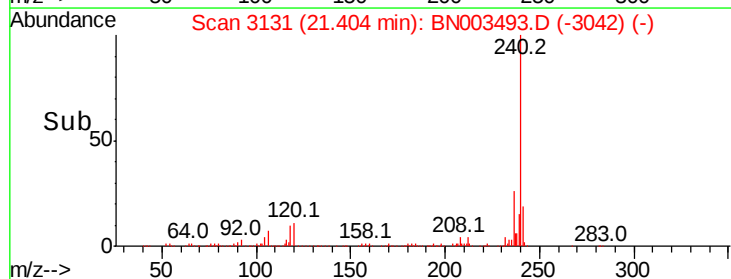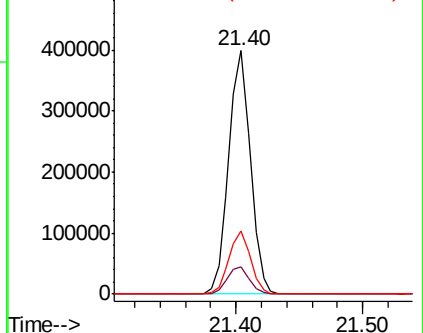

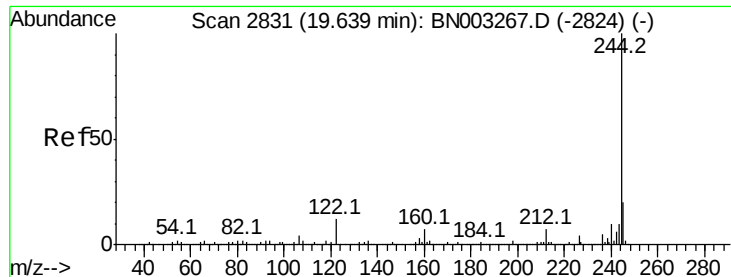

#79

Terphenyl-d14

Concen: 97.838 ng

RT: 19.85 min Scan# 2866

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34

Instrument :

BNA_N

ClientSampleId :

110718-TIPC-F-D-S


Tot Ion:244 Resp: 2166701

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0




122 10.5 9.4 14.2



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

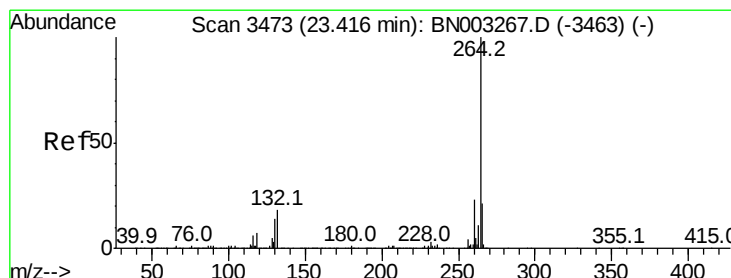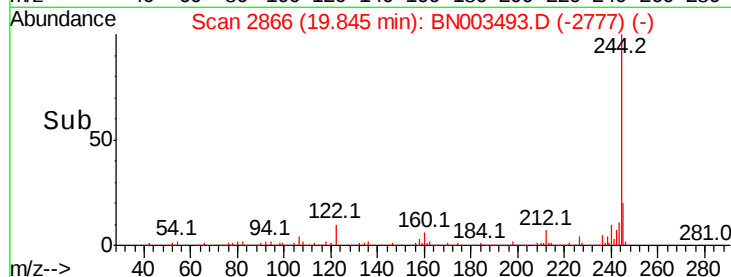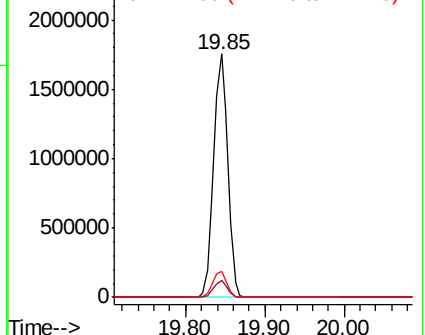

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.72 min Scan# 3524

Delta R.T. -0.01 min

Lab File: BN003493.D

Acq: 10 Nov 2018 03:34


Tgt Ion:264 Resp: 460173

Ion Ratio Lower Upper

264 100

260 23.8 18.5 27.7

265 21.4 16.6 25.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

