


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110918\
 Data File : BN003487.D
 Acq On : 10 Nov 2018 00:02
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN102418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 07 08:25:32 2018

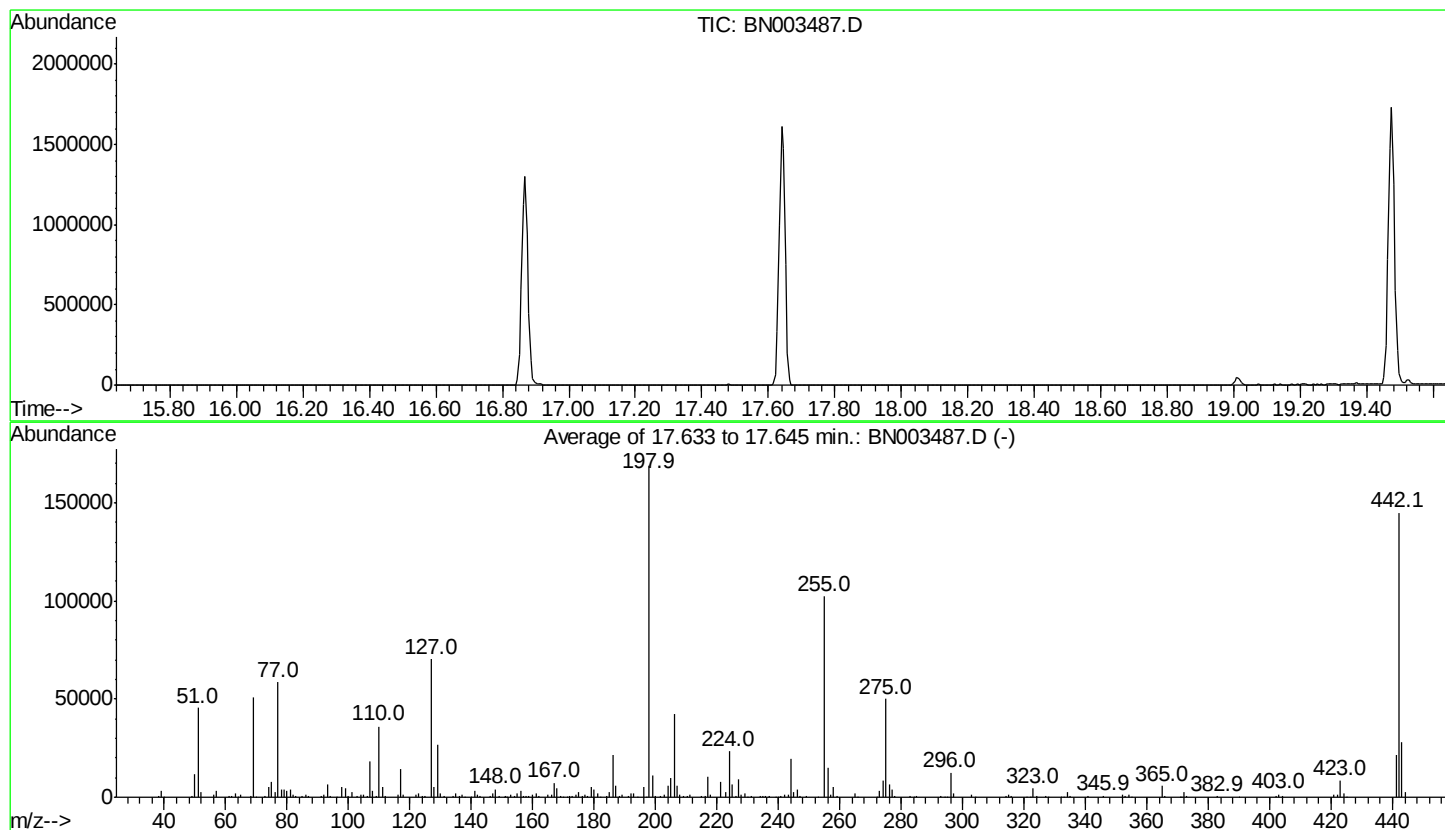

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	45352	PASS
68	69	0.00	2	1.8	934	PASS
69	198	0.00	100	29.9	50576	PASS
70	69	0.00	2	0.2	104	PASS
127	198	10	80	41.7	70424	PASS
197	198	0.00	2	0.2	267	PASS
198	198	100	100	100.0	168925	PASS
199	198	5	9	6.8	11428	PASS
275	198	10	60	29.6	50074	PASS
365	198	1	100	3.5	5846	PASS
441	198	0.01	100	12.9	21841	PASS
442	198	50	100	85.8	144922	PASS
443	442	15	24	19.5	28200	PASS