
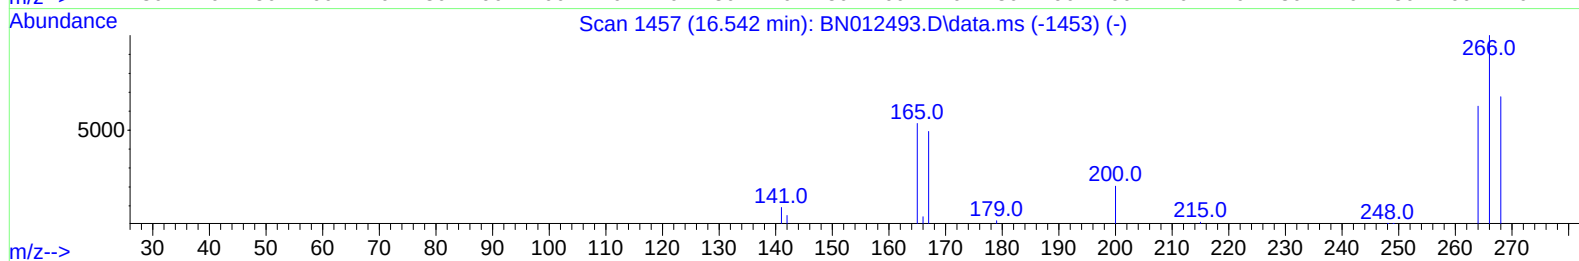
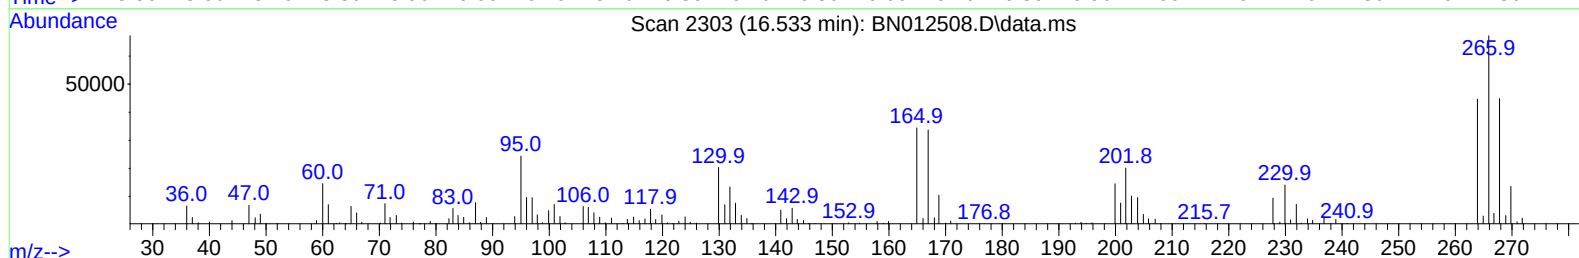


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110920\
Data File : BN012508.D
Acq On : 09 Nov 2020 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 06:43:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 05 05:46:47 2020
Response via : Initial Calibration

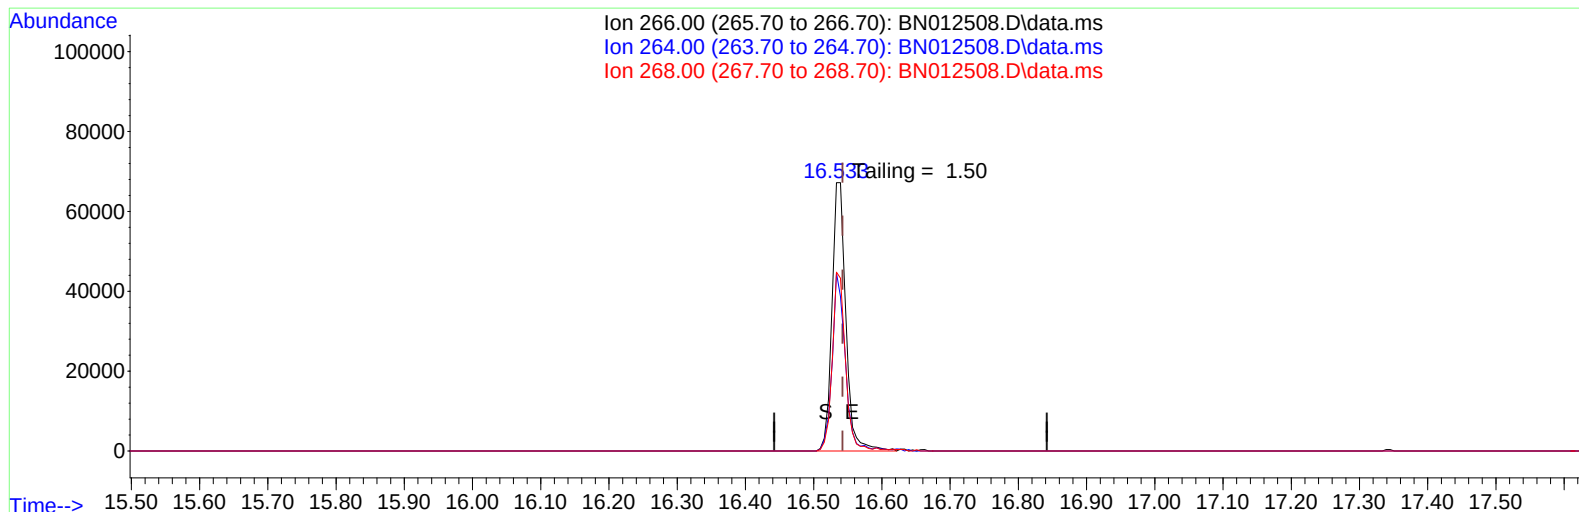

TIC: BN012508.D\data.ms

(24) Pentachlorophenol

16.533min (-0.009) 0.00 ng

response 95374

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.62
268.00	64.40	62.76
0.00	0.00	0.00