


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110920\
 Data File : BN012508.D
 Acq On : 09 Nov 2020 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 05 05:46:47 2020

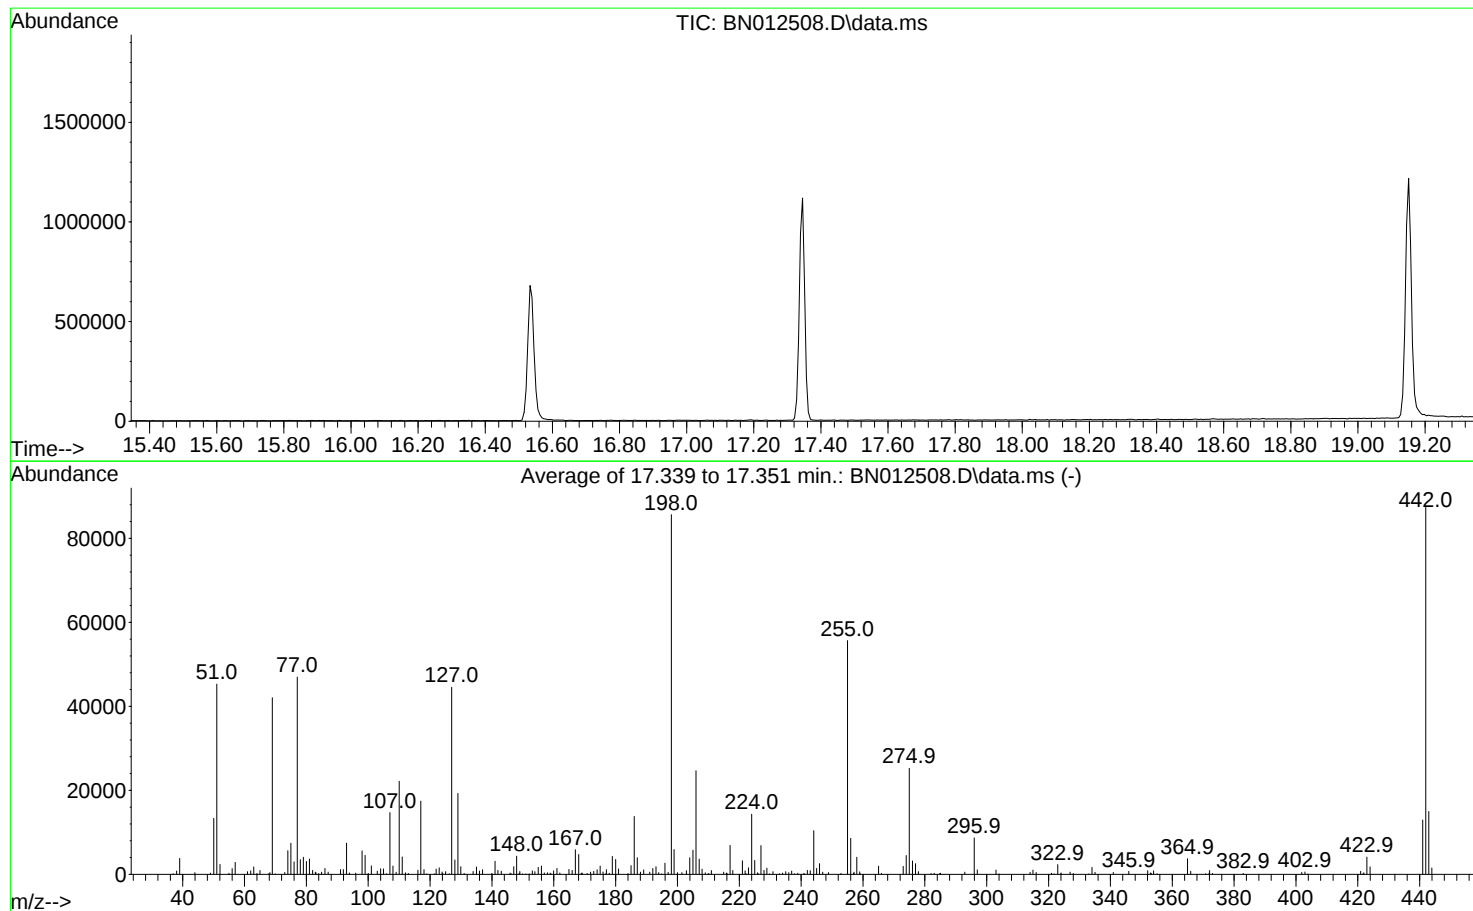

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	45296	PASS
68	69	0.00	2	1.0	405	PASS
69	198	0.00	100	49.1	42061	PASS
70	69	0.00	2	0.2	105	PASS
127	198	10	80	52.0	44549	PASS
197	198	0.00	2	0.6	514	PASS
198	198	100	100	100.0	85637	PASS
199	198	5	9	6.9	5891	PASS
275	198	10	60	29.5	25283	PASS
365	198	1	100	4.3	3721	PASS
441	198	0.01	100	15.1	12954	PASS
442	442	100	100	100.0	87597	PASS
443	442	15	24	17.1	14973	PASS