

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028525.D
 Acq On : 09 Nov 2023 19:08
 Operator : MA/JU
 Sample : PB156743BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK743

Quant Time: Nov 09 23:44:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8153	0.400	ng/ul	0.00
4) Naphthalene-d8	10.496	136	26932	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.354	164	16860	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.103	188	37016	0.400	ng/ul	0.00
17) Chrysene-d12	21.318	240	27512	0.400	ng/ul	0.00
23) Perylene-d12	23.624	264	29483	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	66997	7.435	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	15821	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	37511	0.424	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.353	166	5337	0.074	ng/ul#	12
20) Pyrene	19.513	202	4826	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.481	252	9868	0.094	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028525.D
Acq On : 09 Nov 2023 19:08
Operator : MA/JU
Sample : PB156743BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK743

Quant Time: Nov 09 23:44:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration




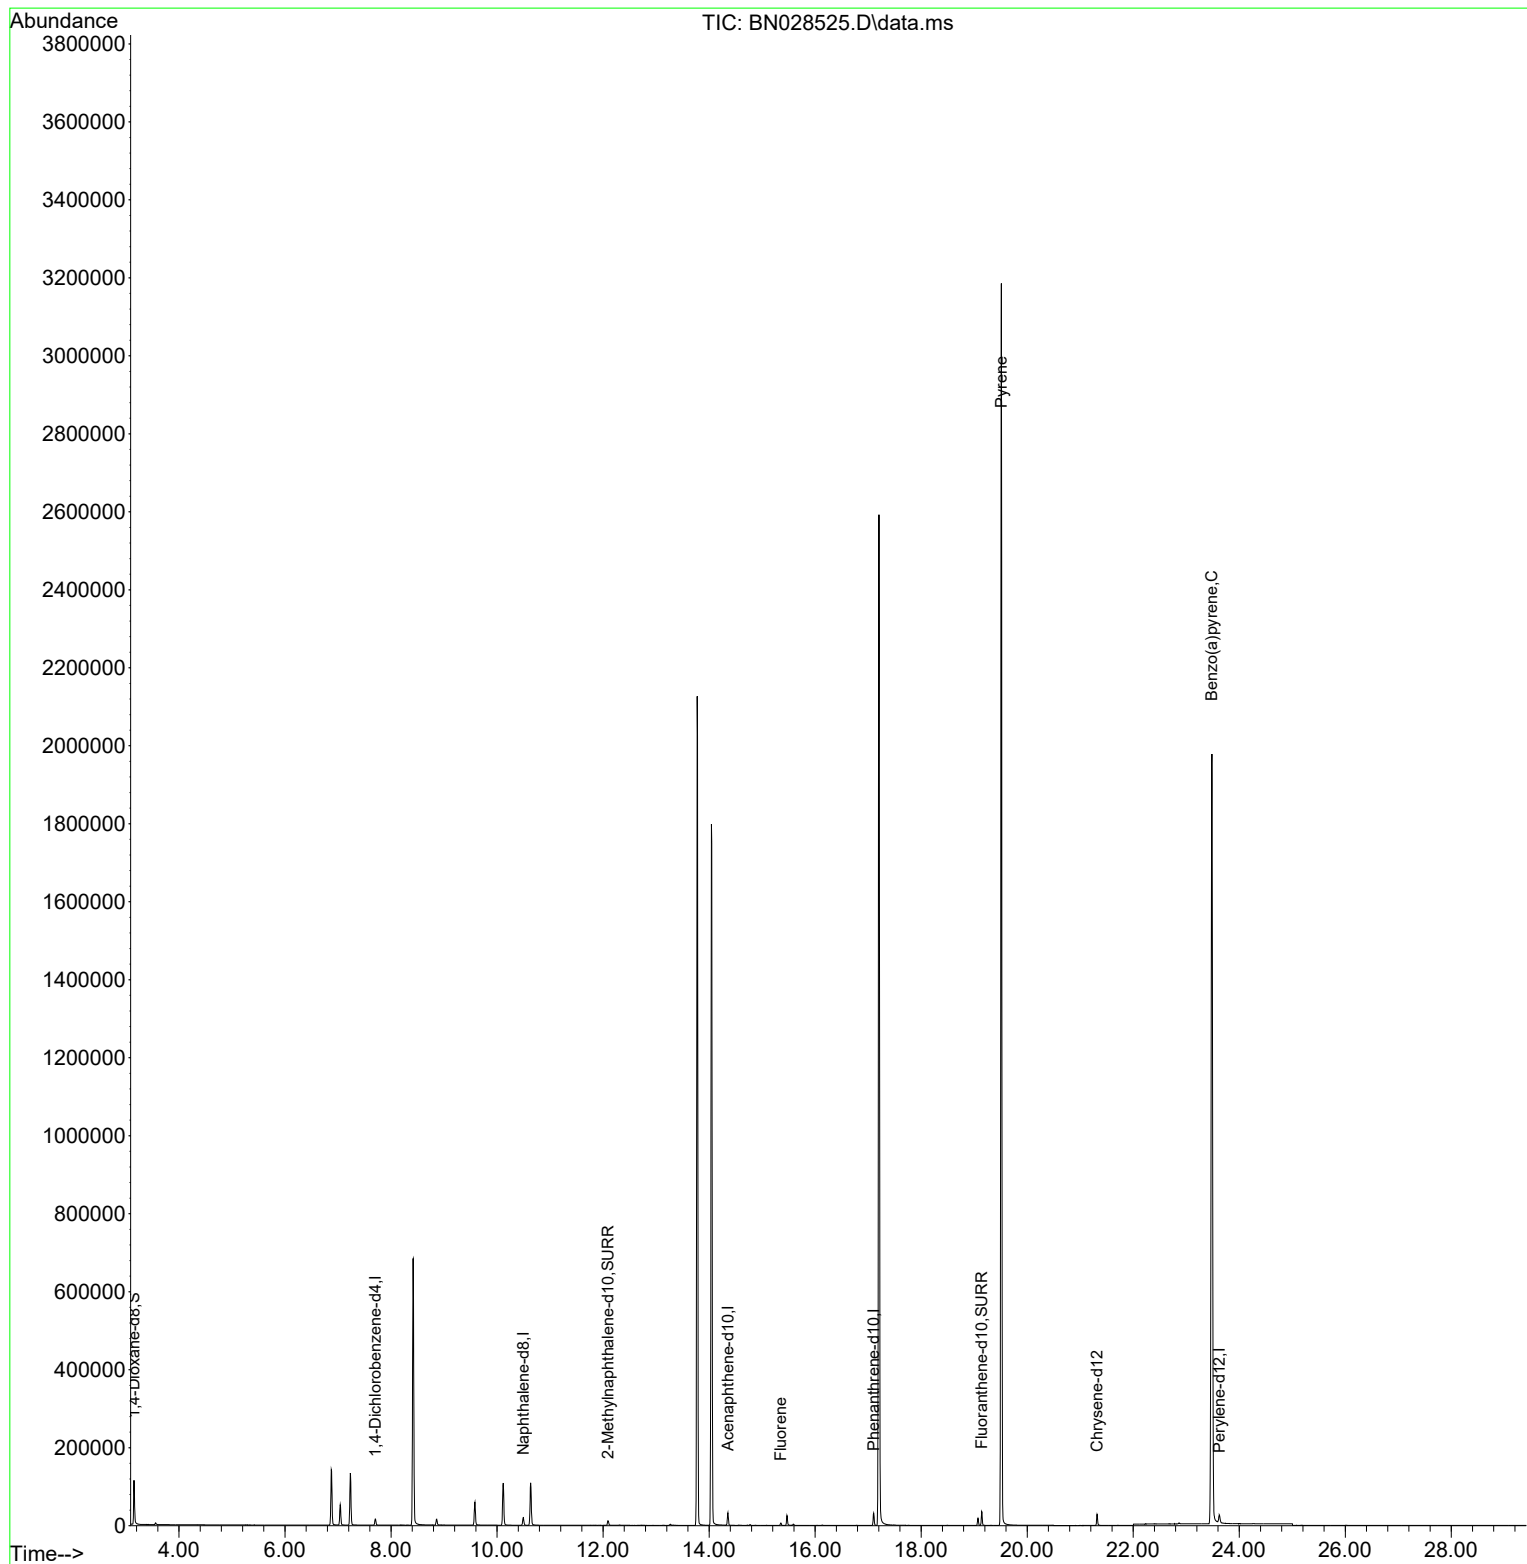


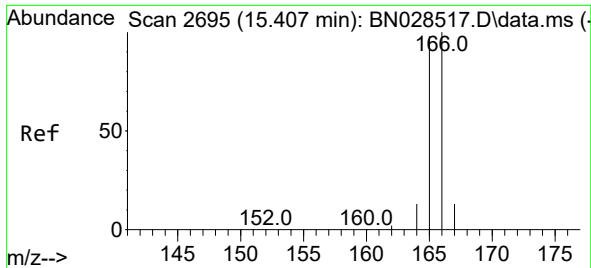

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.353 min Scan# 2683
Delta R.T. -0.054 min
Lab File: BN028525.D
Acq: 09 Nov 2023 19:08




Instrument :
BNA_N
ClientSampleId :
SBLK743


Tgt Ion:166 Resp: 5337
Ion Ratio Lower Upper
166 100
165 5.8 78.6 118.0#
167 34.2 11.0 16.6#

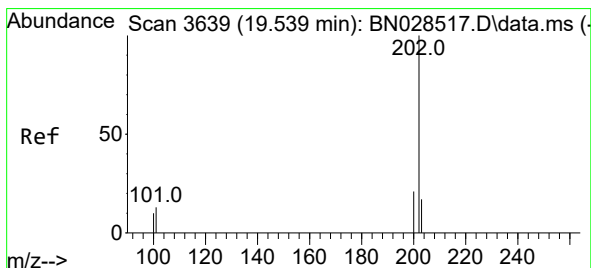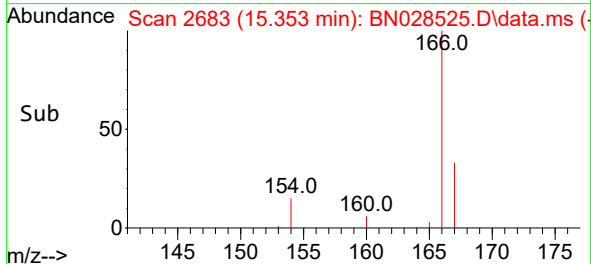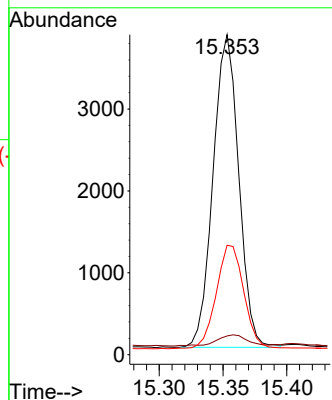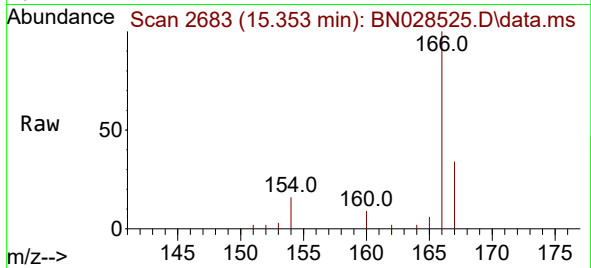

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.026 min
Lab File: BN028525.D
Acq: 09 Nov 2023 19:08


Tgt Ion:202 Resp: 4826
Ion Ratio Lower Upper
202 100
101 142.0 10.3 15.5#
100 1004.9 8.2 12.2#

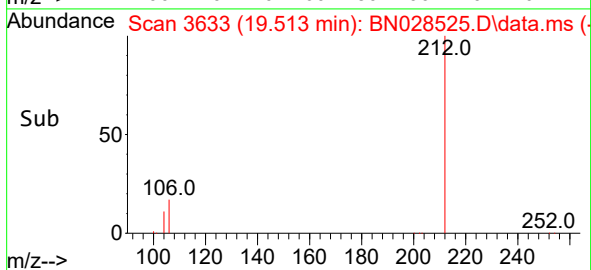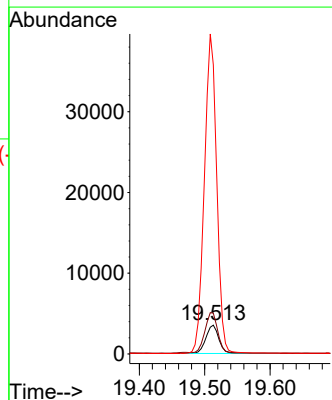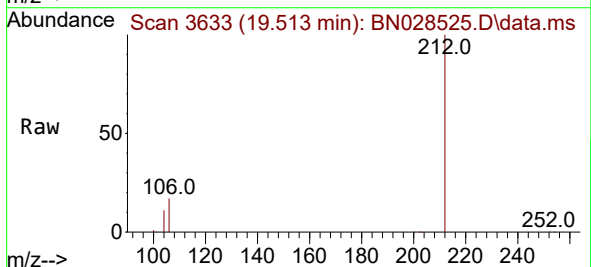

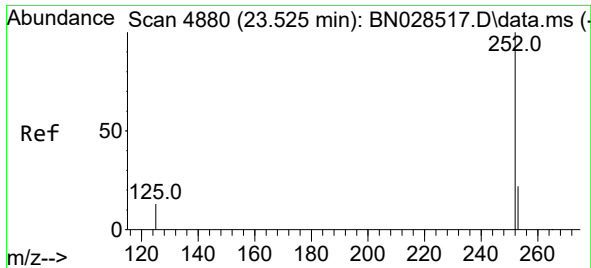

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.481 min Scan# 4865
Delta R.T. -0.044 min
Lab File: BN028525.D
Acq: 09 Nov 2023 19:08

Instrument :
BNA_N
ClientSampleId :
SBLK743

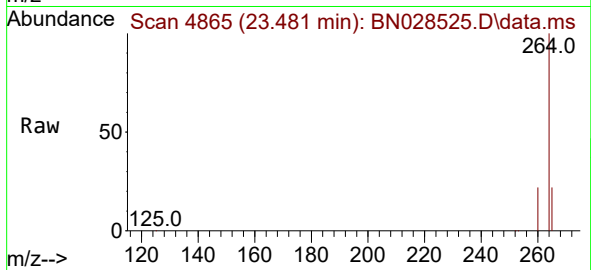

Tgt Ion:252 Resp: 9868
Ion Ratio Lower Upper
252 100
253 36.6 19.0 28.6#
125 33.3 13.2 19.8#

