

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028560.D
 Acq On : 10 Nov 2023 16:45
 Operator : MA/JU
 Sample : PB156720BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK718

Quant Time: Nov 10 23:27:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	6268	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	21267	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.349	164	13719	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.099	188	31005	0.400	ng/ul	0.00
17) Chrysene-d12	21.317	240	23535	0.400	ng/ul	0.00
23) Perylene-d12	23.620	264	24083	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	43873	6.333	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	11809	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	30281	0.400	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.348	166	3970	0.068	ng/ul#	14
20) Pyrene	19.508	202	3784	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.474	252	7157	0.084	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028560.D
Acq On : 10 Nov 2023 16:45
Operator : MA/JU
Sample : PB156720BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK718

Quant Time: Nov 10 23:27:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration




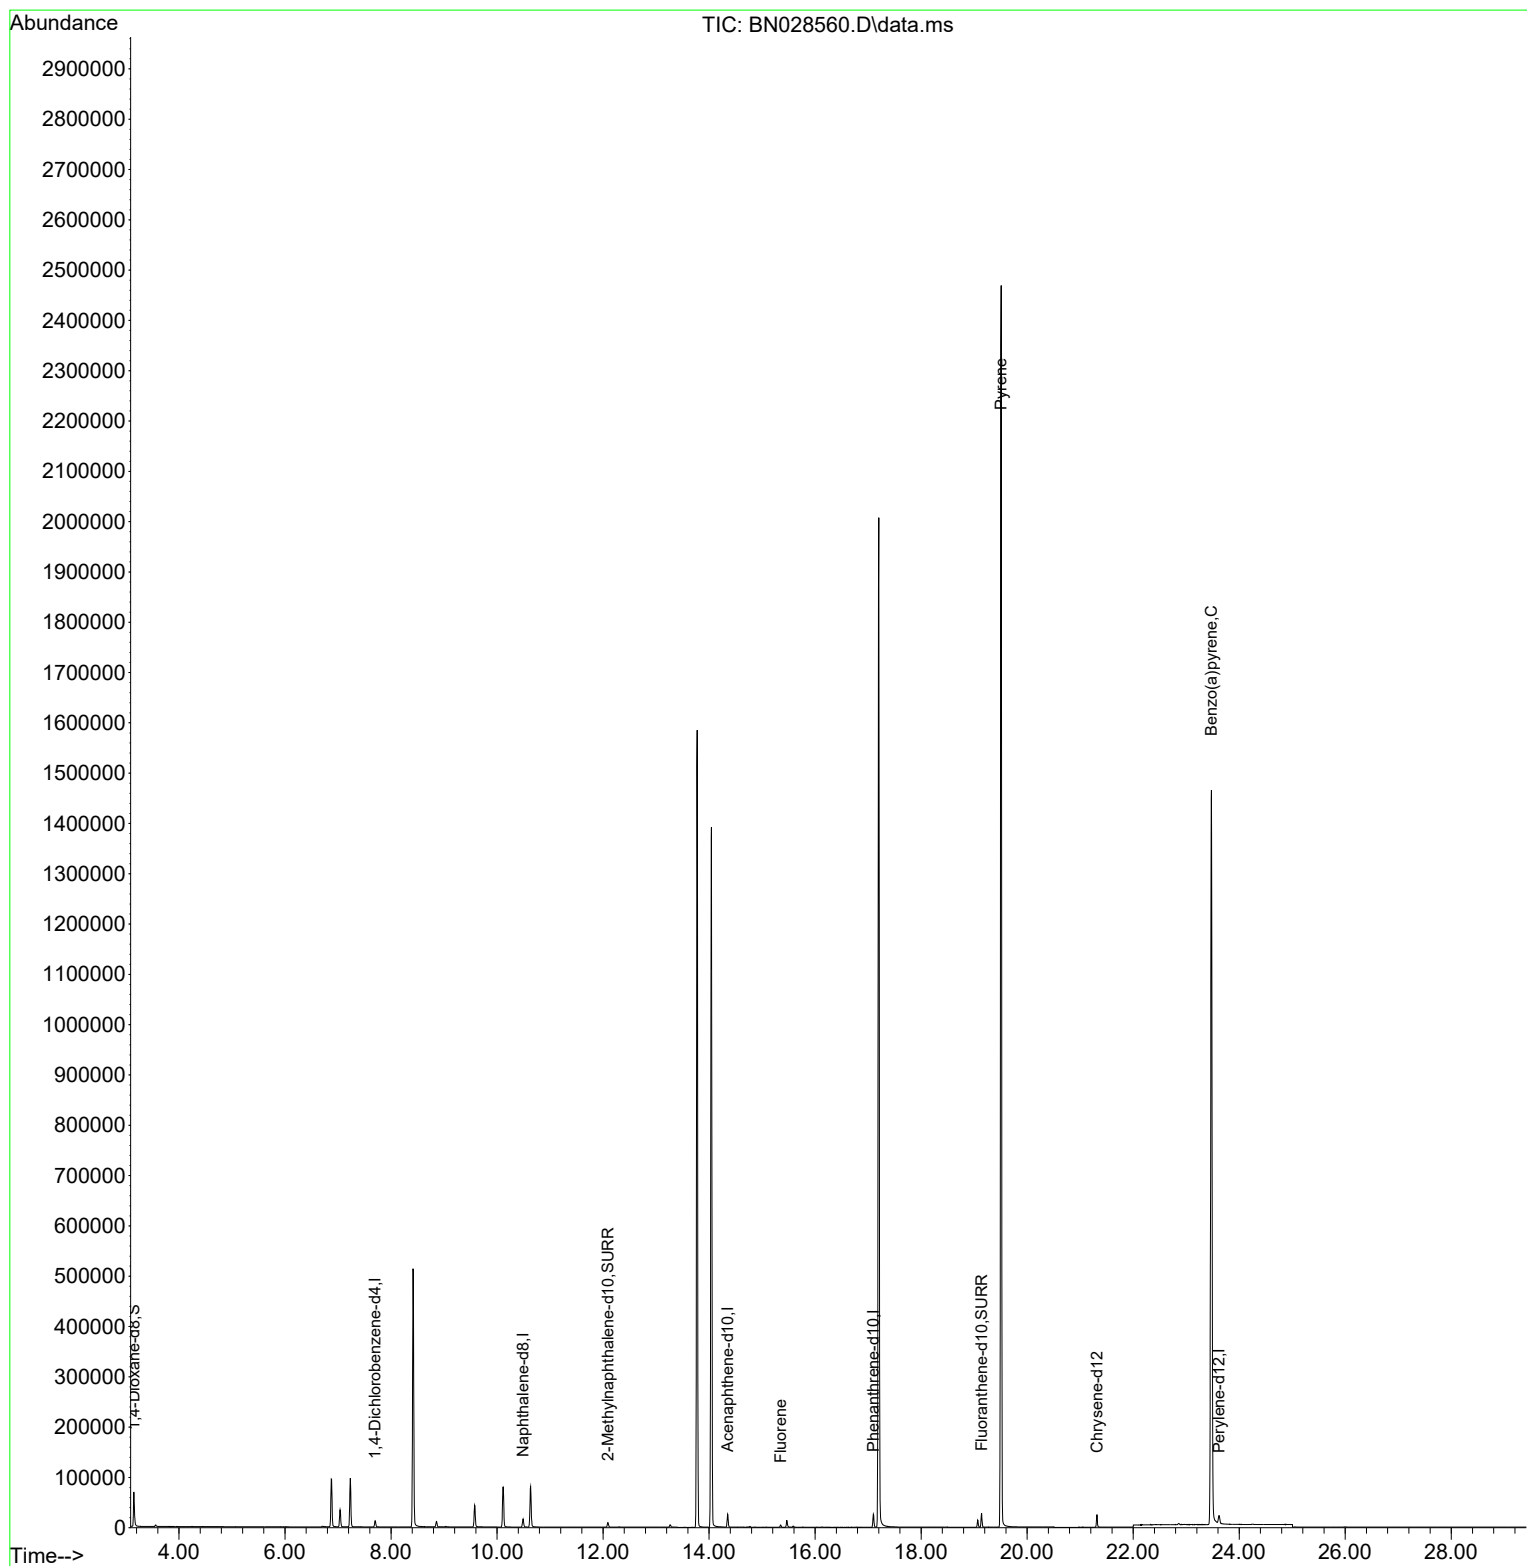


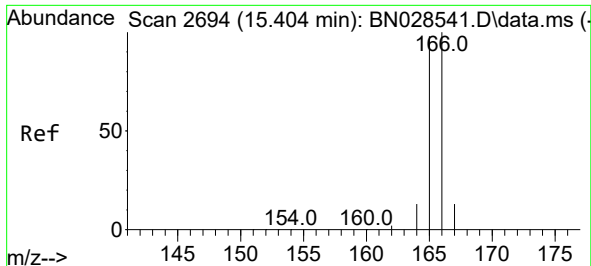

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.348 min Scan# 2682
Delta R.T. -0.059 min
Lab File: BN028560.D
Acq: 10 Nov 2023 16:45




Instrument :
BNA_N
ClientSampleId :
SBLK718


Tgt Ion:166 Resp: 3970
Ion Ratio Lower Upper
166 100
165 7.9 78.6 118.0#
167 33.3 11.0 16.6#

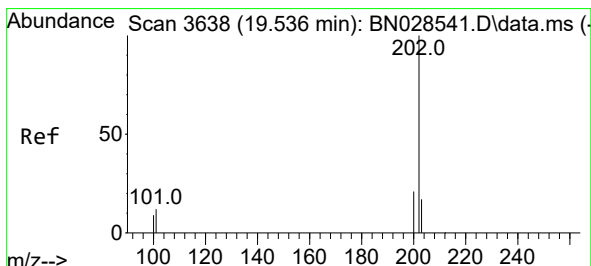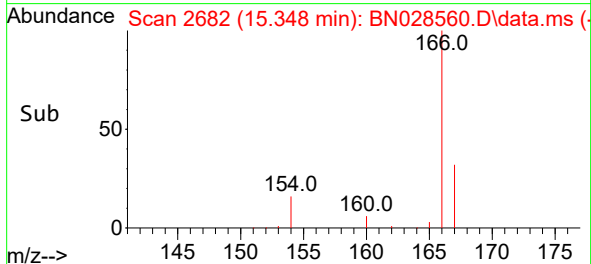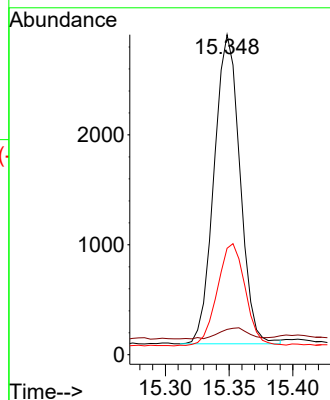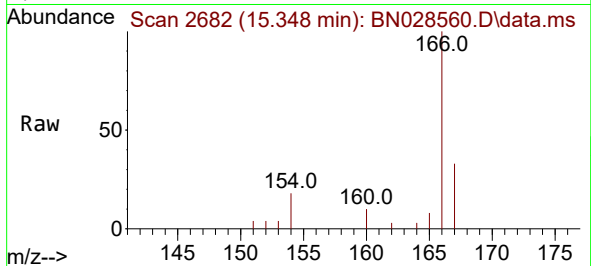

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.508 min Scan# 3632
Delta R.T. -0.031 min
Lab File: BN028560.D
Acq: 10 Nov 2023 16:45


Tgt Ion:202 Resp: 3784
Ion Ratio Lower Upper
202 100
101 136.0 10.3 15.5#
100 975.7 8.2 12.2#

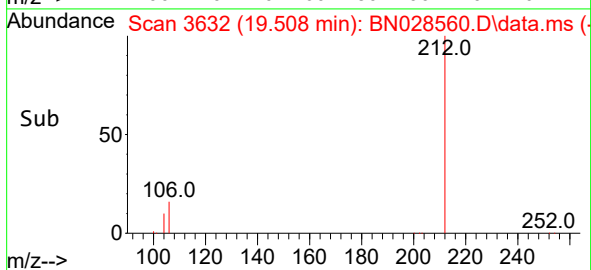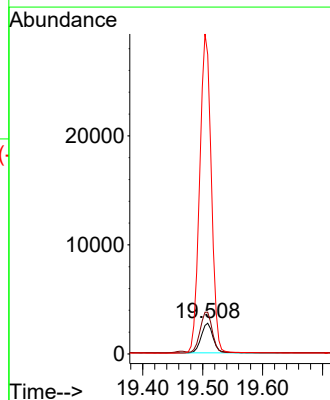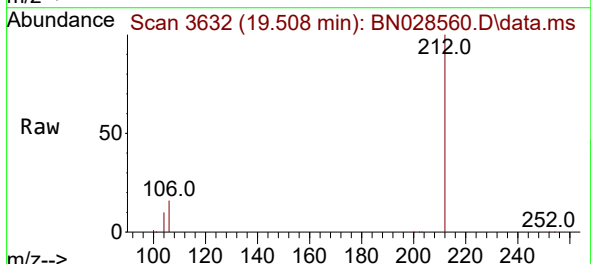

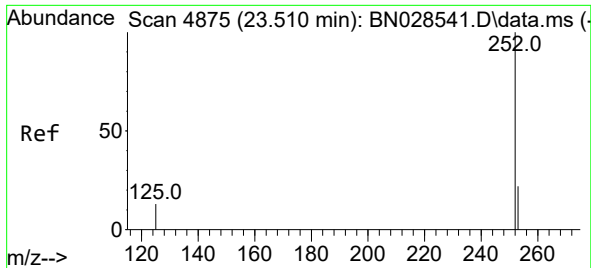

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.474 min Scan# 41
Delta R.T. -0.051 min
Lab File: BN028560.D
Acq: 10 Nov 2023 16:45

Instrument :
BNA_N
ClientSampleId :
SBLK718

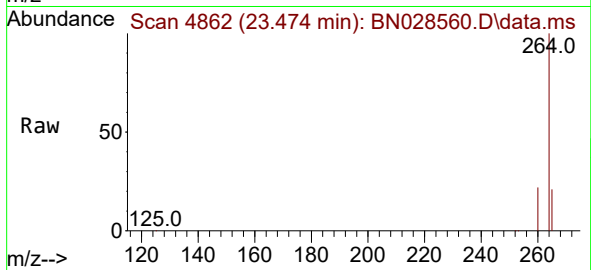

Tgt Ion:252 Resp: 7157
Ion Ratio Lower Upper
252 100
253 42.0 19.0 28.6#
125 38.4 13.2 19.8#

