

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028561.D
 Acq On : 10 Nov 2023 17:21
 Operator : MA/JU
 Sample : PB156717BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK717

Quant Time: Nov 10 23:28:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	7280	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	23920	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.349	164	14717	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.099	188	32193	0.400	ng/ul	0.00
17) Chrysene-d12	21.317	240	22613	0.400	ng/ul	0.00
23) Perylene-d12	23.620	264	23960	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	52783	6.560	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	13002	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	30305	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.348	166	4241	0.067	ng/ul#	14
20) Pyrene	19.508	202	3800	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.477	252	7119	0.084	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028561.D
Acq On : 10 Nov 2023 17:21
Operator : MA/JU
Sample : PB156717BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK717

Quant Time: Nov 10 23:28:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration




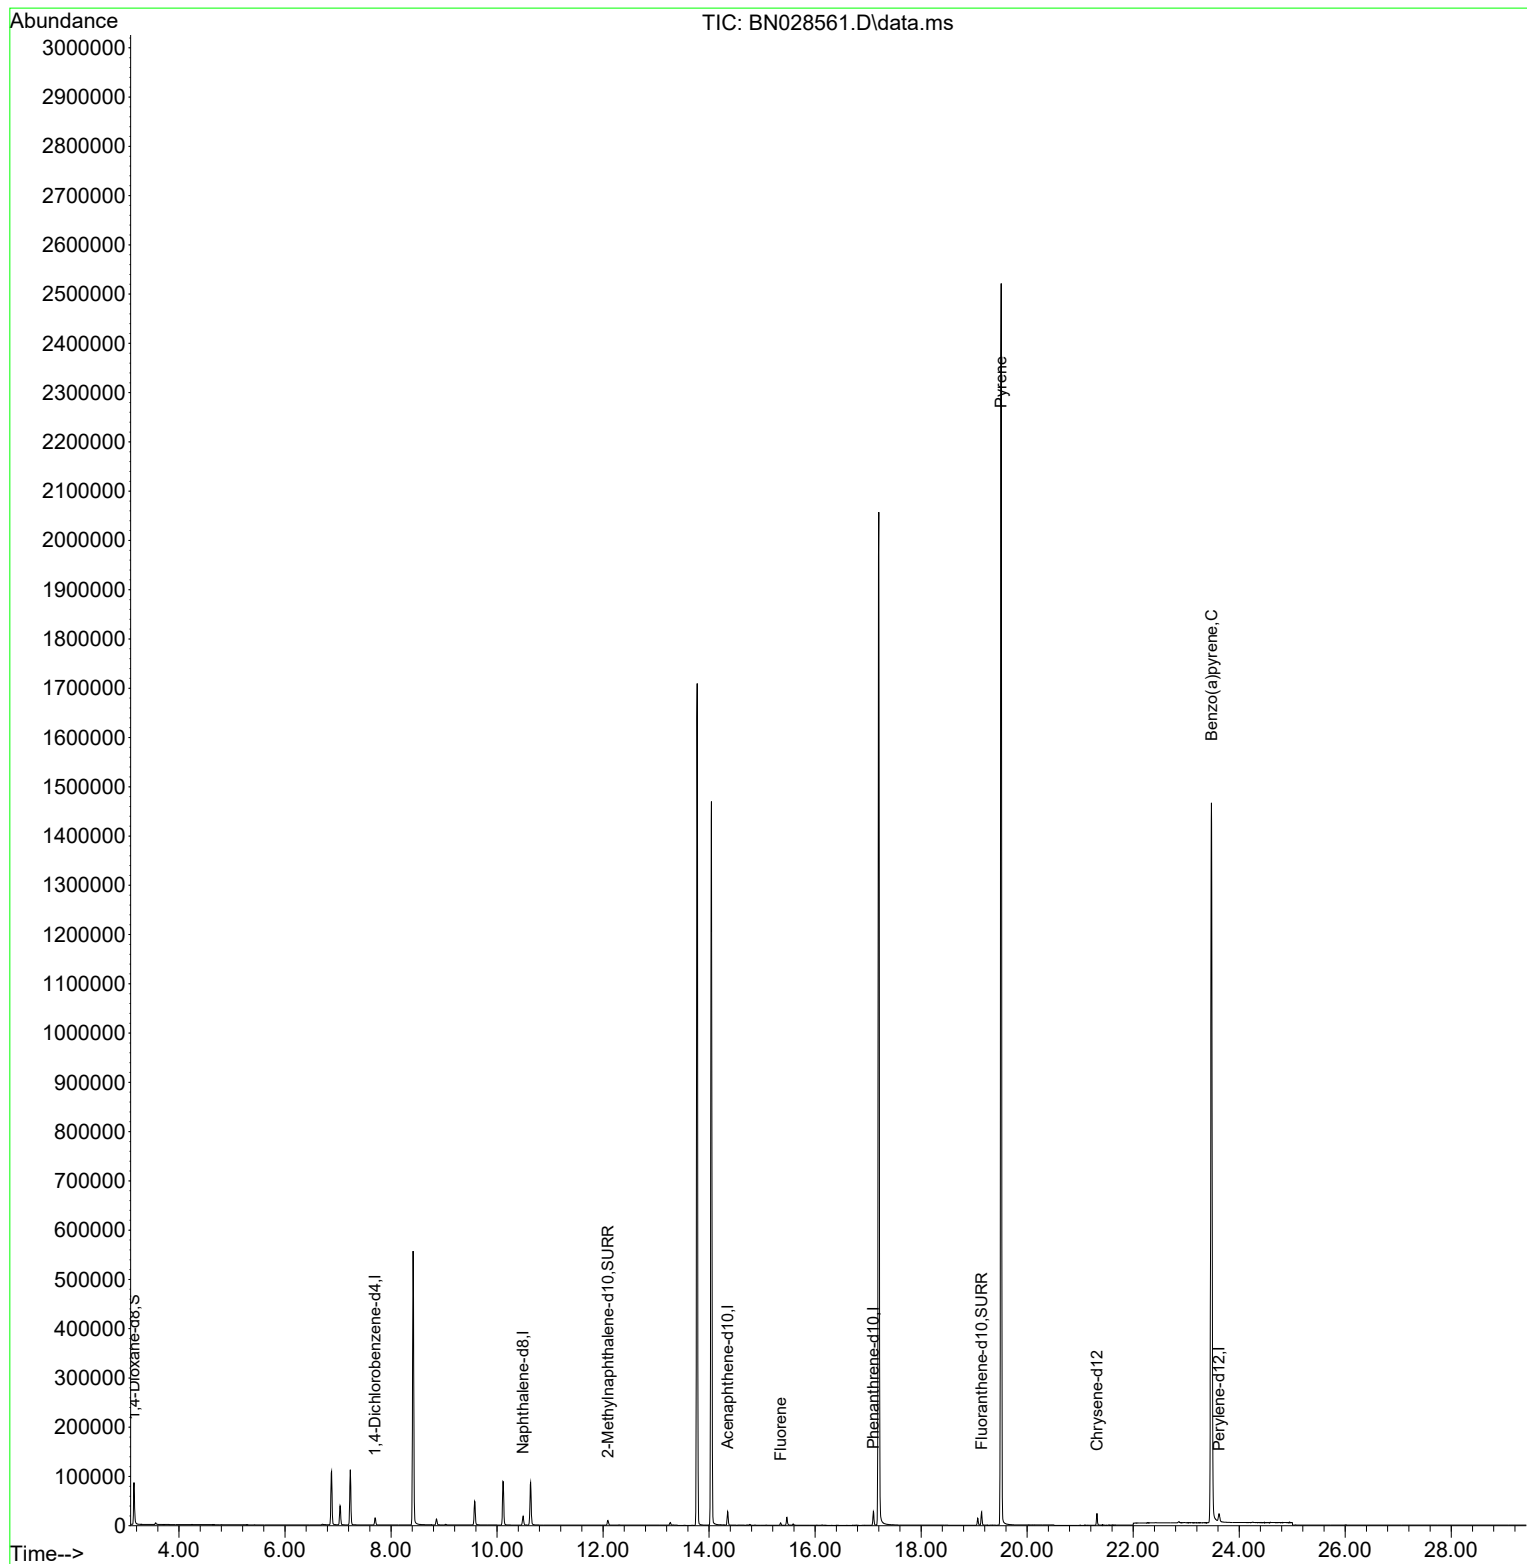


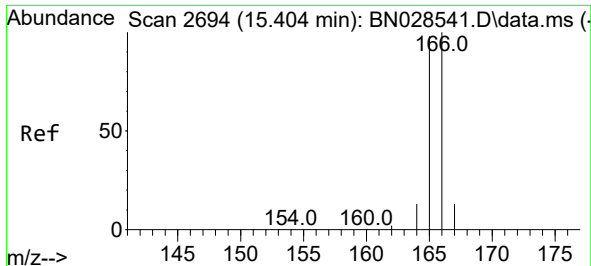

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.348 min Scan# 20
Delta R.T. -0.059 min
Lab File: BN028561.D
Acq: 10 Nov 2023 17:21




Instrument :
BNA_N
ClientSampleId :
SBLK717


Tgt Ion:166 Resp: 4241
Ion Ratio Lower Upper
166 100
165 7.5 78.6 118.0#
167 32.5 11.0 16.6#

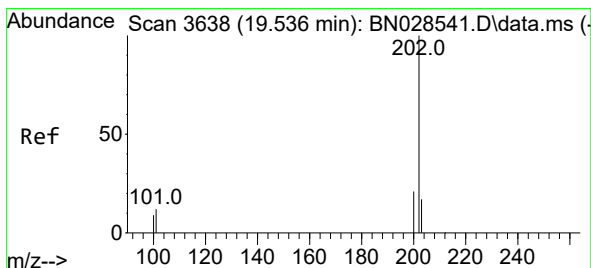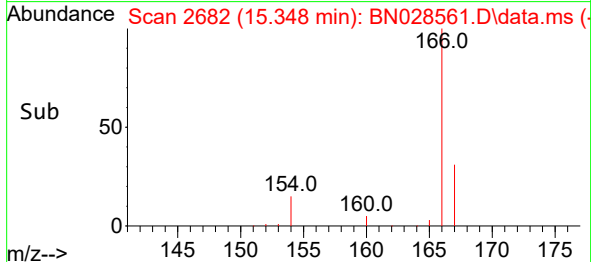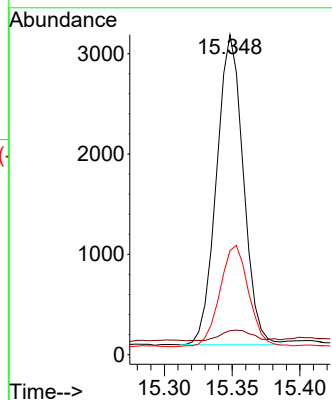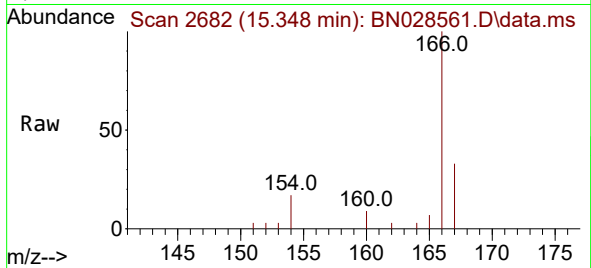

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.508 min Scan# 3632
Delta R.T. -0.031 min
Lab File: BN028561.D
Acq: 10 Nov 2023 17:21


Tgt Ion:202 Resp: 3800
Ion Ratio Lower Upper
202 100
101 138.0 10.3 15.5#
100 1003.6 8.2 12.2#

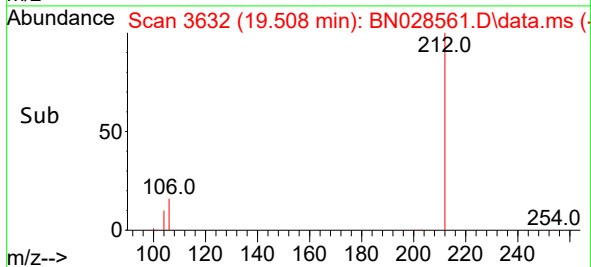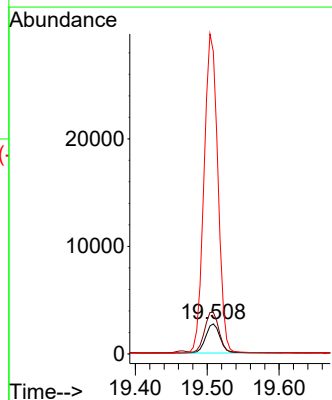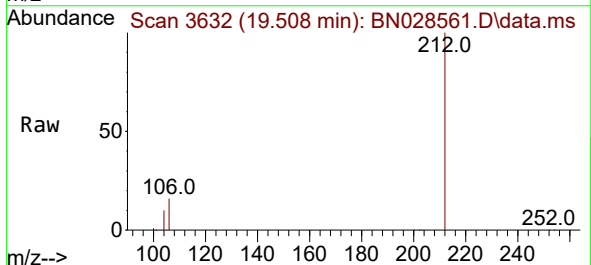

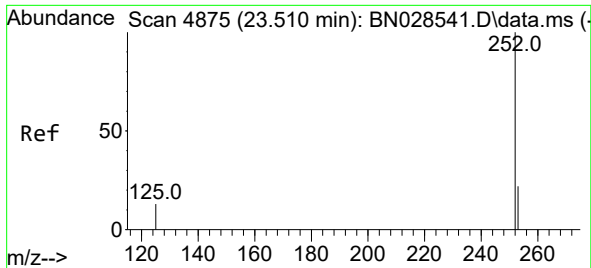

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.477 min Scan# 41
Delta R.T. -0.048 min
Lab File: BN028561.D
Acq: 10 Nov 2023 17:21

Instrument :
BNA_N
ClientSampleId :
SBLK717

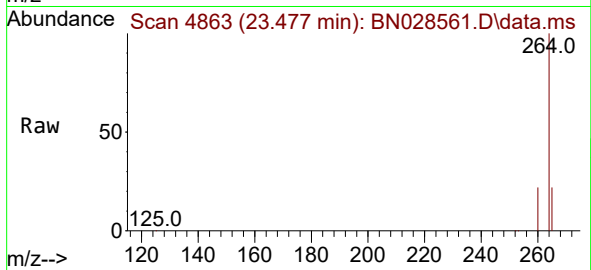

Tgt Ion:252 Resp: 7119
Ion Ratio Lower Upper
252 100
253 42.7 19.0 28.6#
125 38.5 13.2 19.8#

