




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028549.D
 Acq On : 10 Nov 2023 10:10
 Operator : MA/JU
 Sample : 05044-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHEE0

Manual IntegrationsAPPROVED

Quant Time: Nov 10 23:26:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/11/2023

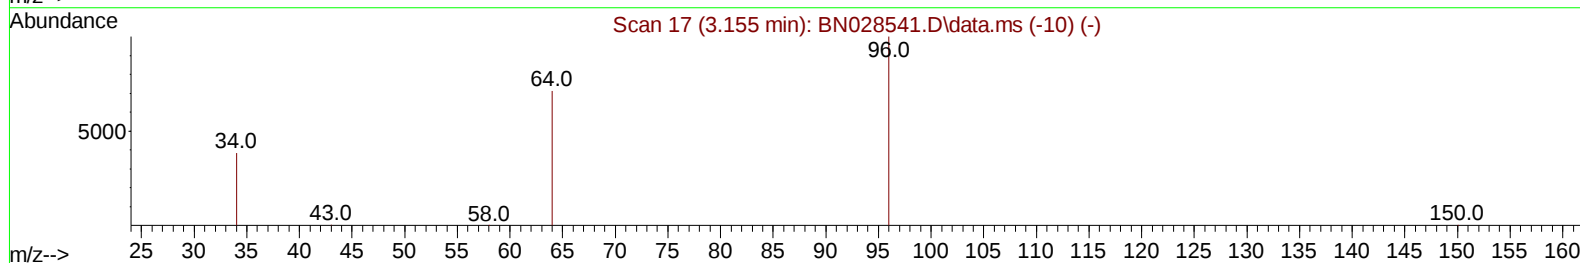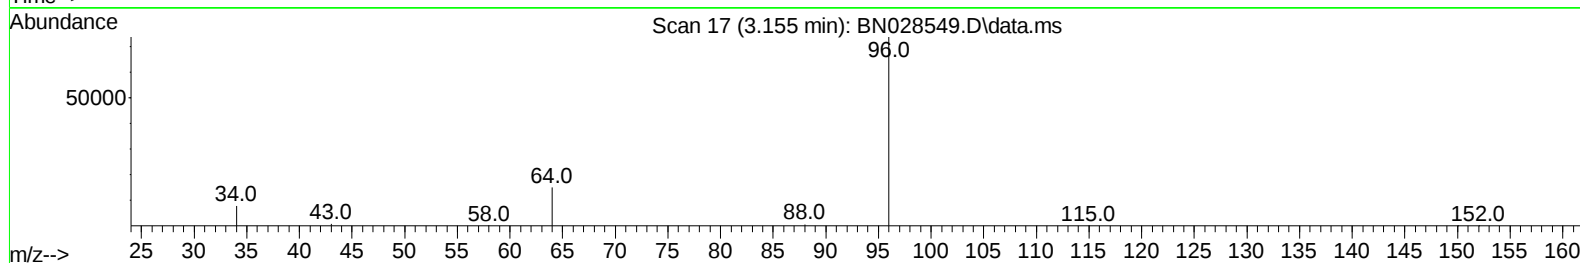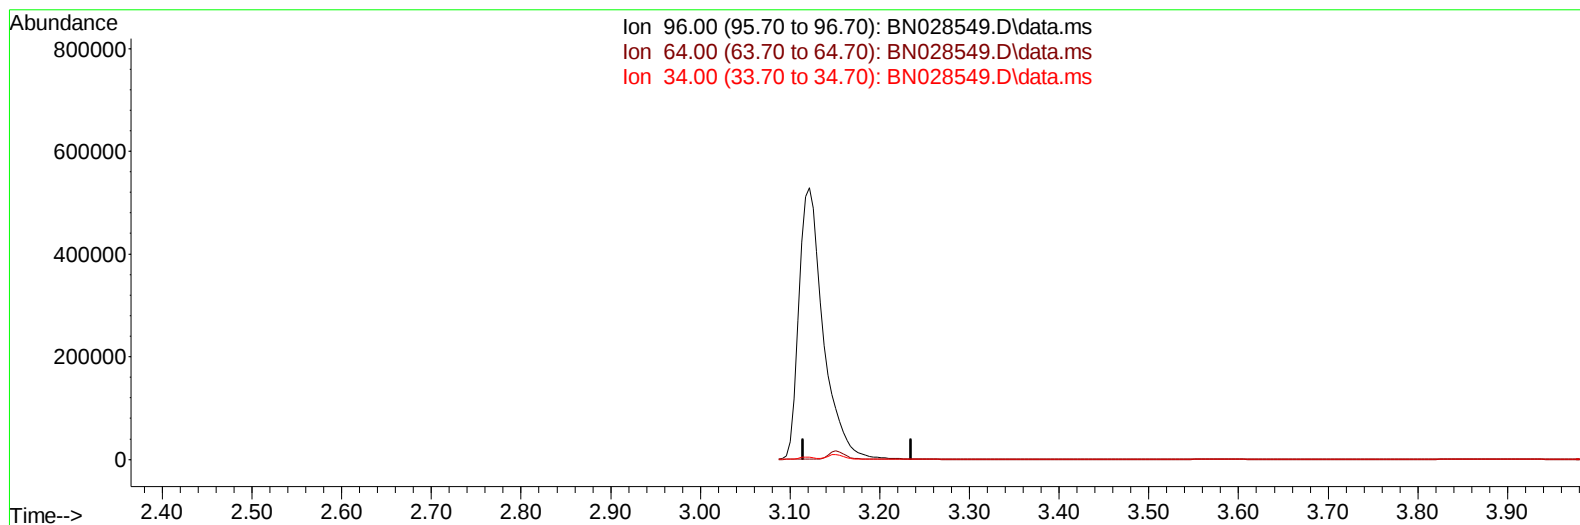

TIC: BN028549.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.155min (-3.155) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	67.40	0.00#
34.00	38.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028549.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : 05044-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHEE0

Manual IntegrationsAPPROVED

Quant Time: Nov 10 23:26:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/11/2023

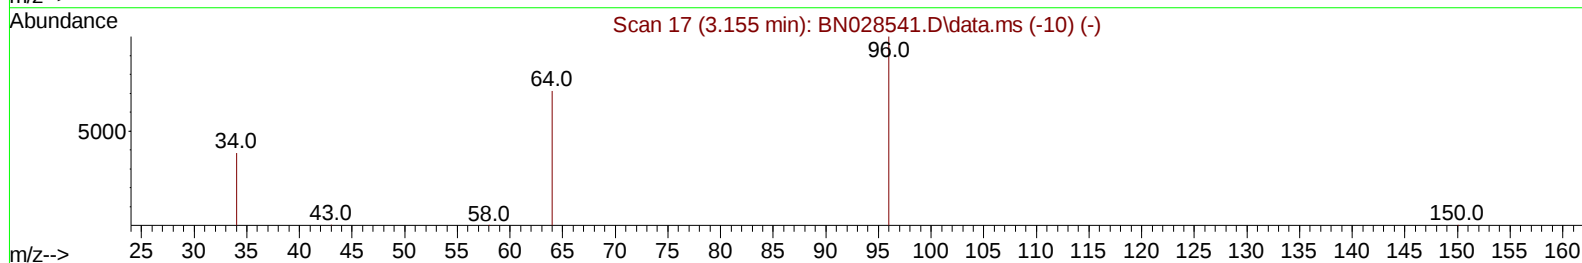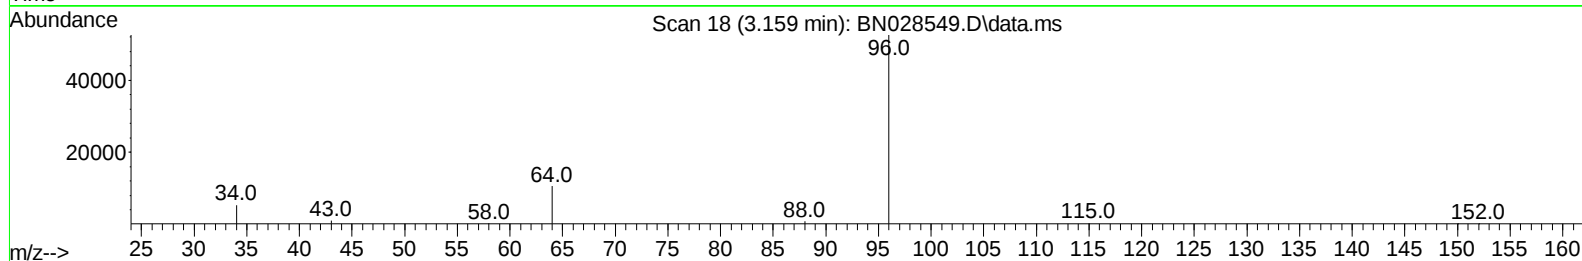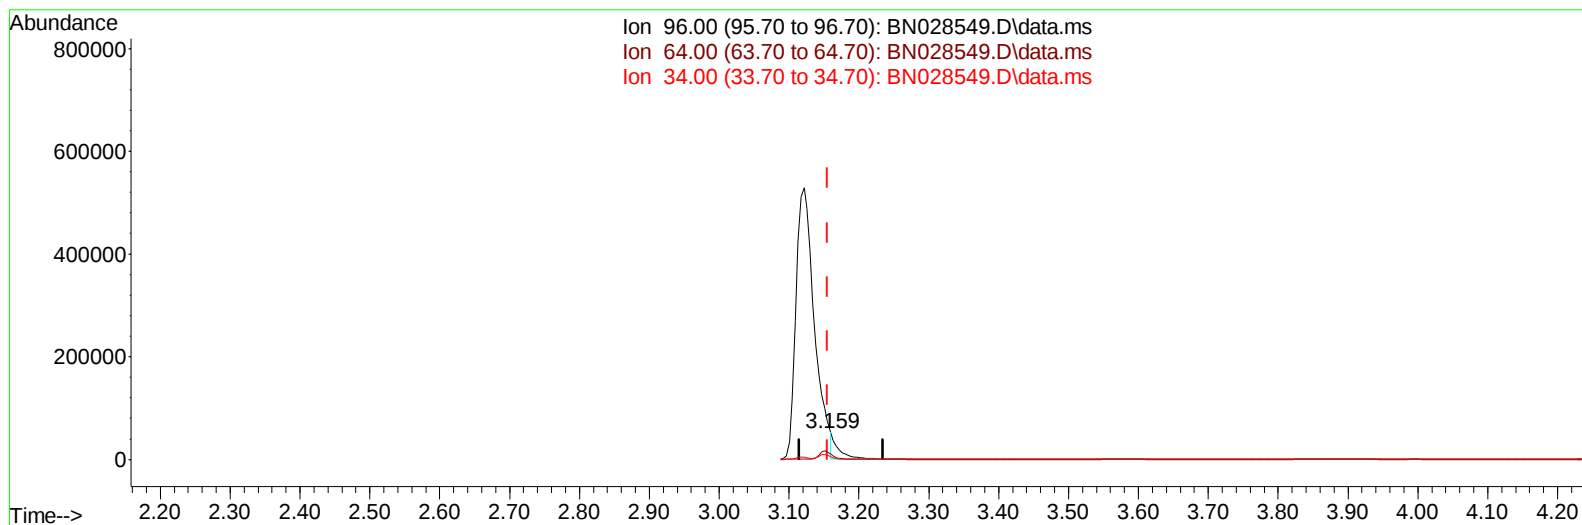

TIC: BN028549.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.159min (+ 0.004) 3.91 ng/ul m

response 33922

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.40	20.08#
34.00	38.60	10.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028549.D
 Acq On : 10 Nov 2023 10:10
 Operator : MA/JU
 Sample : 05044-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHEE0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/11/2023

Quant Time: Nov 10 23:26:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.703	152		7852	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136		26771	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.349	164		17958	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.099	188		37697	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.315	240		28945	0.400	ng/ul	0.00
23) Perylene-d12	23.618	264		29441	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.159	96		33922m	3.909	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152		14025	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.141	212		43560	0.468	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.189	88		7372	0.769	ng/ul#	79
5) Naphthalene	10.546	128		3040	0.041	ng/ul#	22

(#) = qualifier out of range (m) = manual integration (+) = signals summed

