

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028527.D
 Acq On : 09 Nov 2023 20:21
 Operator : MA/JU
 Sample : 05082-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH358

Quant Time: Nov 09 23:45:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8237	0.400	ng/ul	0.00
4) Naphthalene-d8	10.496	136	28453	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.354	164	17112	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.103	188	36484	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.317	240	25972	0.400	ng/ul	0.00
23) Perylene-d12	23.620	264	23163	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	46683	5.128	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.096	152	13451	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	33889	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	3617	0.359	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028527.D
Acq On : 09 Nov 2023 20:21
Operator : MA/JU
Sample : 05082-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH358

Quant Time: Nov 09 23:45:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

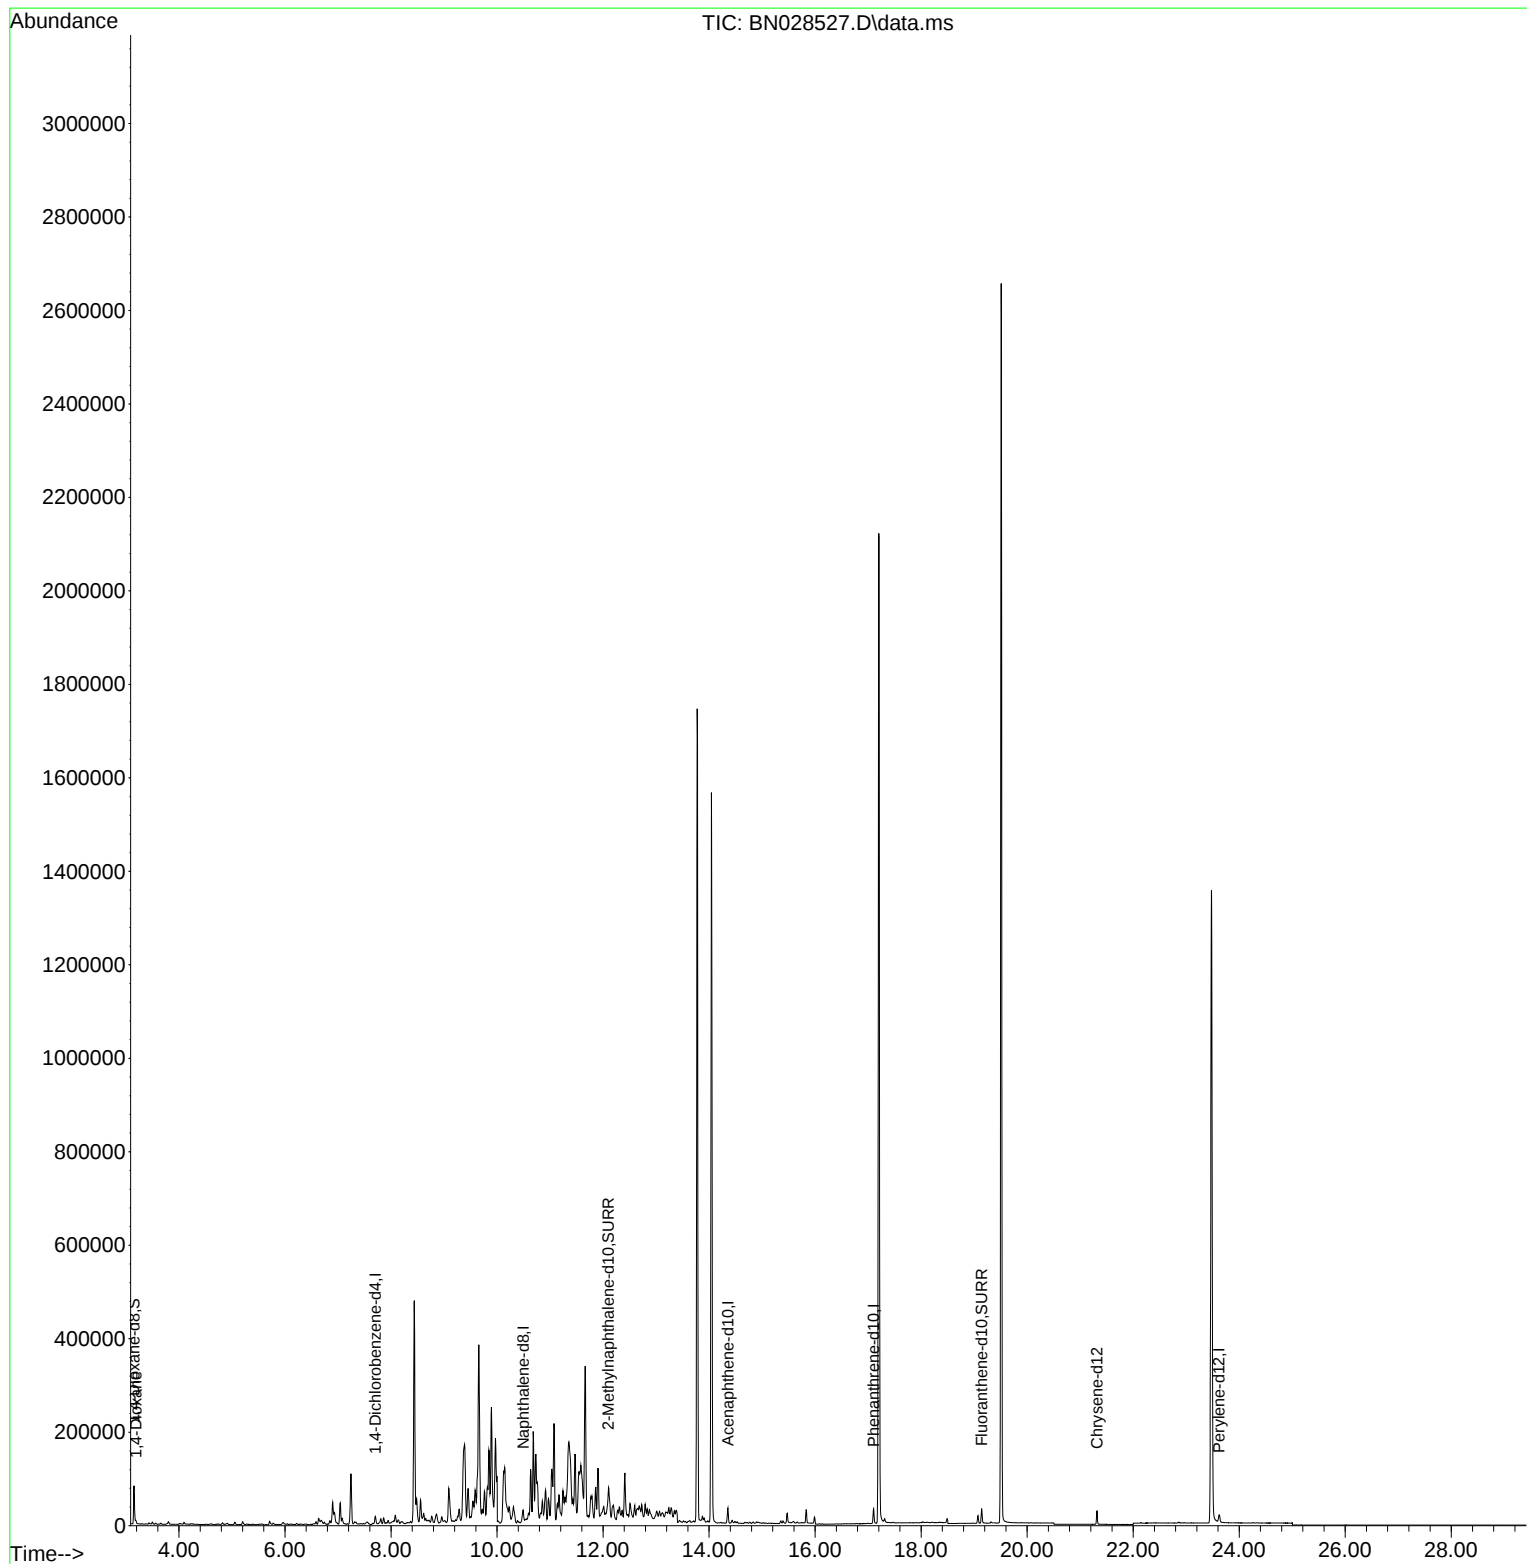

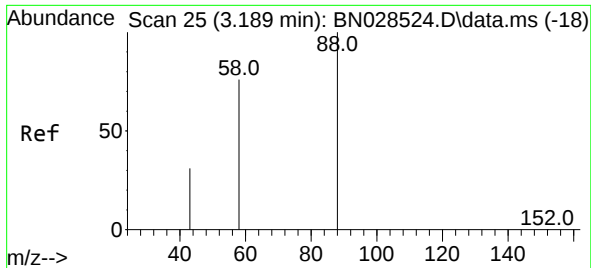

#2
 1,4-Dioxane
 Concen: 0.359 ng/ul
 RT: 3.189 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN028527.D
 Acq: 09 Nov 2023 20:21

Instrument :
 BNA_N
 ClientSampleId :
 BH358

Tgt Ion: 88 Resp: 3617
 Ion Ratio Lower Upper
 88 100
 43 61.5 32.9 49.3#
 58 58.3 41.8 62.8

