

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028531.D
 Acq On : 09 Nov 2023 22:45
 Operator : MA/JU
 Sample : 05082-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH356

Quant Time: Nov 09 23:45:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8081	0.400	ng/ul	0.00
4) Naphthalene-d8	10.496	136	27926	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.353	164	18356	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.103	188	40669	0.400	ng/ul	0.00
17) Chrysene-d12	21.316	240	31736	0.400	ng/ul	0.00
23) Perylene-d12	23.619	264	33344	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.150	96	37962	4.250	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	15909	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	49816	0.488	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.188	88	24656	2.498	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028531.D
Acq On : 09 Nov 2023 22:45
Operator : MA/JU
Sample : 05082-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH356


Quant Time: Nov 09 23:45:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

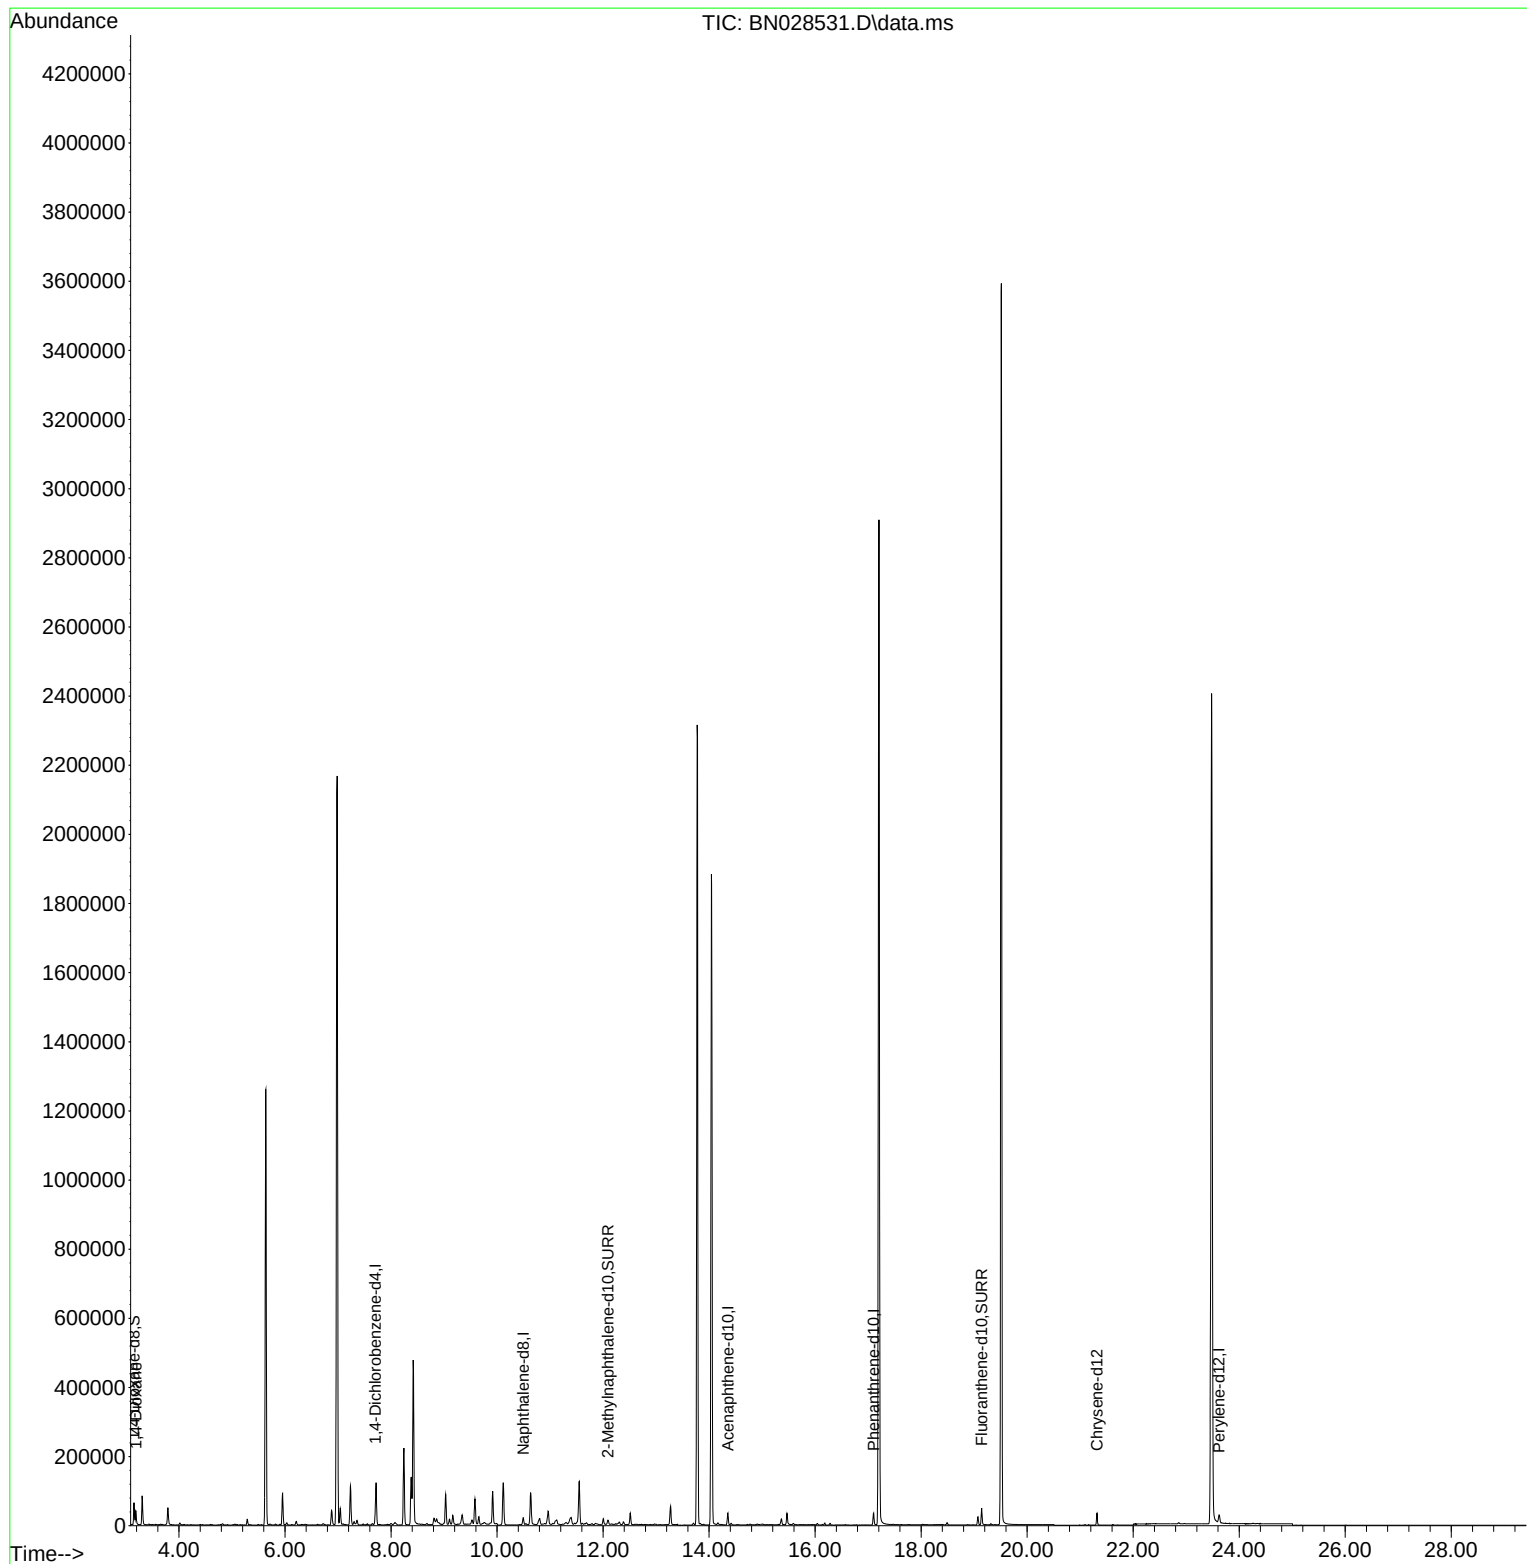

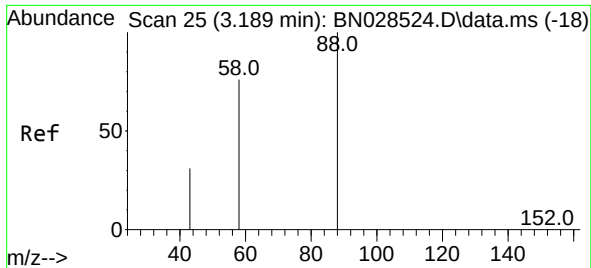

#2
 1,4-Dioxane
 Concen: 2.498 ng/ul
 RT: 3.188 min Scan# 21
 Delta R.T. -0.001 min
 Lab File: BN028531.D
 Acq: 09 Nov 2023 22:45

Instrument :
 BNA_N
 ClientSampleId :
 BH356

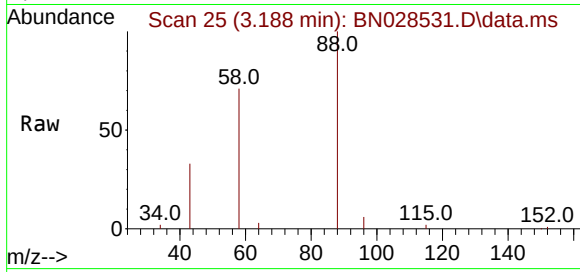

Tgt Ion:	88	Resp:	24656
Ion	Ratio	Lower	Upper
88	100		
43	33.1	32.9	49.3
58	71.4	41.8	62.8#

