

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028534.D
 Acq On : 10 Nov 2023 00:33
 Operator : MA/JU
 Sample : 05082-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH354

Quant Time: Nov 10 01:00:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8440	0.400	ng/ul	0.00
4) Naphthalene-d8	10.496	136	28547	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.354	164	18345	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.103	188	38959	0.400	ng/ul	0.00
17) Chrysene-d12	21.314	240	25717	0.400	ng/ul	0.00
23) Perylene-d12	23.617	264	25728	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	46080	4.940	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	19458	0.453	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	52497	0.634	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	310174	30.083	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028534.D
Acq On : 10 Nov 2023 00:33
Operator : MA/JU
Sample : 05082-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH354


Quant Time: Nov 10 01:00:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

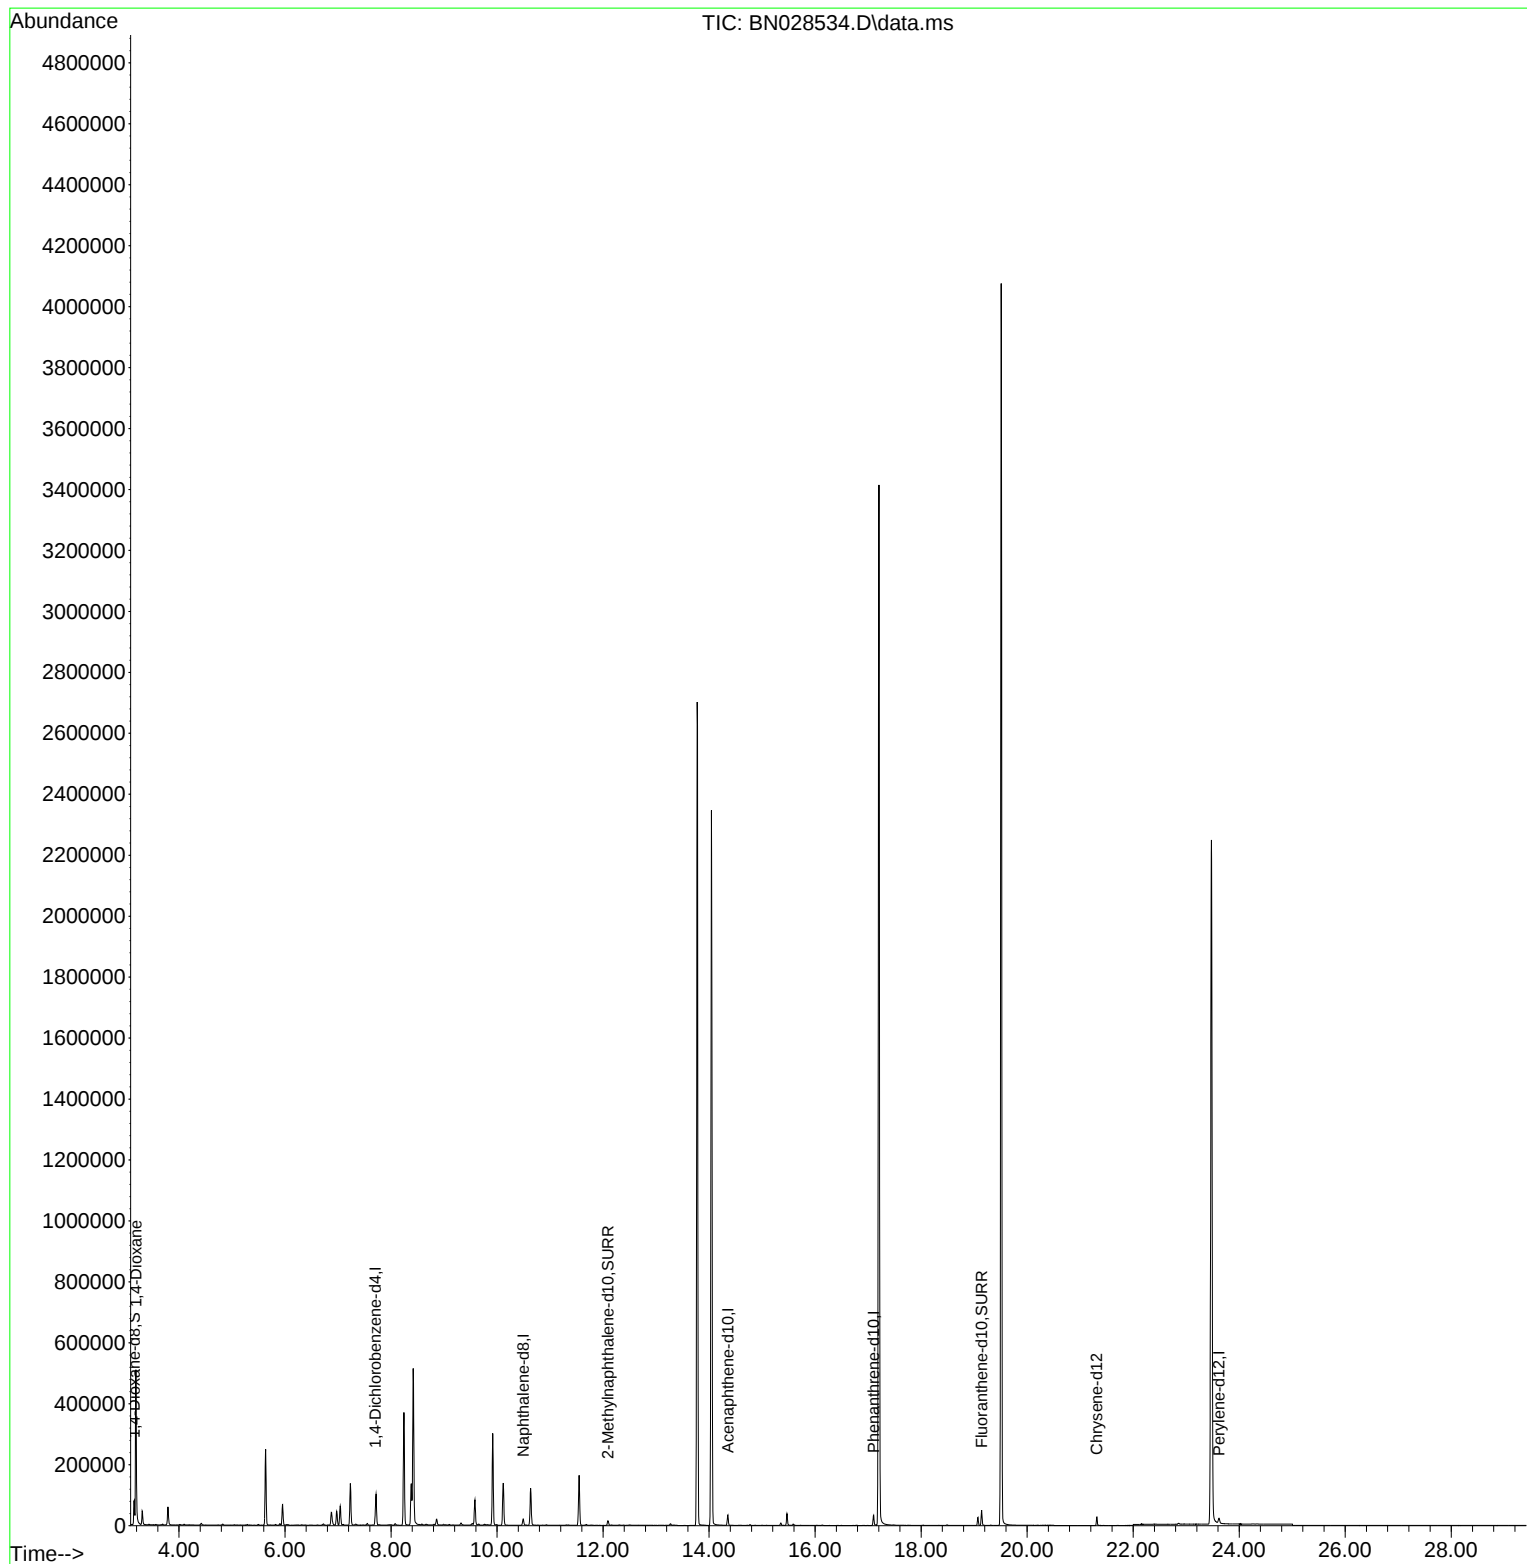

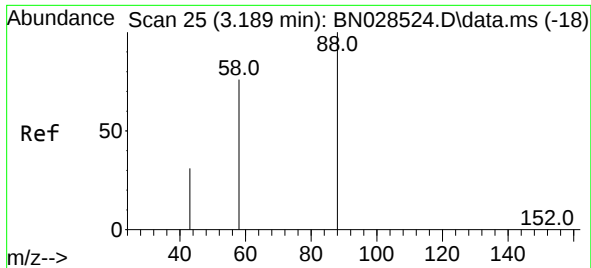

#2
 1,4-Dioxane
 Concen: 30.083 ng/ul
 RT: 3.189 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN028534.D
 Acq: 10 Nov 2023 00:33

Instrument :
 BNA_N
 ClientSampleId :
 BH354

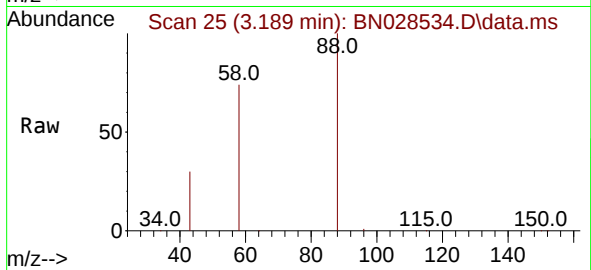

Tgt Ion: 88 Resp: 310174

Ion	Ratio	Lower	Upper
88	100		
43	29.6	32.9	49.3#
58	73.9	41.8	62.8#

