

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028537.D
 Acq On : 10 Nov 2023 02:21
 Operator : MA/JU
 Sample : 05082-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH323

Quant Time: Nov 10 02:53:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8758	0.400	ng/ul	0.00
4) Naphthalene-d8	10.495	136	29593	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.352	164	18580	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.102	188	40586	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	31030	0.400	ng/ul	0.00
23) Perylene-d12	23.615	264	30774	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	41029	4.239	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.090	152	15925	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.140	212	44001	0.441	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.184	88	72236	6.752	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028537.D
Acq On : 10 Nov 2023 02:21
Operator : MA/JU
Sample : 05082-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH323


Quant Time: Nov 10 02:53:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

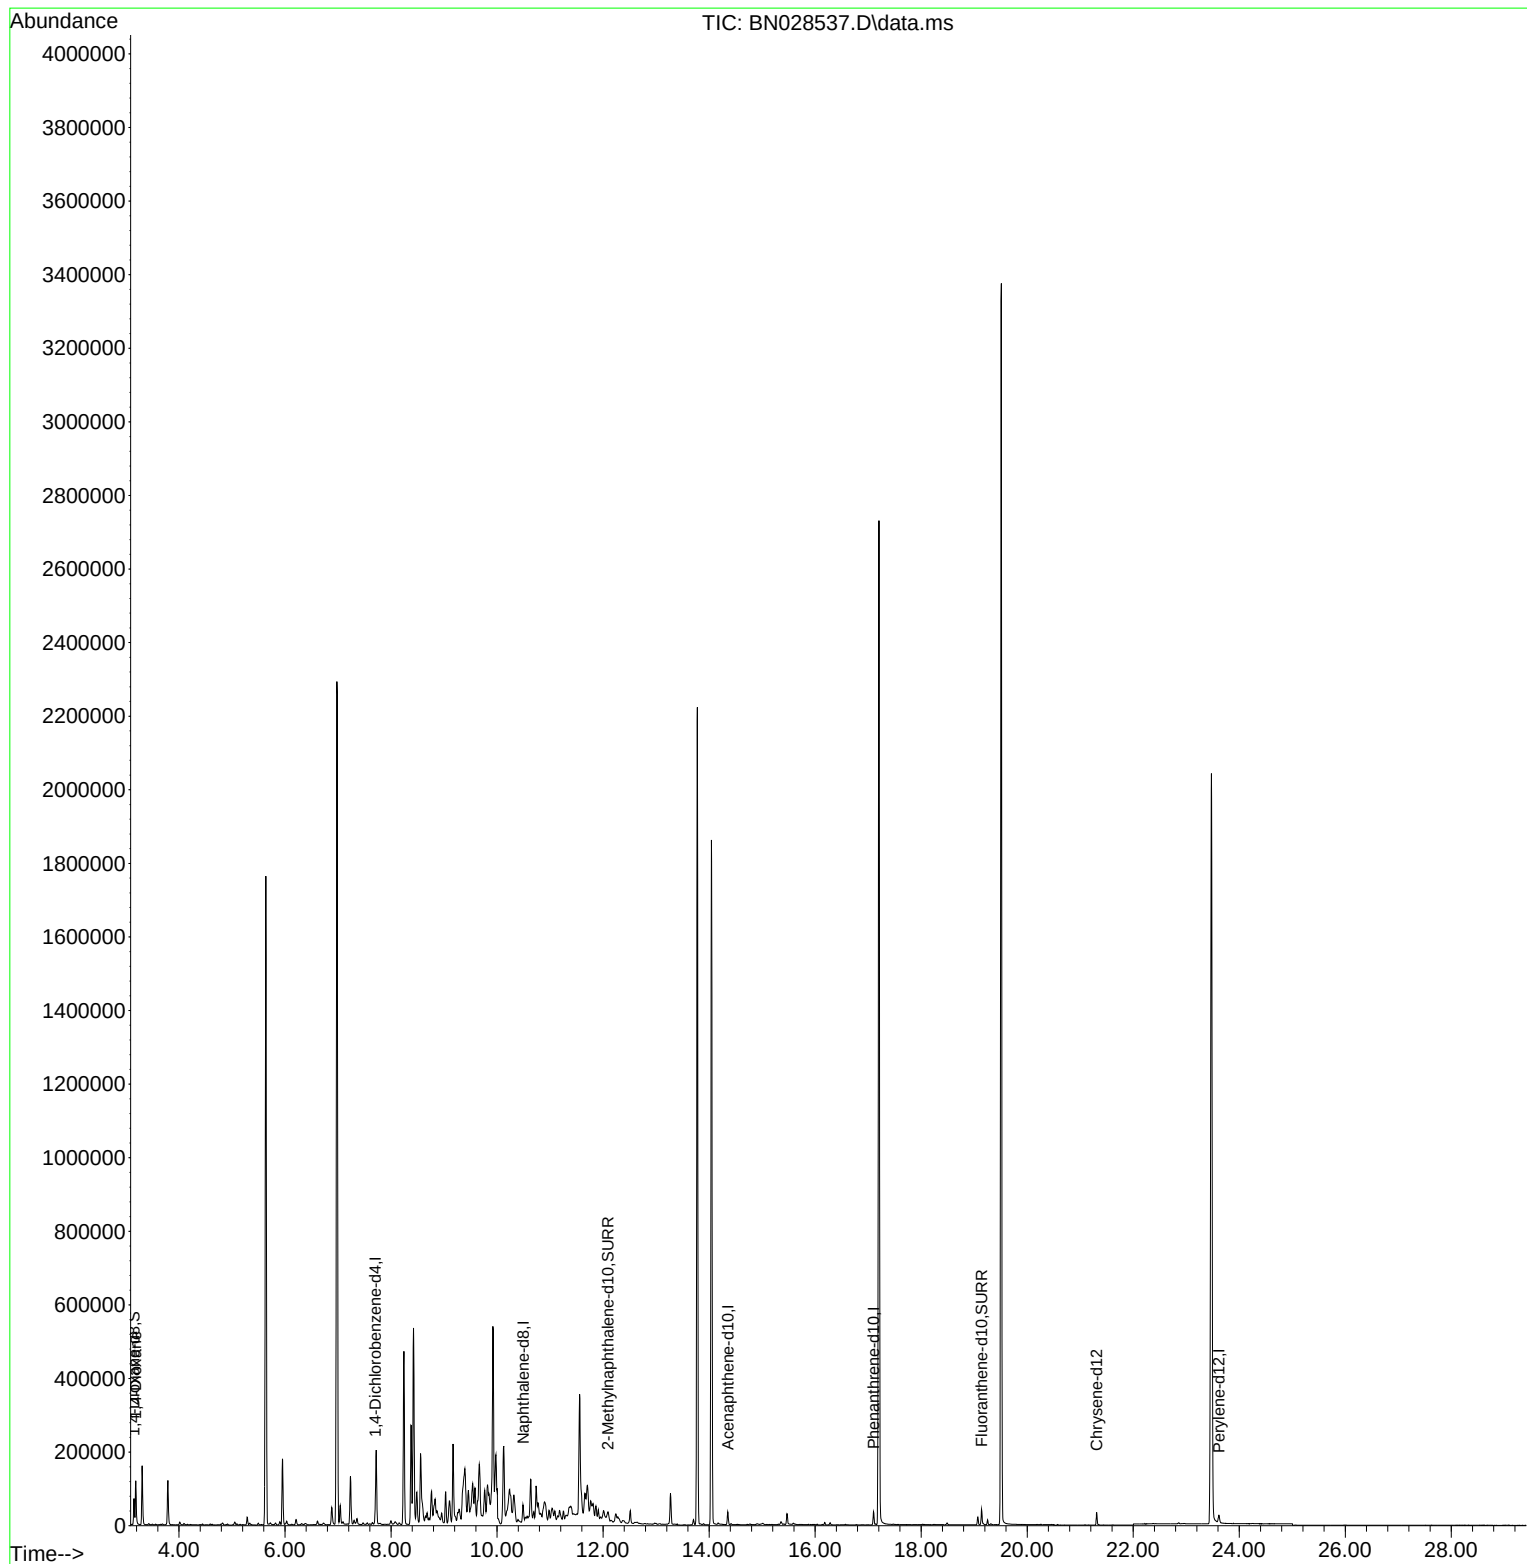

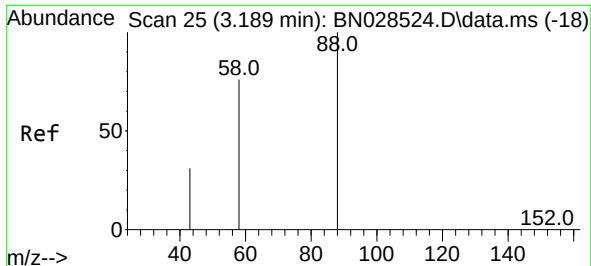

#2
 1,4-Dioxane
 Concen: 6.752 ng/ul
 RT: 3.184 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BN028537.D
 Acq: 10 Nov 2023 02:21

Instrument :
 BNA_N
 ClientSampleId :
 BH323

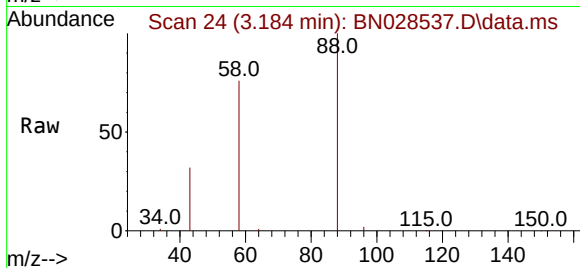

Tgt Ion: 88 Resp: 72236
 Ion Ratio Lower Upper
 88 100
 43 32.3 32.9 49.3#
 58 76.1 41.8 62.8#

