

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028539.D
 Acq On : 10 Nov 2023 03:33
 Operator : MA/JU
 Sample : 05082-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH330

Quant Time: Nov 10 04:05:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	9202	0.400	ng/ul	0.00
4) Naphthalene-d8	10.496	136	31380	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.354	164	19112	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.103	188	42003	0.400	ng/ul	0.00
17) Chrysene-d12	21.311	240	31198	0.400	ng/ul	0.00
23) Perylene-d12	23.614	264	30871	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.155	96	43304	4.258	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	18268	0.387	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	52755	0.525	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	20060	1.784	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028539.D
Acq On : 10 Nov 2023 03:33
Operator : MA/JU
Sample : 05082-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH330


Quant Time: Nov 10 04:05:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

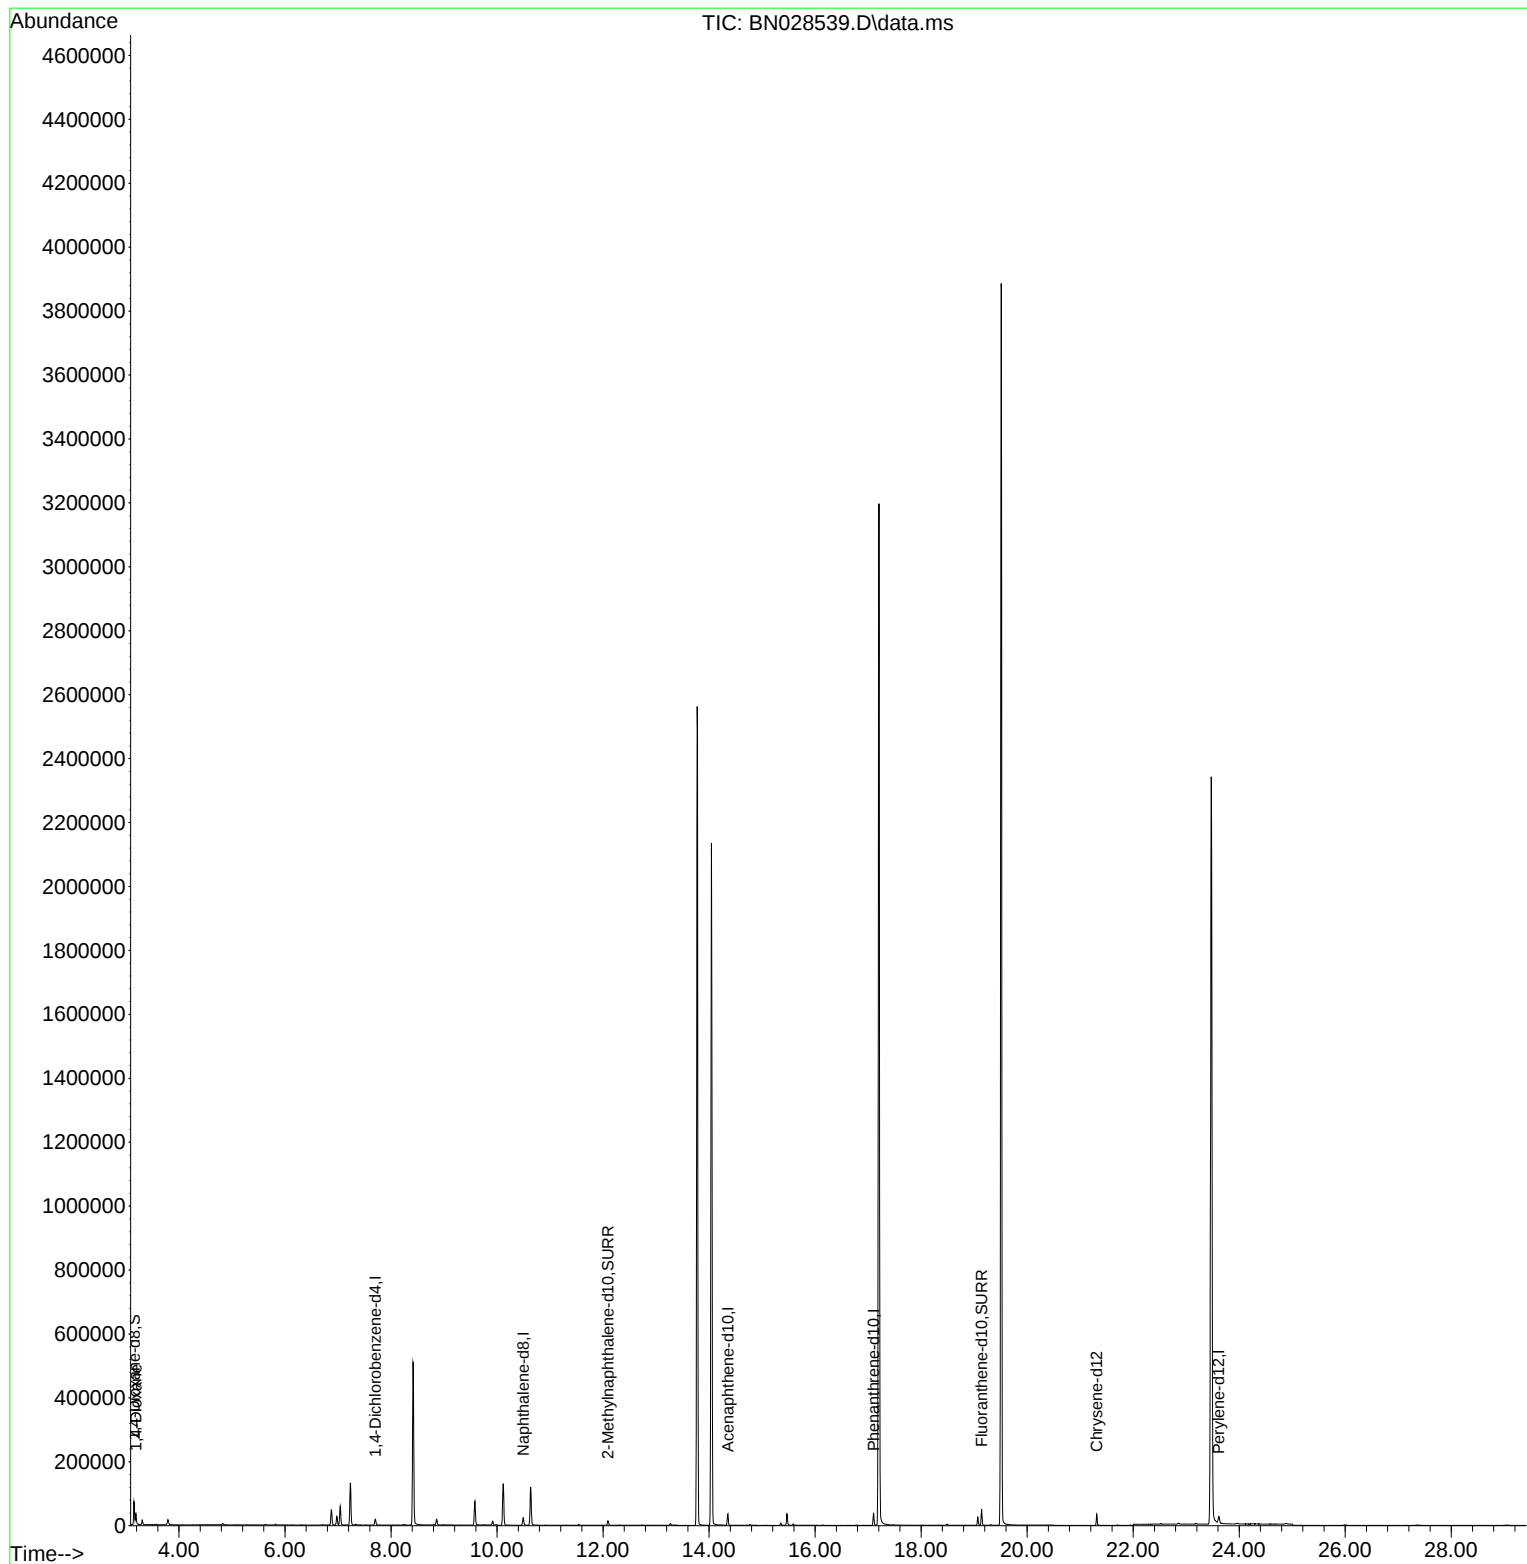

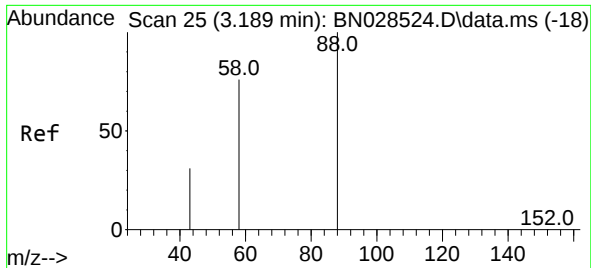

#2
 1,4-Dioxane
 Concen: 1.784 ng/ul
 RT: 3.189 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN028539.D
 Acq: 10 Nov 2023 03:33

Instrument :
 BNA_N
 ClientSampleId :
 BH330

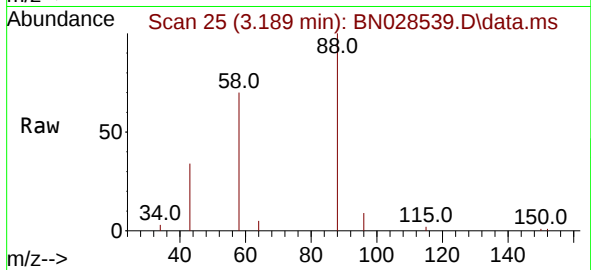

Tgt Ion: 88 Resp: 20060
 Ion Ratio Lower Upper
 88 100
 43 33.6 32.9 49.3
 58 69.9 41.8 62.8#

