

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028544.D
 Acq On : 10 Nov 2023 07:09
 Operator : MA/JU
 Sample : 05082-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH332

Quant Time: Nov 10 07:40:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	7457	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	25238	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.350	164	15672	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.100	188	35442	0.400	ng/ul	0.00
17) Chrysene-d12	21.313	240	28129	0.400	ng/ul	0.00
23) Perylene-d12	23.616	264	31032	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	34744	4.216	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	14276	0.376	ng/ul	0.00
18) Fluoranthene-d10	19.137	212	40117	0.443	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.184	88	8211	0.901	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028544.D
Acq On : 10 Nov 2023 07:09
Operator : MA/JU
Sample : 05082-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH332


Quant Time: Nov 10 07:40:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

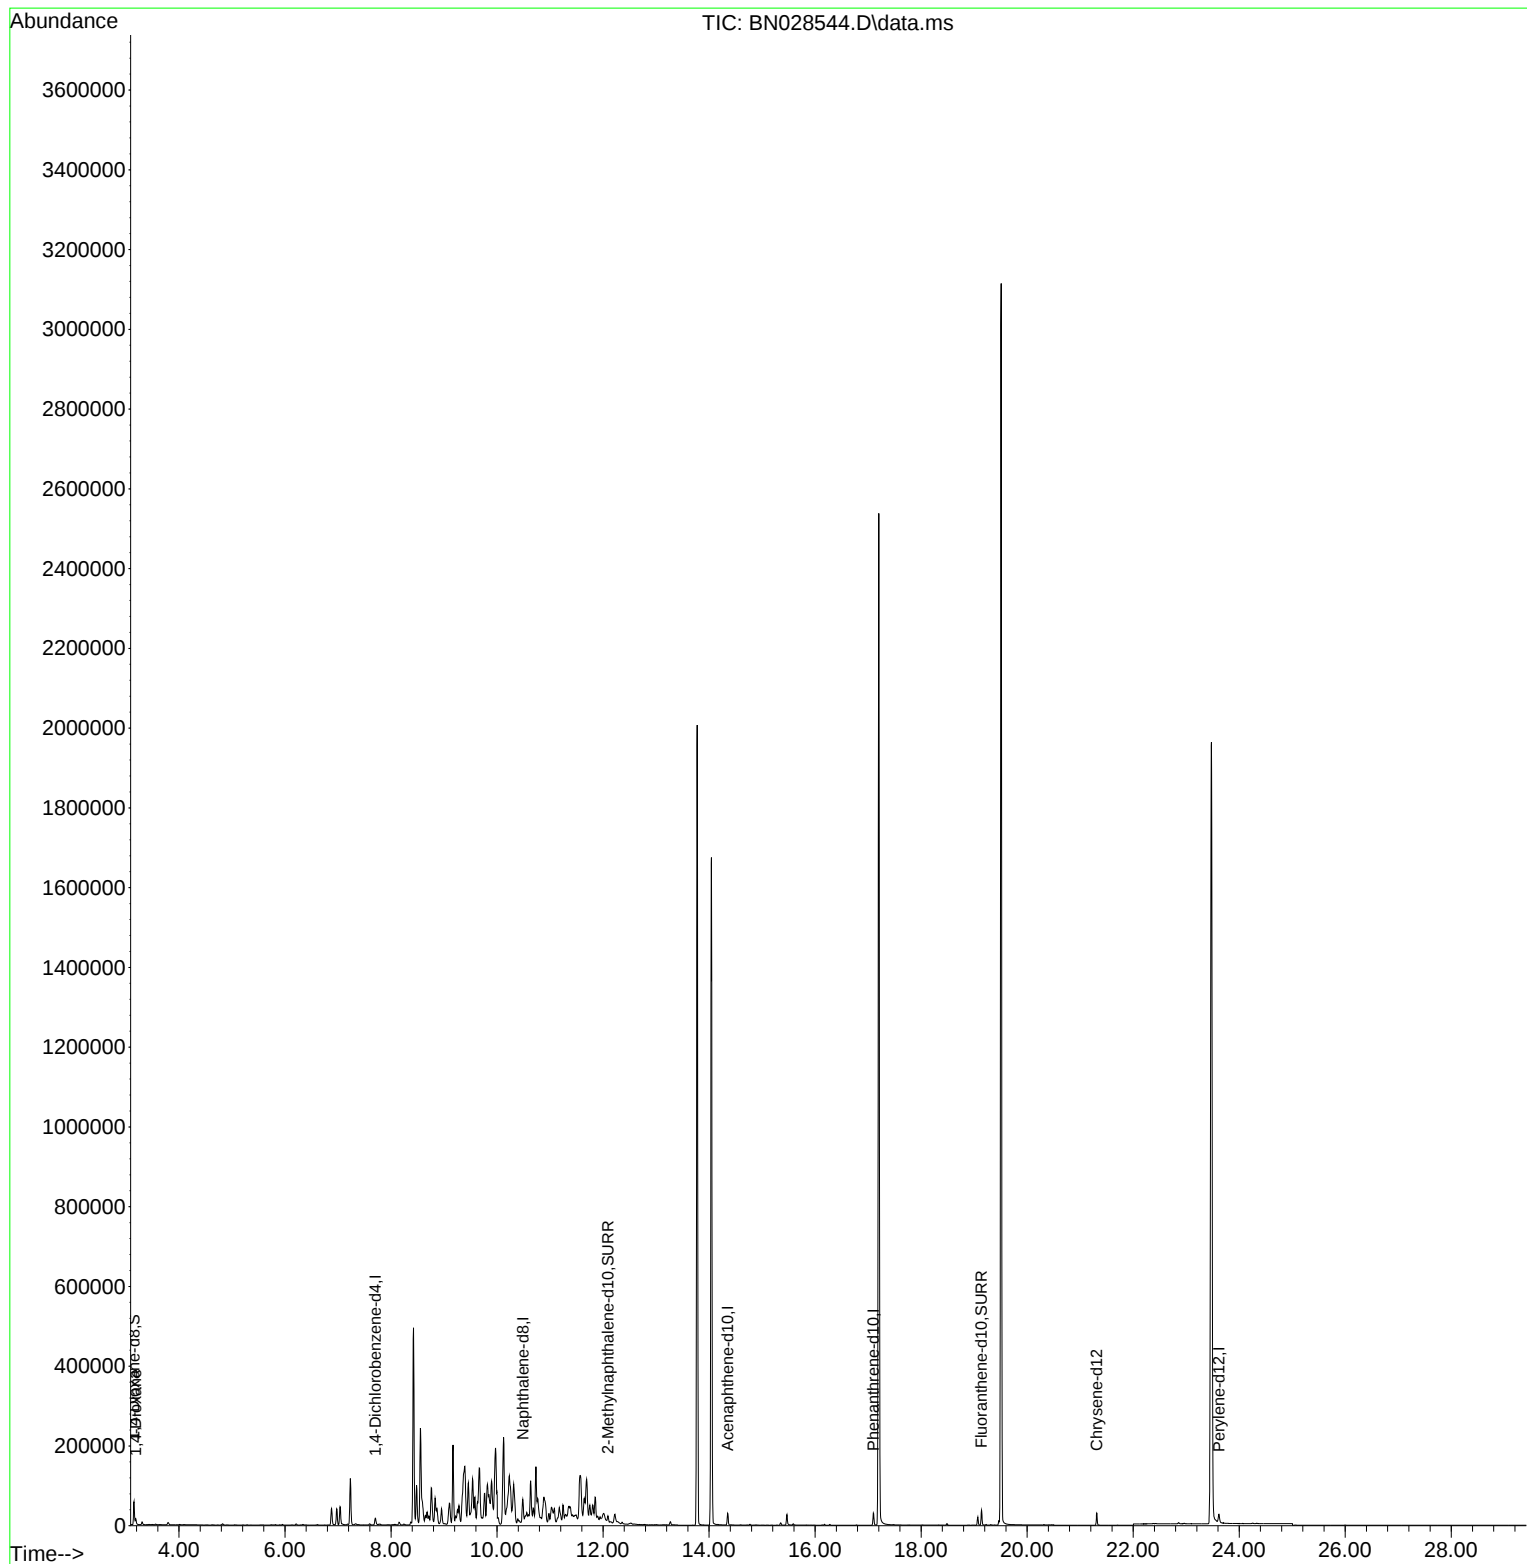

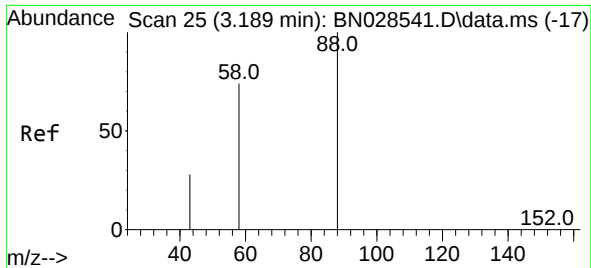

#2
 1,4-Dioxane
 Concen: 0.901 ng/ul
 RT: 3.184 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BN028544.D
 Acq: 10 Nov 2023 07:09

Instrument :
 BNA_N
 ClientSampleId :
 BH332

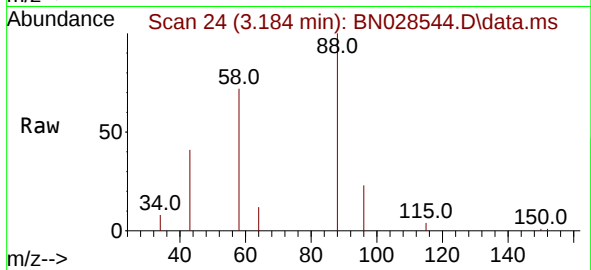

Tgt Ion:	88	Resp:	8211
Ion	Ratio	Lower	Upper
88	100		
43	41.0	32.9	49.3
58	71.6	41.8	62.8

