

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028548.D
 Acq On : 10 Nov 2023 09:33
 Operator : MA/JU
 Sample : 05044-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHEF8

Quant Time: Nov 10 23:26:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	7165	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	23997	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.349	164	14969	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.099	188	33748	0.400	ng/ul	0.00
17) Chrysene-d12	21.314	240	27079	0.400	ng/ul	0.00
23) Perylene-d12	23.617	264	28827	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	32839	4.147	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	11602	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.137	212	34243	0.393	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.184	88	2902	0.332	ng/ul#	85
15) Phenanthrene	17.141	178	3325	0.032	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028548.D
Acq On : 10 Nov 2023 09:33
Operator : MA/JU
Sample : 05044-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Nov 10 23:26:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration




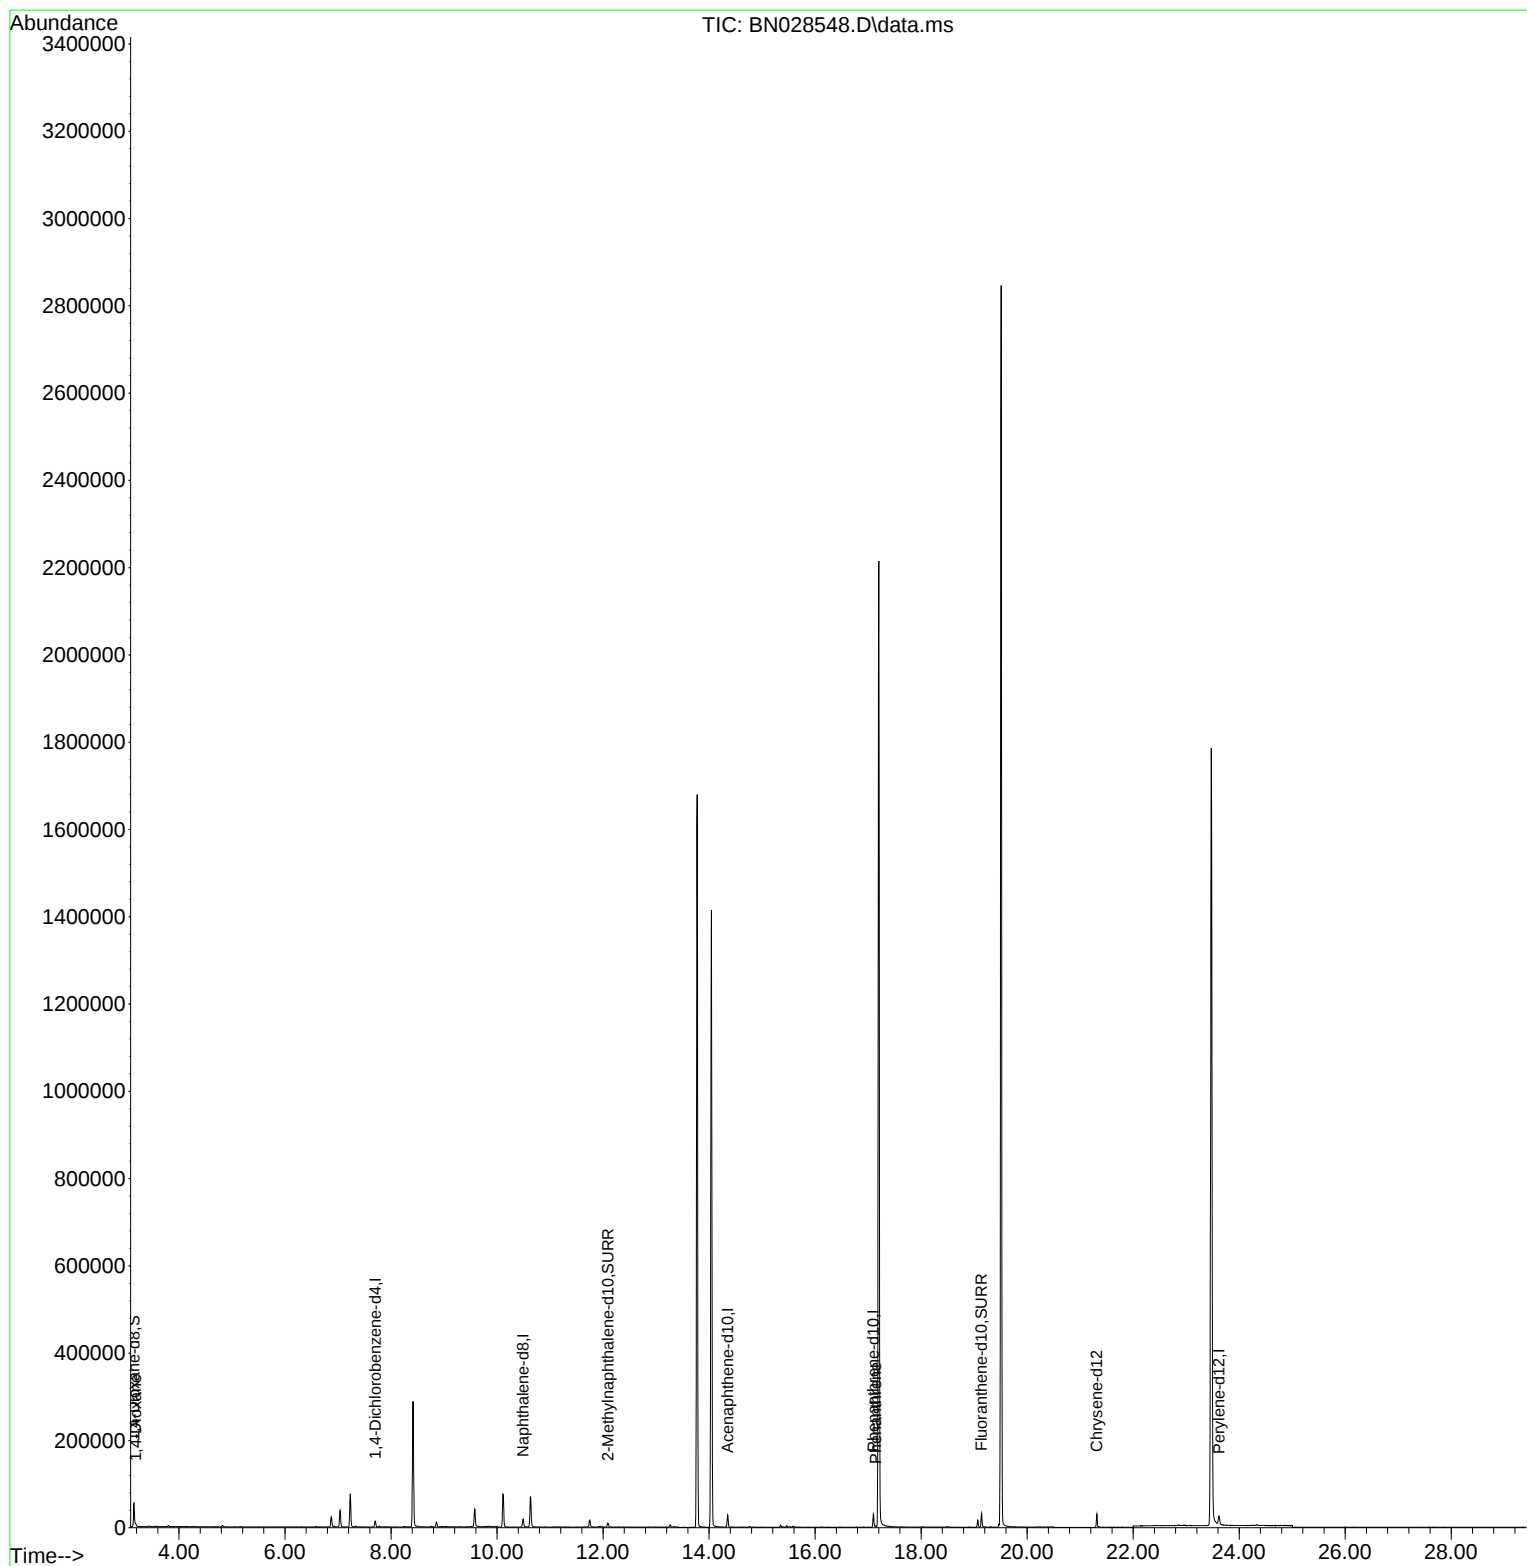


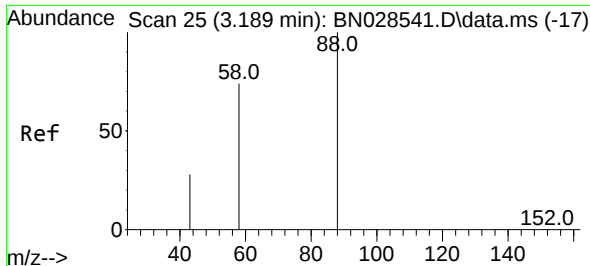

#2
 1,4-Dioxane
 Concen: 0.332 ng/ul
 RT: 3.184 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BN028548.D
 Acq: 10 Nov 2023 09:33

Instrument :
 BNA_N
 ClientSampleId :
 BHEF8

Tgt Ion: 88 Resp: 2902
 Ion Ratio Lower Upper
 88 100
 43 51.1 32.9 49.3#
 58 62.3 41.8 62.8

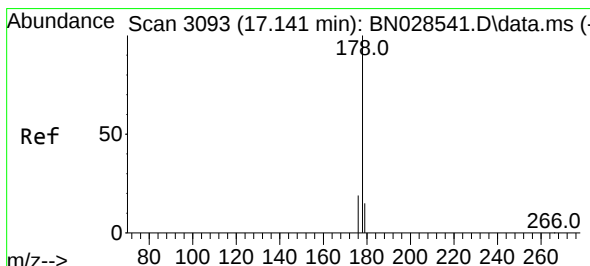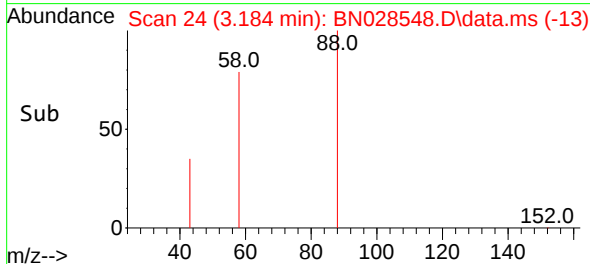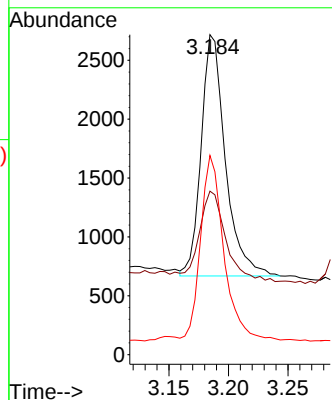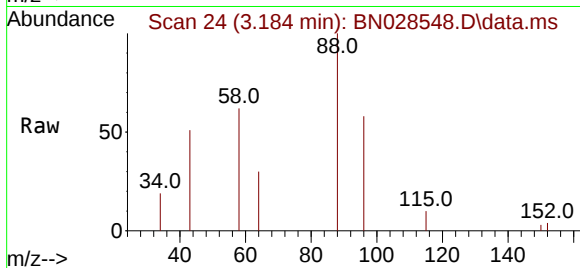

#15
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.141 min Scan# 3093
 Delta R.T. -0.003 min
 Lab File: BN028548.D
 Acq: 10 Nov 2023 09:33

Tgt Ion: 178 Resp: 3325
 Ion Ratio Lower Upper
 178 100
 179 22.0 12.4 18.6#
 176 23.1 15.4 23.2

