

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028557.D
 Acq On : 10 Nov 2023 14:57
 Operator : MA/JU
 Sample : 05082-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH321

Quant Time: Nov 10 23:27:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8074	0.400	ng/ul	0.00
4) Naphthalene-d8	10.489	136	27584	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.352	164	17960	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.102	188	40510	0.400	ng/ul	0.00
17) Chrysene-d12	21.315	240	30656	0.400	ng/ul	0.00
23) Perylene-d12	23.621	264	30879	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	32915	3.689	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.090	152	14773	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.140	212	48389	0.490	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	1252	0.127	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028557.D
Acq On : 10 Nov 2023 14:57
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH321

Quant Time: Nov 10 23:27:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

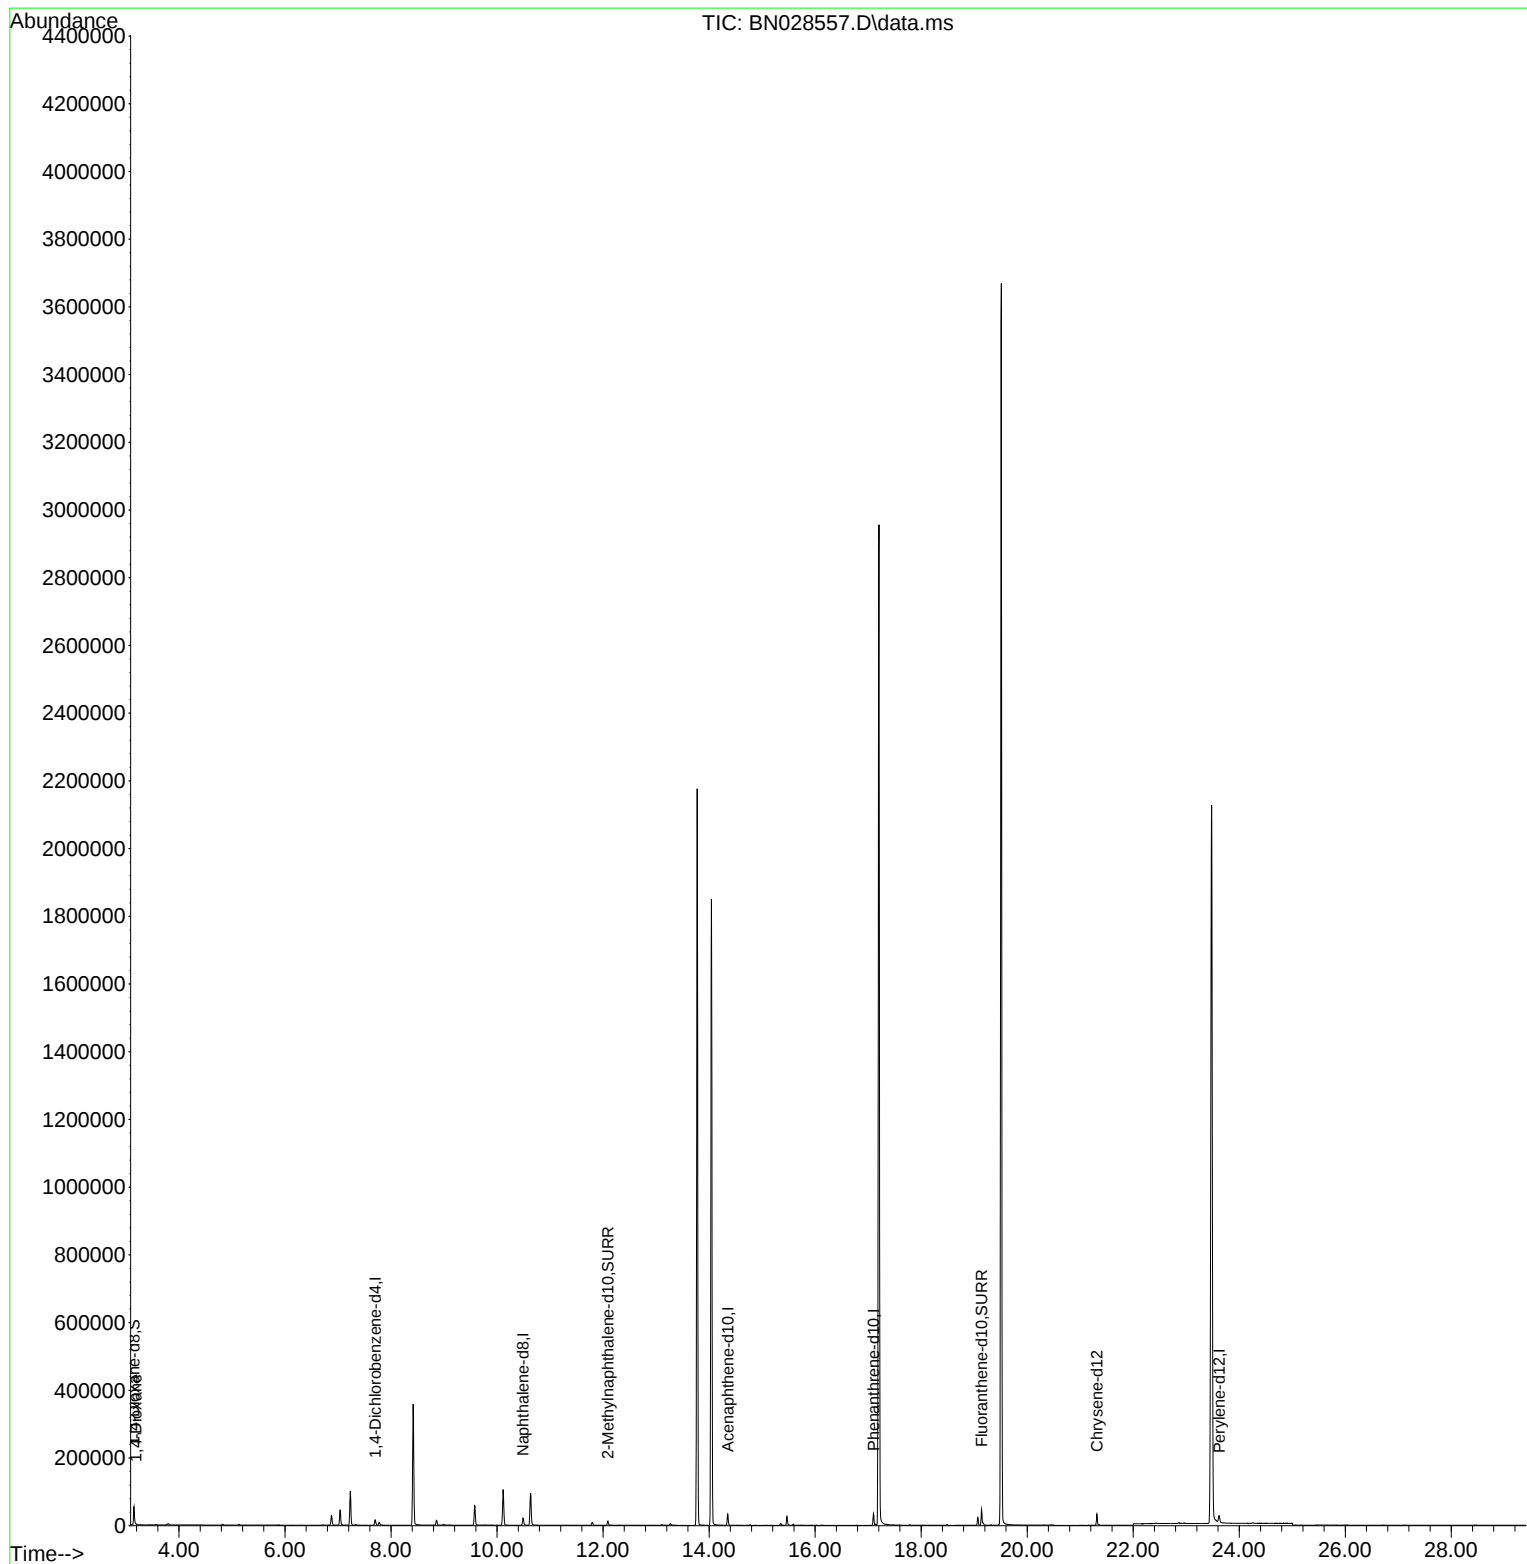

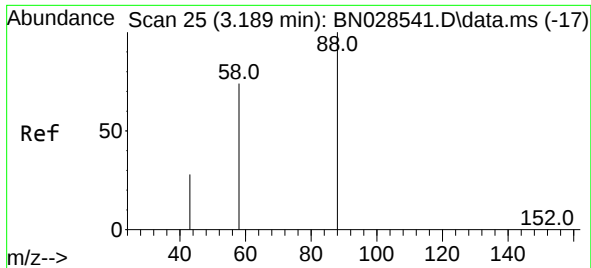

#2
 1,4-Dioxane
 Concen: 0.127 ng/ul
 RT: 3.189 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN028557.D
 Acq: 10 Nov 2023 14:57

Instrument :
 BNA_N
 ClientSampleId :
 BH321

Tgt Ion: 88 Resp: 1252

Ion	Ratio	Lower	Upper
88	100		
43	63.3	32.9	49.3#
58	47.6	41.8	62.8

