

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028569.D
 Acq On : 10 Nov 2023 22:09
 Operator : MA/JU
 Sample : 05044-13
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHEH2

Quant Time: Nov 10 23:29:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8070	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	26901	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.349	164	16935	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.099	188	36721	0.400	ng/ul	0.00
17) Chrysene-d12	21.314	240	25953	0.400	ng/ul	0.00
23) Perylene-d12	23.614	264	27347	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	36136	4.052	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.091	152	12194	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.137	212	39874	0.477	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	1486	0.151	ng/ul#	72
5) Naphthalene	10.540	128	3038	0.040	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028569.D
Acq On : 10 Nov 2023 22:09
Operator : MA/JU
Sample : 05044-13
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHEH2

Quant Time: Nov 10 23:29:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

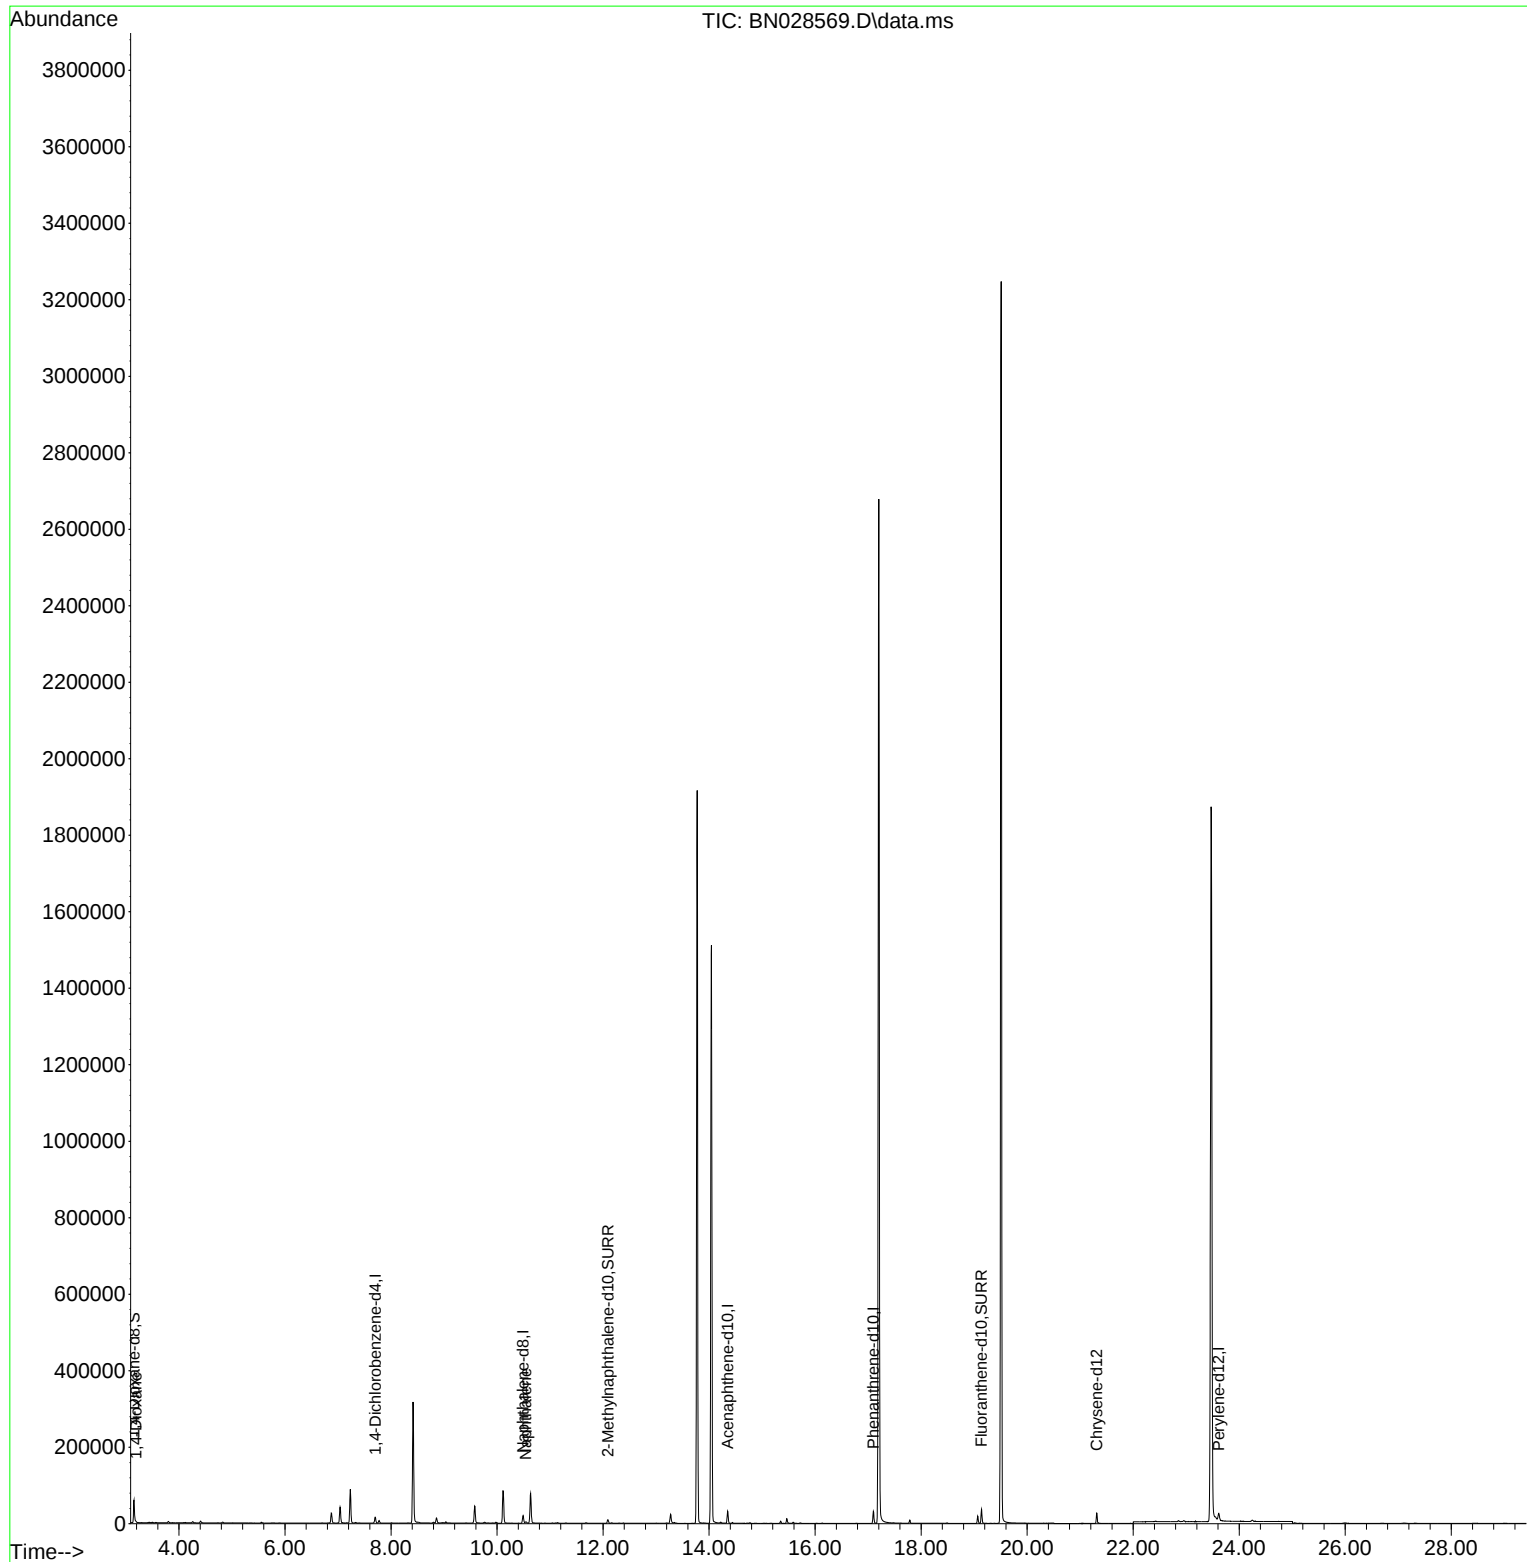

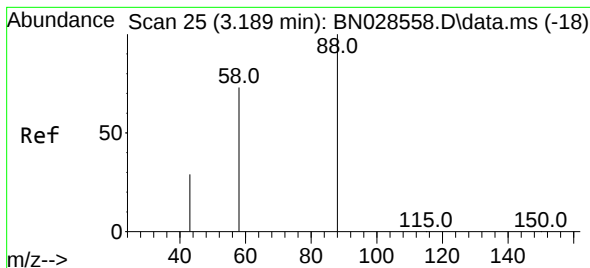

#2

1,4-Dioxane

Concen: 0.151 ng/ul

RT: 3.189 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN028569.D

Acq: 10 Nov 2023 22:09

Instrument :

BNA_N

ClientSampleId :

BHEH2





Tgt Ion: 88 Resp: 1486

Ion Ratio Lower Upper

88 100

43 76.7 32.9 49.3#

58 49.0 41.8 62.8

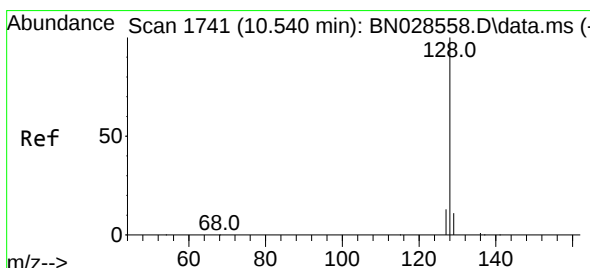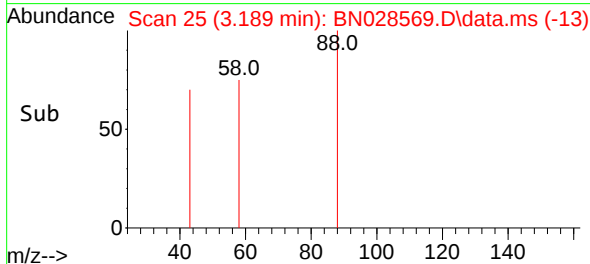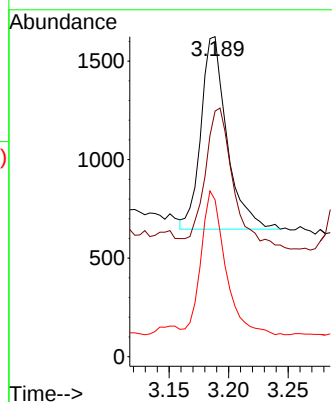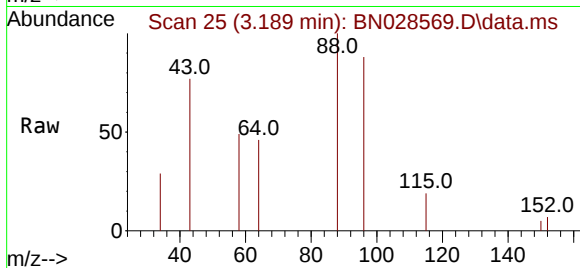

#5

Naphthalene

Concen: 0.040 ng/ul

RT: 10.540 min Scan# 1741

Delta R.T. -0.004 min

Lab File: BN028569.D

Acq: 10 Nov 2023 22:09

Tgt Ion:128 Resp: 3038

Ion Ratio Lower Upper

128 100

129 16.4 9.2 13.8#

127 16.2 10.7 16.1#

