

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
 Data File : BN028572.D
 Acq On : 10 Nov 2023 23:57
 Operator : MA/JU
 Sample : 05044-11DL 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHEH4DL

Quant Time: Nov 11 00:24:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.703	152	8671	0.400	ng/ul	0.00
4) Naphthalene-d8	10.491	136	29271	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.354	164	15298	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.103	188	38842	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.312	240	28304	0.400	ng/ul	0.00
23) Perylene-d12	23.615	264	24215	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	3299	0.344	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.135	152	10828	0.246	ng/ul	0.04
18) Fluoranthene-d10	19.141	212	3308	0.036	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.546	128	3266	0.040	ng/ul#	1
8) 1-Methylnaphthalene	12.388	142	7358	0.134	ng/ul#	14
20) Pyrene	19.536	202	5892	0.047	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110923\
Data File : BN028572.D
Acq On : 10 Nov 2023 23:57
Operator : MA/JU
Sample : 05044-11DL 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHEH4DL

Quant Time: Nov 11 00:24:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration




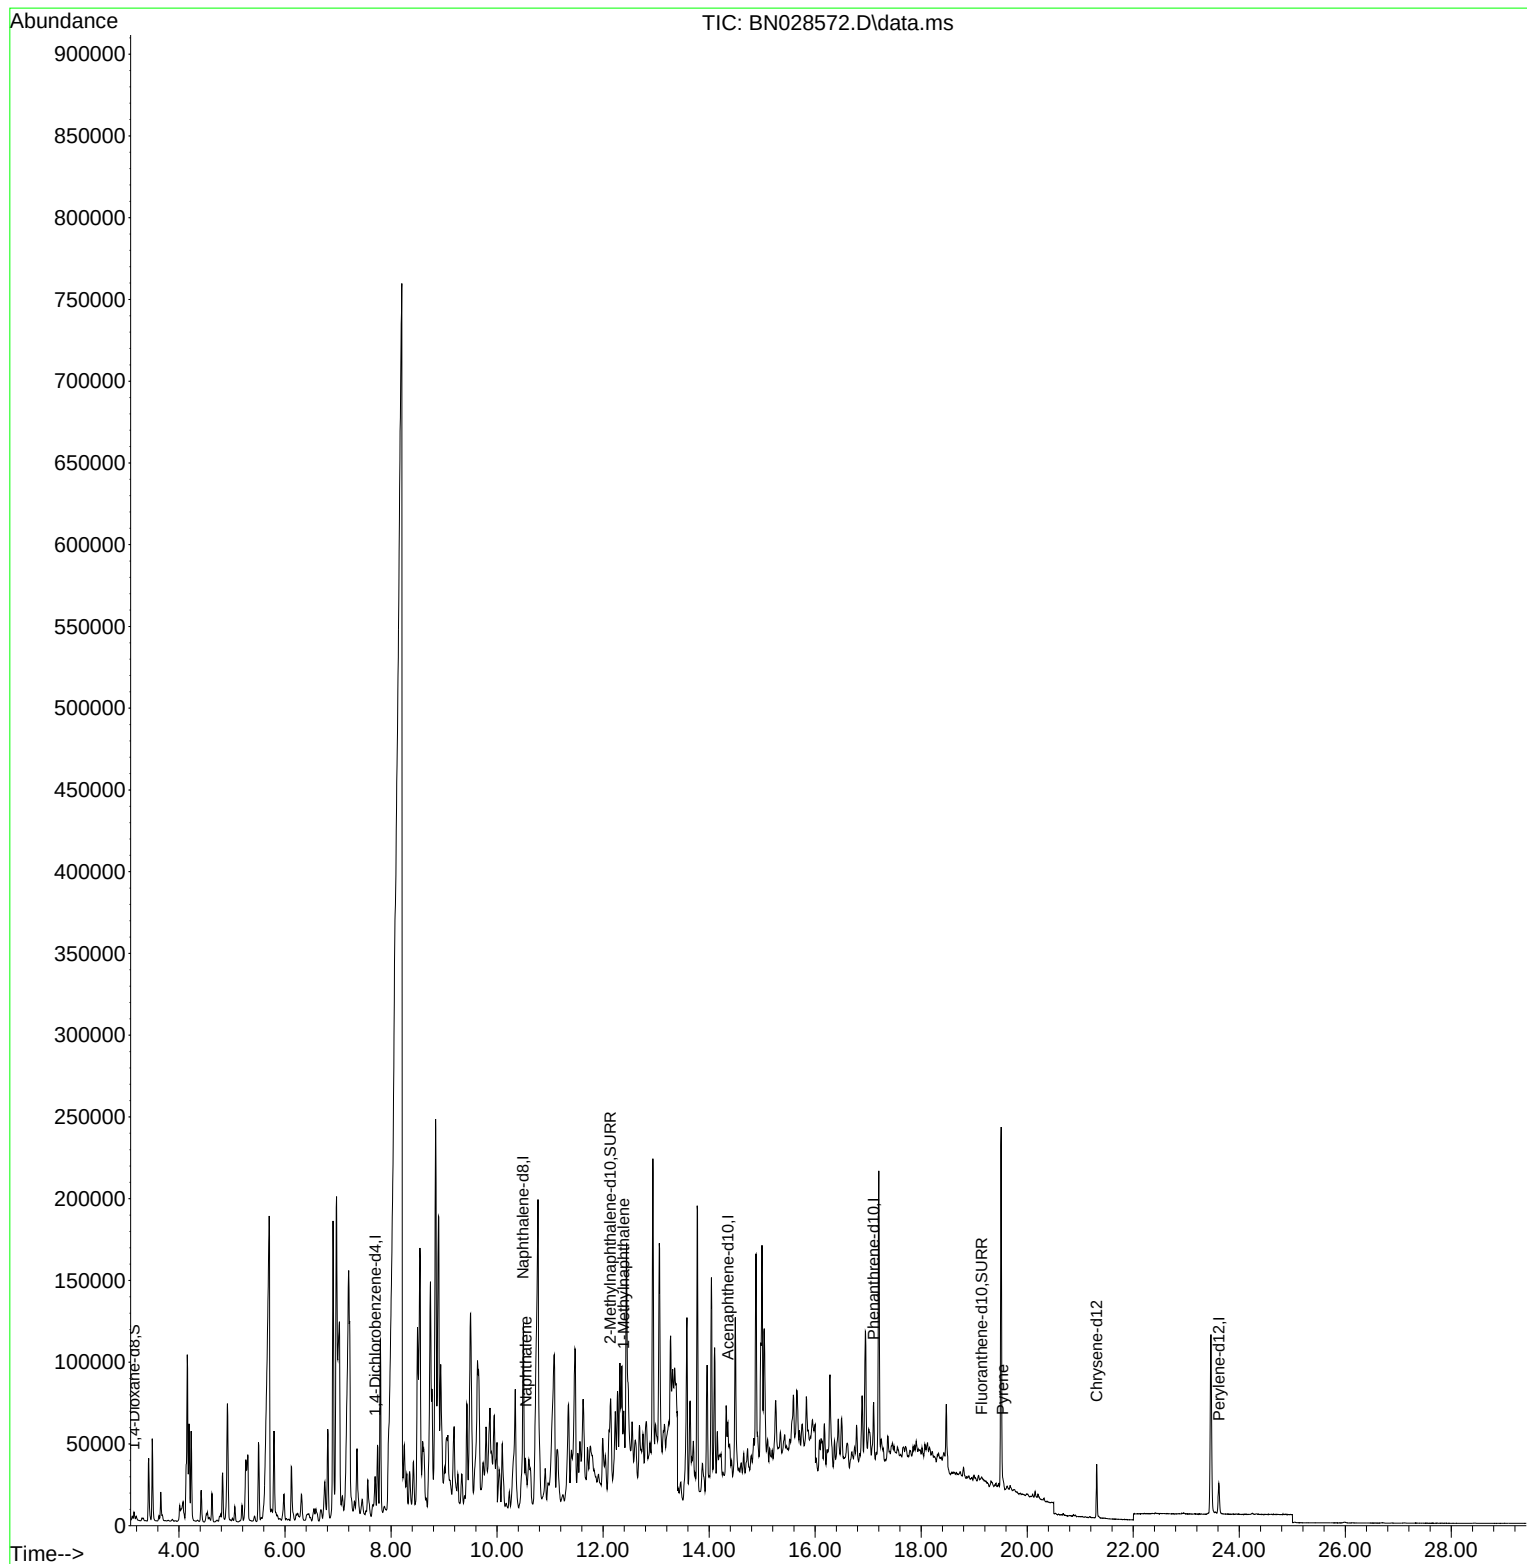


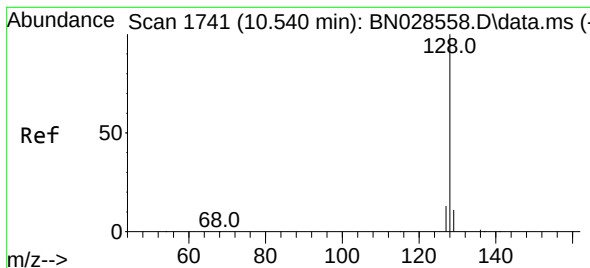

#5
Naphthalene
Concen: 0.040 ng/ul
RT: 10.546 min Scan# 1742
Delta R.T. 0.001 min
Lab File: BN028572.D
Acq: 10 Nov 2023 23:57




Instrument :
BNA_N
ClientSampleId :
BHEH4DL


Tgt Ion:128 Resp: 3266
Ion Ratio Lower Upper
128 100
129 55.4 9.2 13.8#
127 211.3 10.7 16.1#

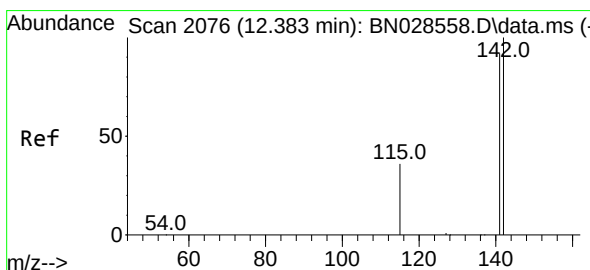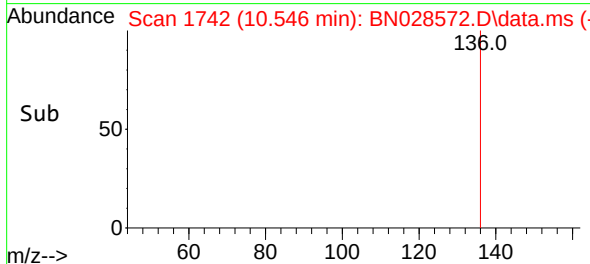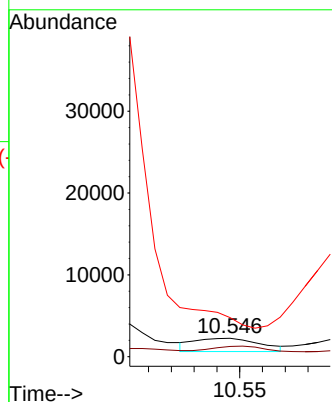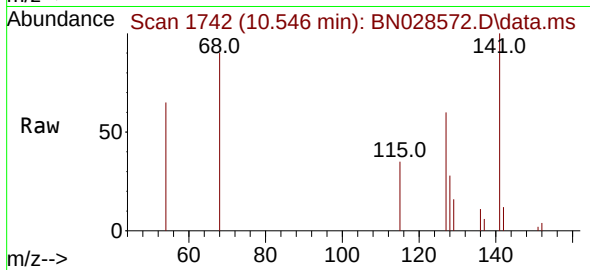

#8
1-Methylnaphthalene
Concen: 0.134 ng/ul
RT: 12.388 min Scan# 2077
Delta R.T. 0.001 min
Lab File: BN028572.D
Acq: 10 Nov 2023 23:57

Tgt Ion:142 Resp: 7358
Ion Ratio Lower Upper
142 100
141 175.2 74.1 111.1#

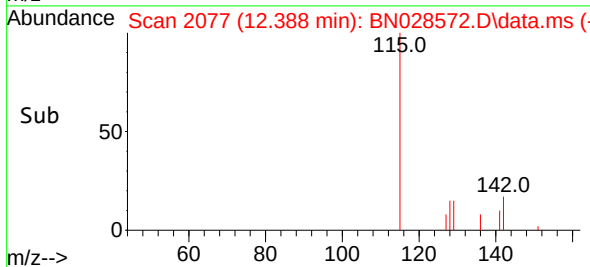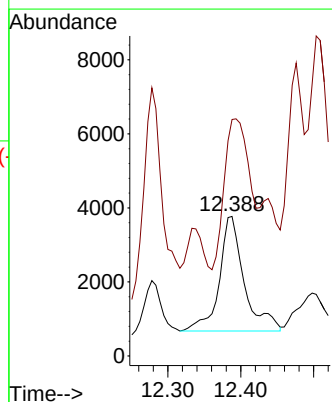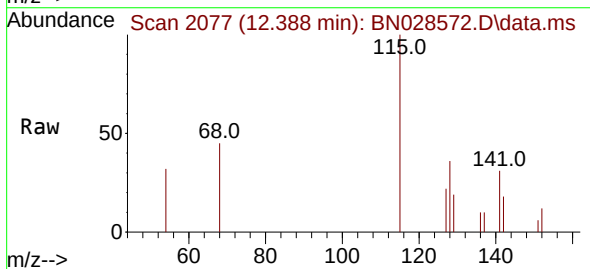

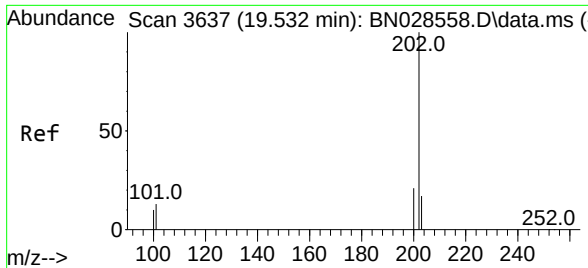

#20
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.536 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BN028572.D
 Acq: 10 Nov 2023 23:57

Instrument :
 BNA_N
 ClientSampleId :
 BHEH4DL

Tgt Ion:	202	Resp:	5892
Ion Ratio	Lower	Upper	
202	100		
101	34.2	10.3	15.5#
100	20.8	8.2	12.2#

