
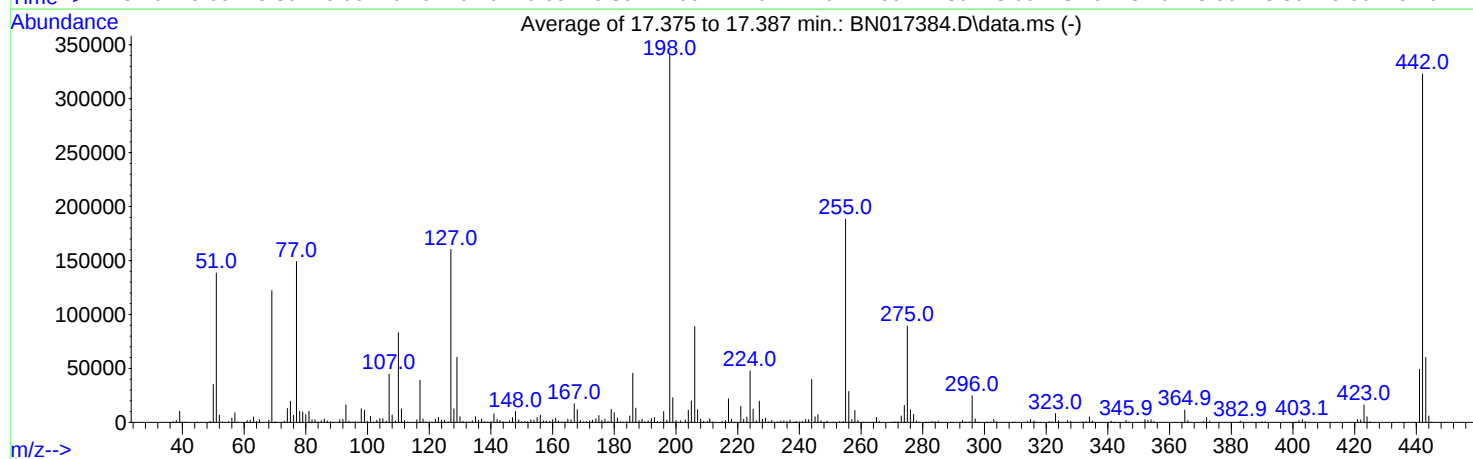


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111121\
 Data File : BN017384.D
 Acq On : 10 Nov 2021 17:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN111121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 11 08:04:11 2021

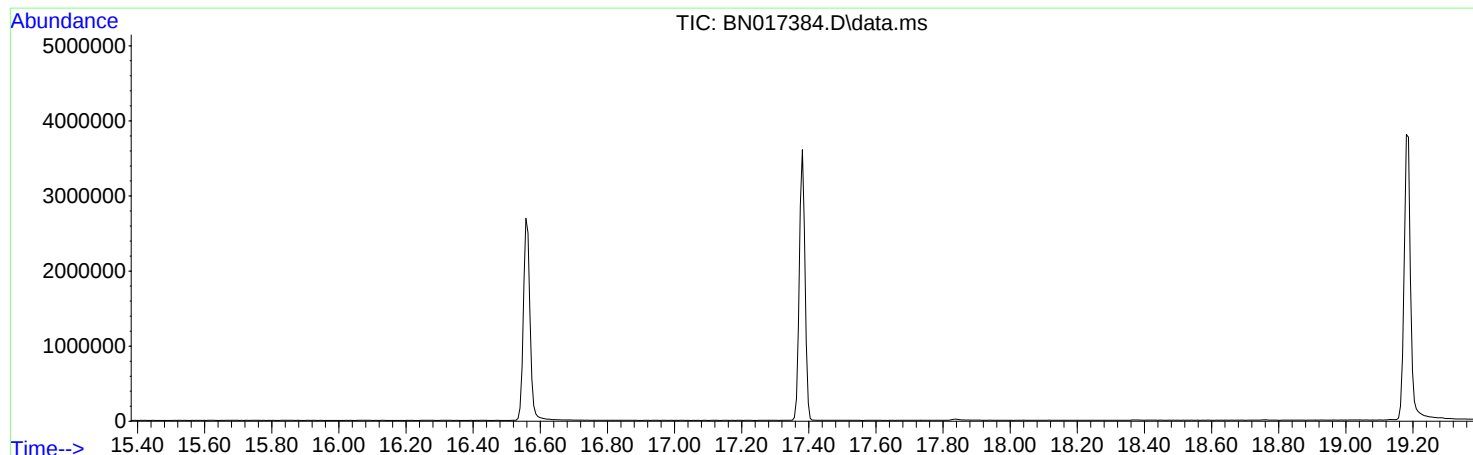

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	138427	PASS
68	69	0.00	2	1.7	2078	PASS
69	198	0.00	100	35.8	122123	PASS
70	69	0.00	2	0.5	669	PASS
127	198	10	80	47.0	160208	PASS
197	198	0.00	2	0.6	2049	PASS
198	198	100	100	100.0	340971	PASS
199	198	5	9	6.7	22888	PASS
275	198	10	60	26.2	89229	PASS
365	198	1	100	3.3	11372	PASS
441	198	0.01	100	14.4	49168	PASS
442	442	50	100	100.0	322816	PASS
443	442	15	24	18.7	60301	PASS