


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111225\
Data File : BN038182.D
Acq On : 12 Nov 2025 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 29 13:09:46 2025

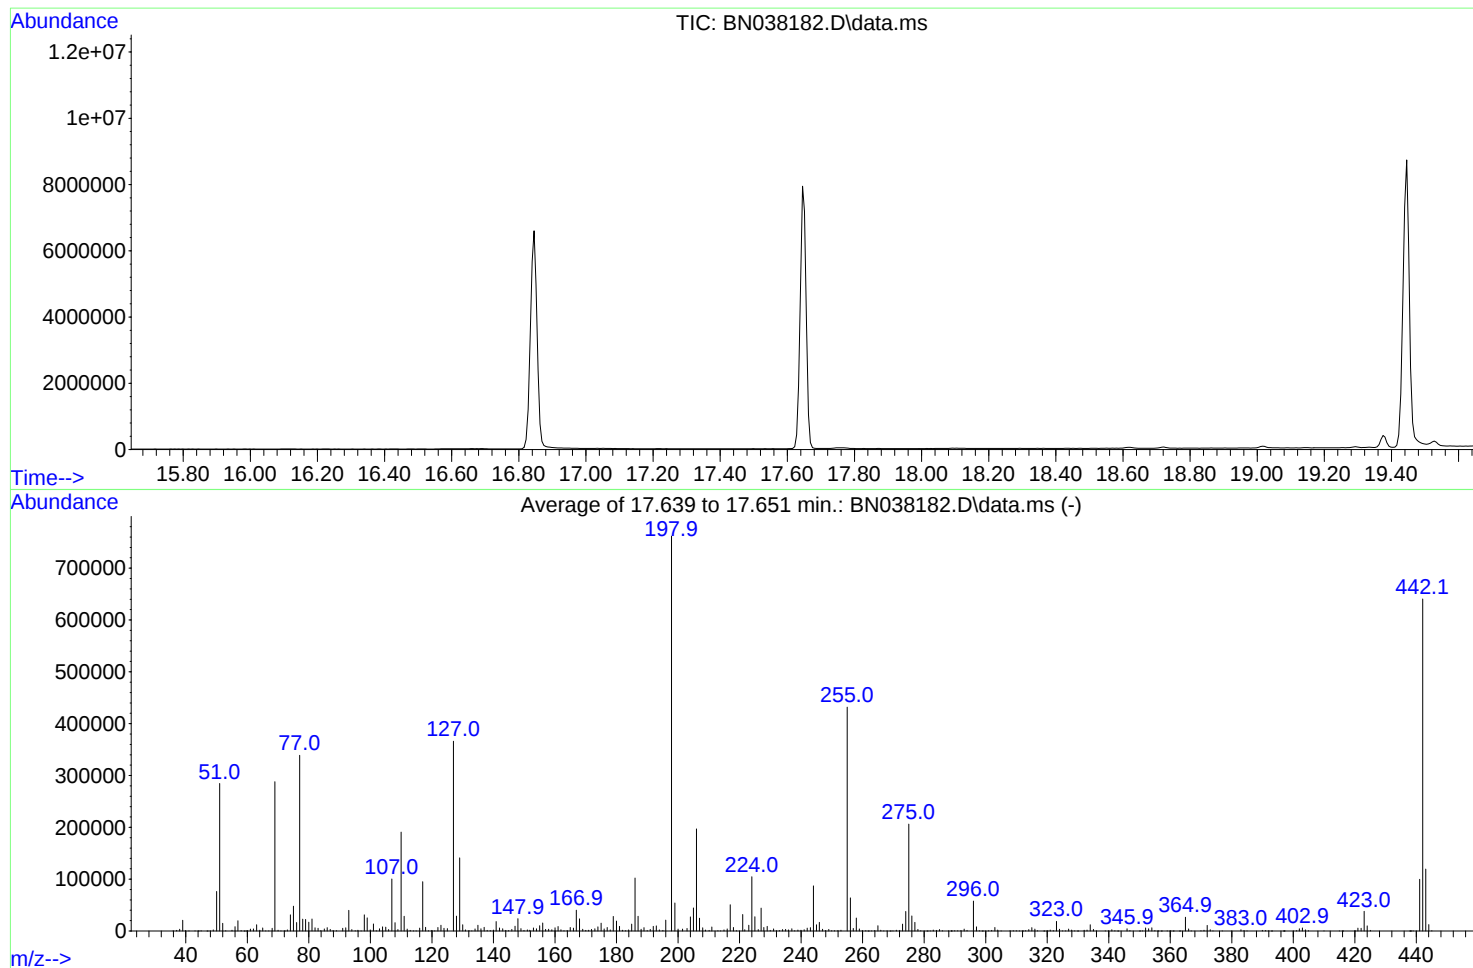

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467




Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	5354	PASS
69	69	100	100	100.0	287920	PASS
70	69	0.00	2	0.5	1437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	761707	PASS
199	198	5	9	7.1	53917	PASS
365	198	1	100	3.5	26494	PASS
441	443	0.01	150	83.5	99787	PASS
442	442	100	100	100.0	640512	PASS
443	442	15	24	18.6	119448	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/12/2025	BNA_N	<u>BN038182.D</u>
Compound Name	Response	Retention Time
DDT	2757316	20.68
DDD	65562	20.239
DDE	9652	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
75214	2832530	2.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111225\
Data File : BN038182.D
Acq On : 12 Nov 2025 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 09:43:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 09:43:16 2025
Response via : Initial Calibration

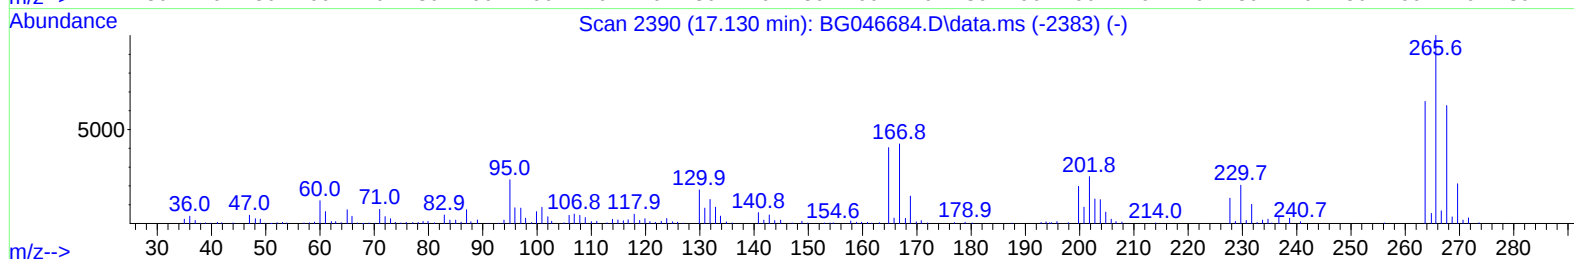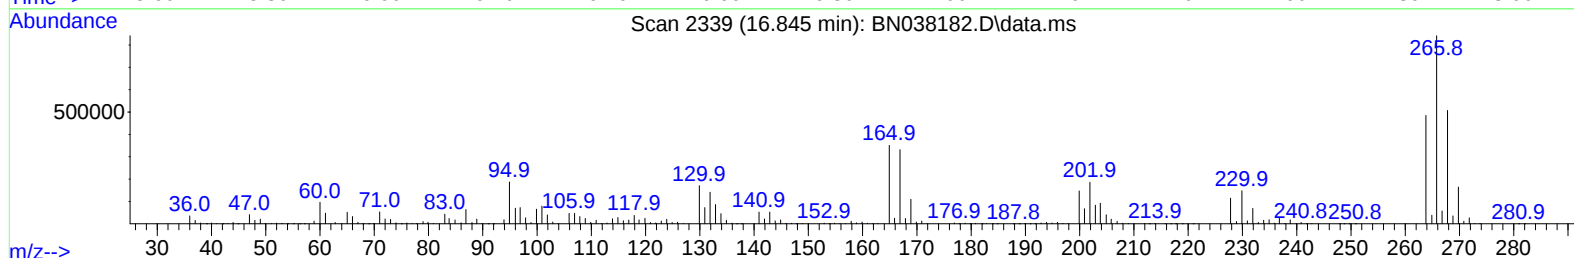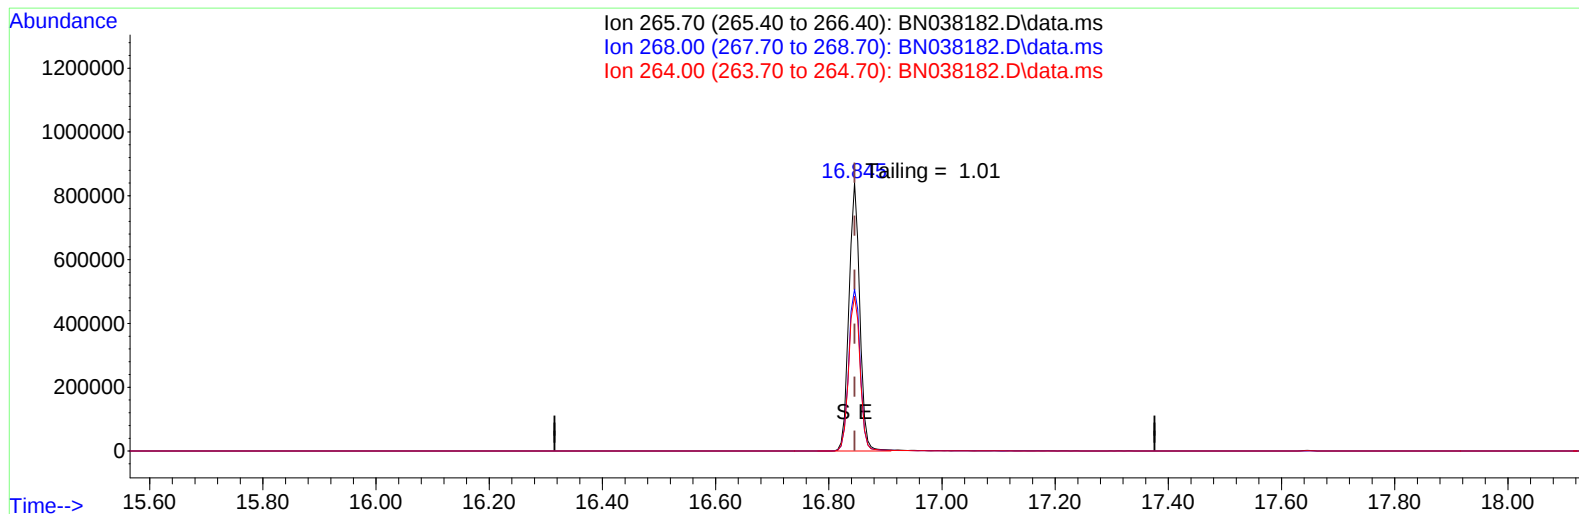

TIC: BN038182.D\data.ms

(70) Pentachlorophenol (C)




16.845min (0.000) 277.65 ng

response 1120061

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.25
264.00	61.60	57.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111225\
Data File : BN038182.D
Acq On : 12 Nov 2025 08:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 09:43:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 12 09:43:16 2025
Response via : Initial Calibration

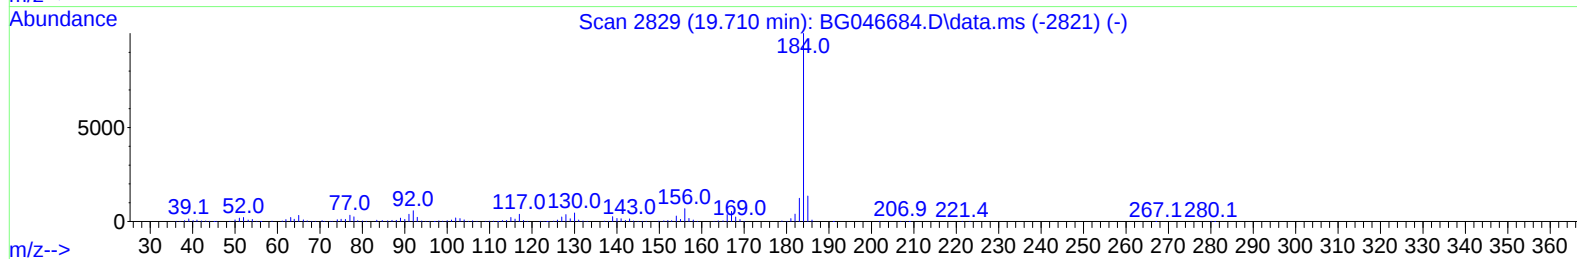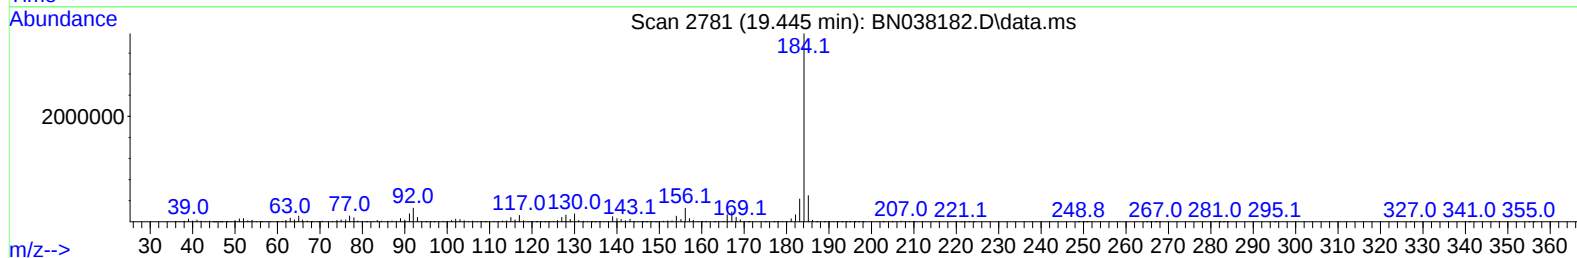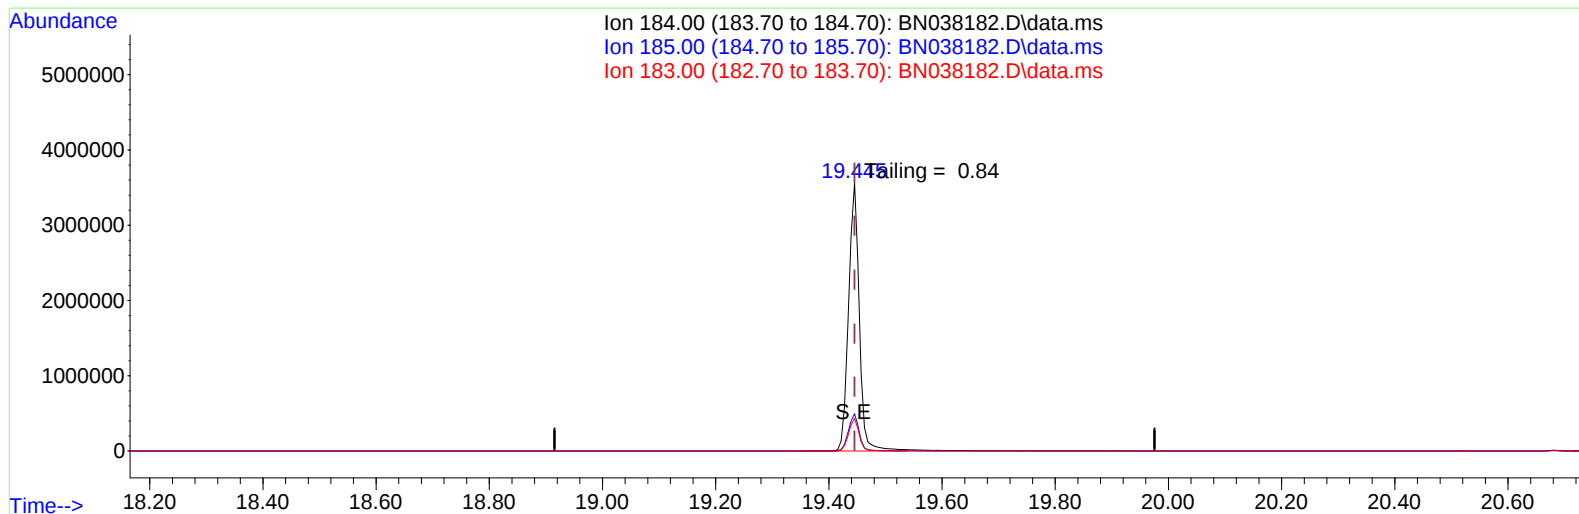

TIC: BN038182.D\data.ms

(77) Benzidine**19.445min (0.000) 279.97 ng****response 4753744**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.10
0.00	0.00	0.00