

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN111318\  
 Data File : BN003530.D  
 Acq On : 14 Nov 2018 01:58  
 Operator : MJ/SJ  
 Sample : J5916-22  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 110918-JETT-F-U-S

Quant Time: Nov 14 02:54:27 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-BN111218.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Nov 12 15:59:25 2018  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|--------------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 7.85  | 152  | 88119    | 20.00  | ng    | 0.00     |
| 21) Naphthalene-d8             | 10.64 | 136  | 395920   | 20.00  | ng    | 0.00     |
| 39) Acenaphthene-d10           | 14.48 | 164  | 237652   | 20.00  | ng    | 0.00     |
| 64) Phenanthrene-d10           | 17.22 | 188  | 507583   | 20.00  | ng    | 0.00     |
| 76) Chrysene-d12               | 21.40 | 240  | 410041   | 20.00  | ng    | 0.00     |
| 87) Perylene-d12               | 23.71 | 264  | 414511   | 20.00  | ng    | 0.00     |
| System Monitoring Compounds    |       |      |          |        |       |          |
| 5) 2-Fluorophenol              | 5.41  | 112  | 212104   | 43.41  | ng    | 0.00     |
| 7) Phenol-d6                   | 7.00  | 99   | 169172   | 24.97  | ng    | 0.00     |
| 23) Nitrobenzene-d5            | 9.02  | 82   | 634256   | 100.84 | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol       | 15.97 | 330  | 338958   | 95.68  | ng    | 0.00     |
| 45) 2-Fluorobiphenyl           | 13.10 | 172  | 1761339  | 98.92  | ng    | 0.00     |
| 79) Terphenyl-d14              | 19.84 | 244  | 2006183  | 96.32  | ng    | 0.00     |
| Target Compounds               |       |      |          |        |       |          |
| 19) n-Nitroso-di-n-propylamine | 9.02  | 70   | 80594    | 17.666 | ng    | # 75     |
| 51) 2,6-Dinitrotoluene         | 14.48 | 165  | 30285    | 6.969  | ng    | # 32     |
| 57) 2,4-Dinitrotoluene         | 14.48 | 165  | 30285    | 5.156  | ng    | # 32     |
| 65) 4,6-Dinitro-2-methylphenol | 15.97 | 198  | 494      | 5.063  | ng    | # 1      |
| 67) 4-Bromophenyl-phenylether  | 15.97 | 248  | 21974    | 3.432  | ng    | # 1      |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN111318\  
Data File : BN003530.D  
Acq On : 14 Nov 2018 01:58  
Operator : MJ/SJ  
Sample : J5916-22  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
110918-JETT-F-U-S

Quant Time: Nov 14 02:54:27 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-BN111218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Nov 12 15:59:25 2018  
Response via : Initial Calibration

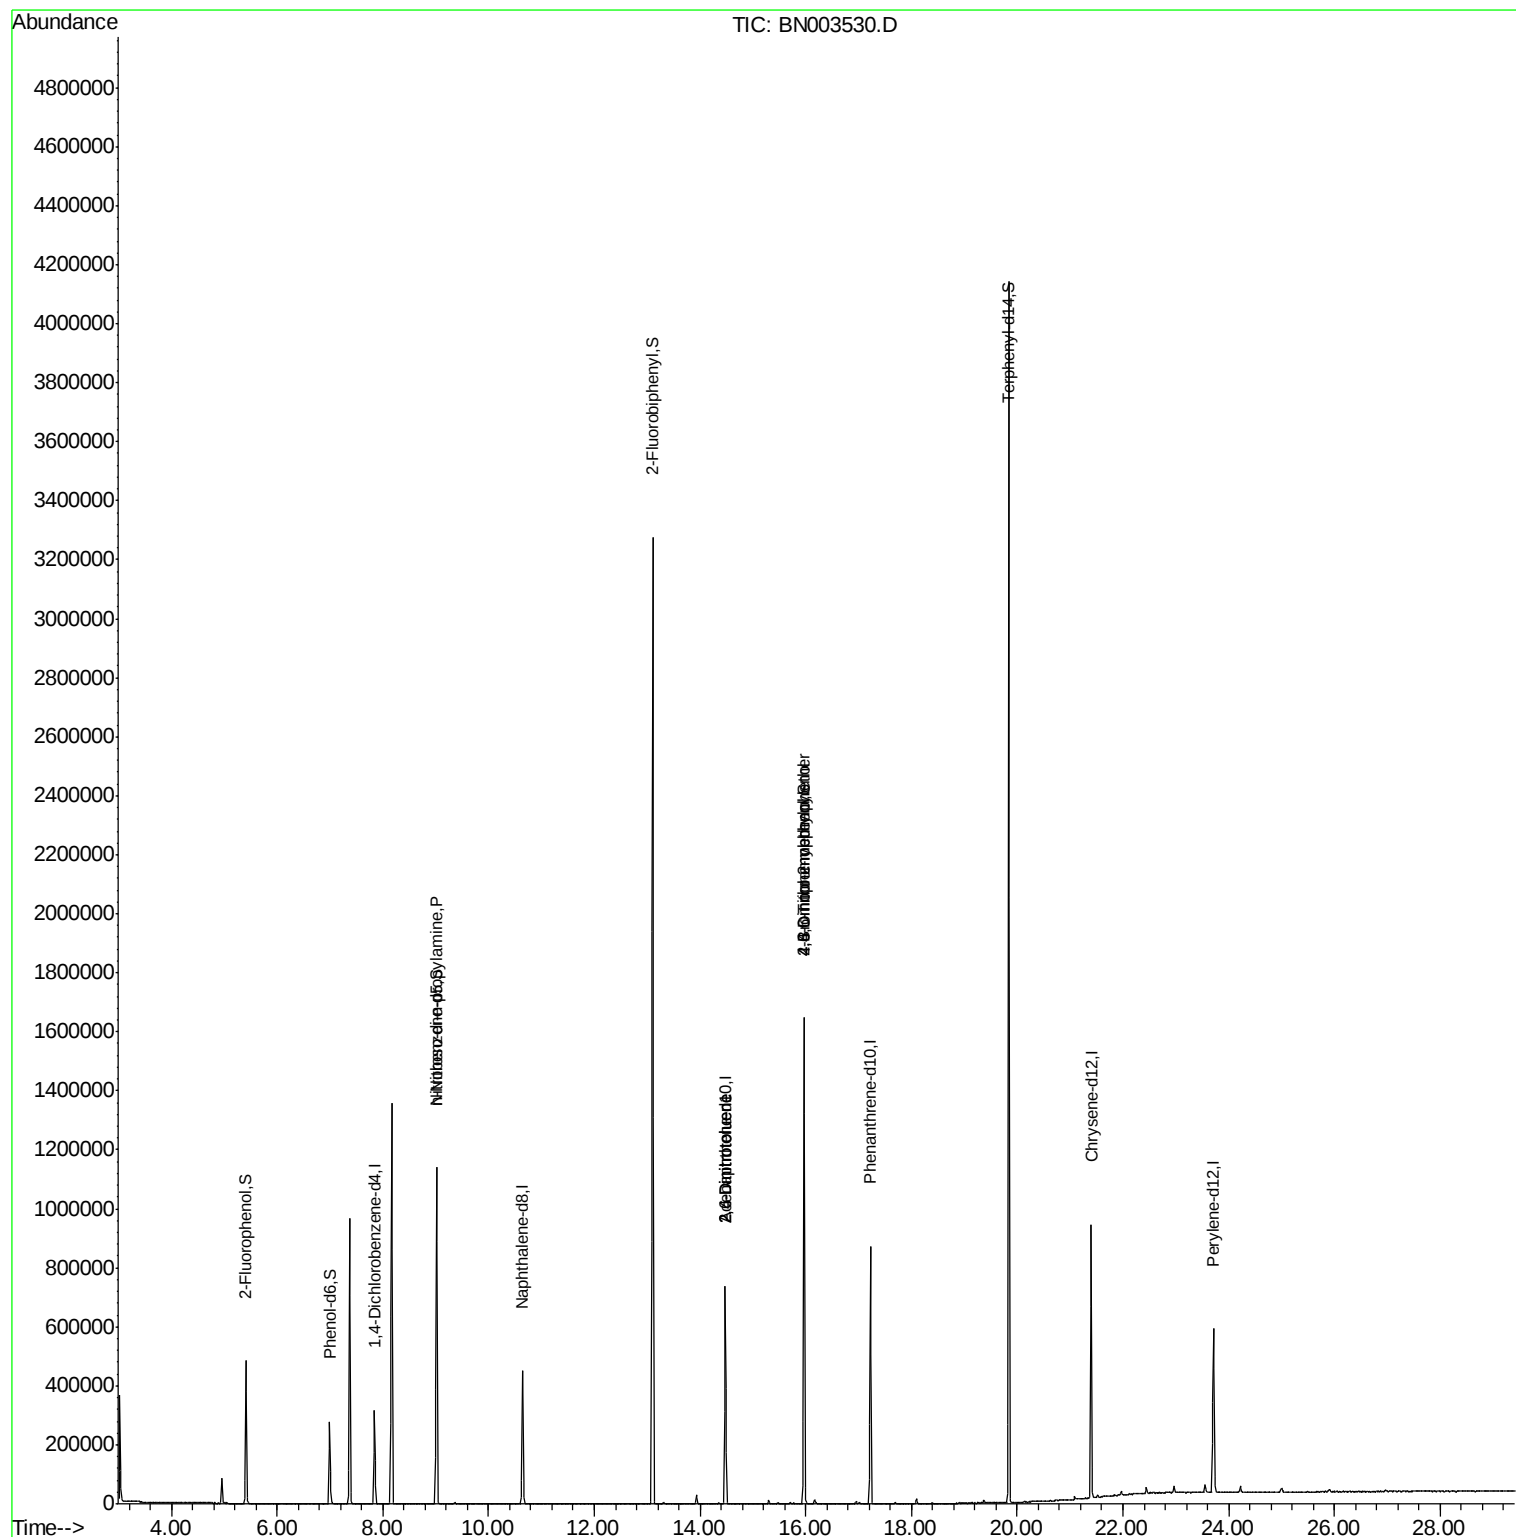


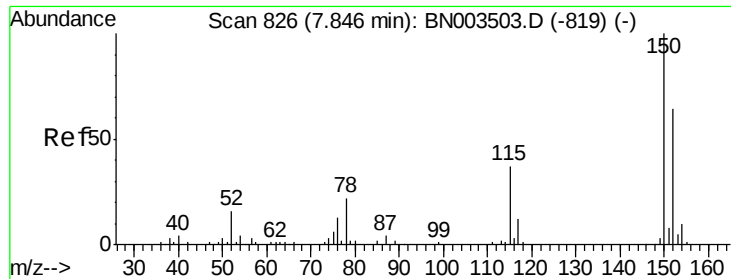




#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 7.85 min Scan# 826  
 Delta R.T. 0.00 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Instrument :  
 BNA\_N  
 ClientSampleId :  
 110918-JETT-F-U-S

Tgt Ion:152 Resp: 88119  
 Ion Ratio Lower Upper  
 152 100  
 150 152.6 125.4 188.0  
 115 58.6 45.9 68.9

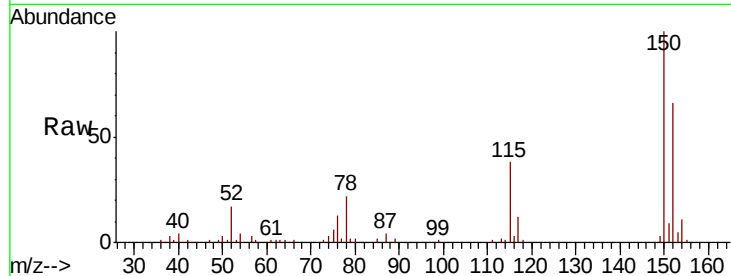


Abundance Ion 152.00 (151.70 to 152.70): E  
 Ion 150.00 (149.70 to 150.70): E  
 Ion 115.00 (114.70 to 115.70): E


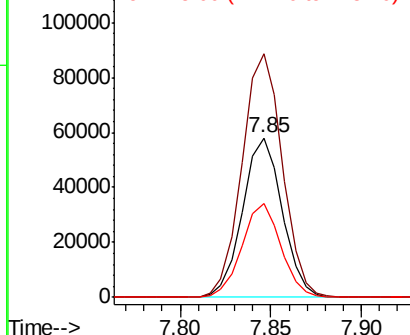



#5  
 2-Fluorophenol  
 Concen: 43.412 ng  
 RT: 5.41 min Scan# 412  
 Delta R.T. 0.00 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Tgt Ion:112 Resp: 212104  
 Ion Ratio Lower Upper  
 112 100  
 64 52.7 41.4 62.2  
 63 25.9 20.5 30.7



Abundance Ion 112.00 (111.70 to 112.70): E  
 Ion 64.00 (63.70 to 64.70): BNC  
 Ion 63.00 (62.70 to 63.70): BNC

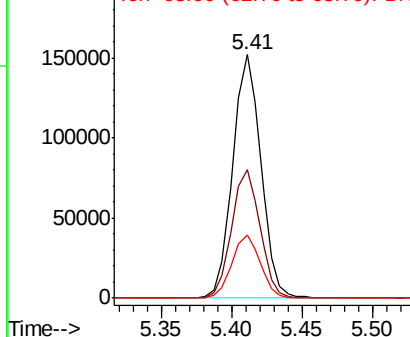

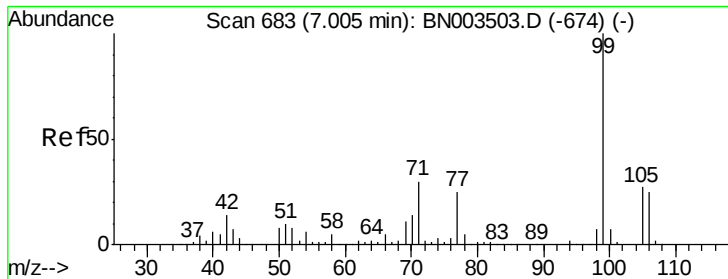

#7

Phenol-d6

Concen: 24.967 ng

RT: 7.00 min Scan# 682

Delta R.T. -0.01 min

Lab File: BN003530.D

Acq: 14 Nov 2018 01:58

Instrument :

BNA\_N

ClientSampleId :

110918-JETT-F-U-S


Tgt Ion: 99 Resp: 169172

Ion Ratio Lower Upper




99 100

42 14.5 11.6 17.4

71 29.2 24.2 36.2

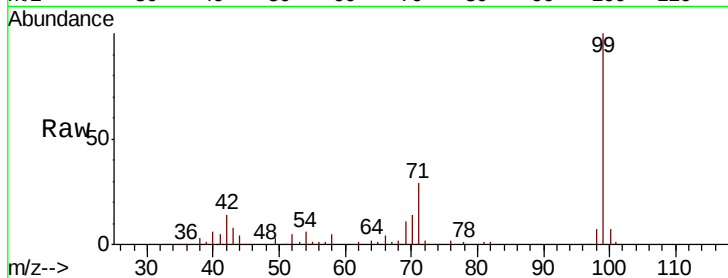

Abundance Ion 99.00 (98.70 to 99.70): BN0  
Ion 42.00 (41.70 to 42.70): BN0  
Ion 71.00 (70.70 to 71.70): BN0

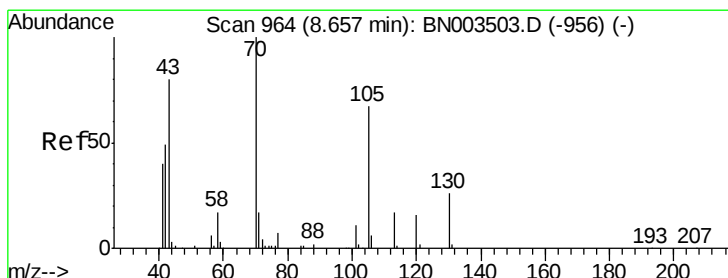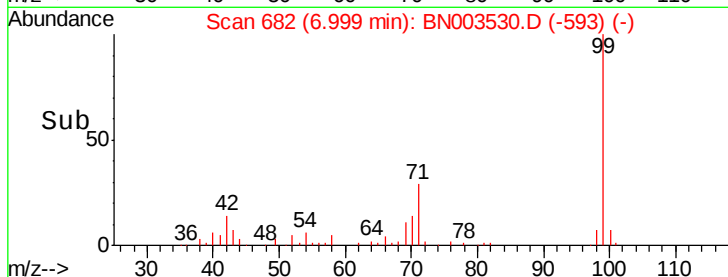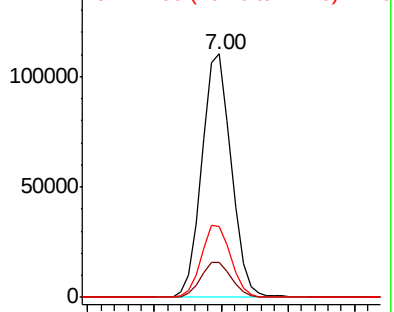

#19

n-Nitroso-di-n-propylamine

Concen: 17.666 ng

RT: 9.02 min Scan# 1025

Delta R.T. 0.36 min

Lab File: BN003530.D

Acq: 14 Nov 2018 01:58

Tgt Ion: 70 Resp: 80594


Ion Ratio Lower Upper

70 100



42 41.3 39.7 59.5


101 0.0 8.8 13.2#

130 2.3 20.8 31.2#

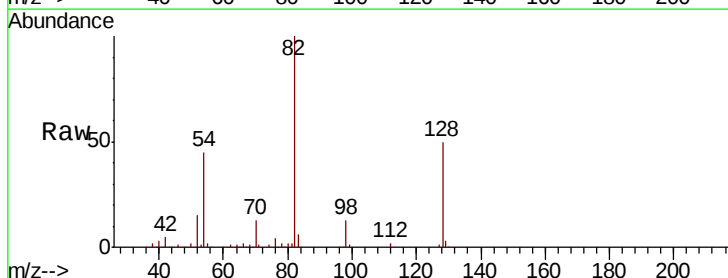

Abundance Ion 70.00 (69.70 to 70.70): BN0  
Ion 42.00 (41.70 to 42.70): BN0  
Ion 101.00 (100.70 to 101.70): E  
Ion 130.00 (129.70 to 130.70): E



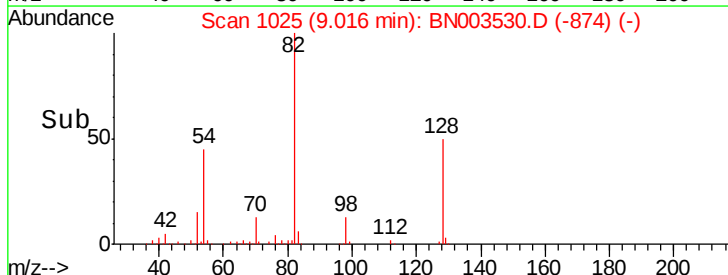
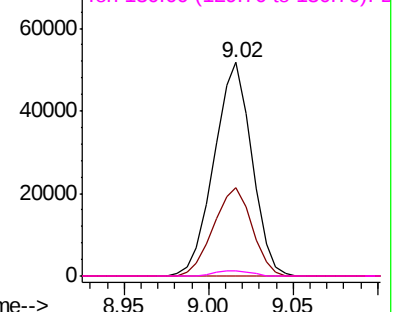


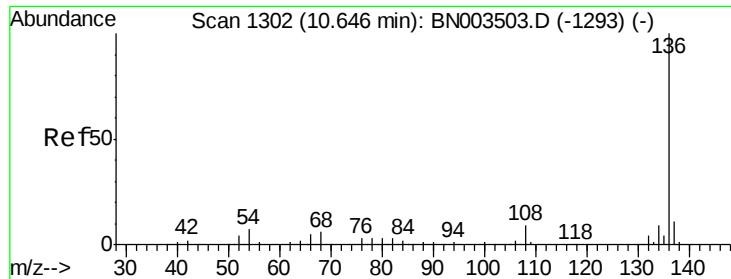

#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 10.64 min Scan# 1301  
Delta R.T. -0.01 min  
Lab File: BN003530.D  
Acq: 14 Nov 2018 01:58




Instrument :  
BNA\_N  
ClientSampleId :  
110918-JETT-F-U-S


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 136   | Resp: | 395920 |
| Ion      | Ratio | Lower | Upper  |
| 136      | 100   |       |        |
| 137      | 11.2  | 8.7   | 13.1   |
| 54       | 7.3   | 5.7   | 8.5    |
| 68       | 6.1   | 4.7   | 7.1    |

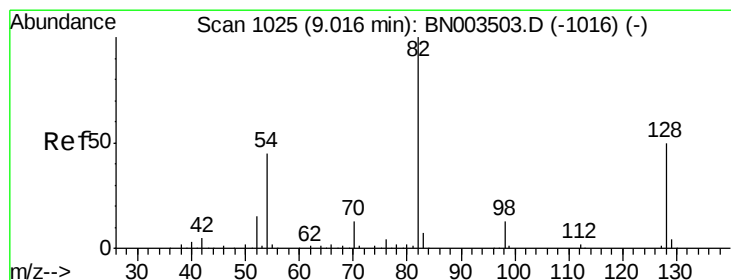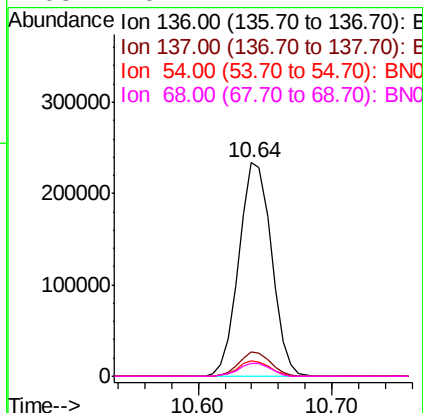

#23  
Nitrobenzene-d5  
Concen: 100.840 ng  
RT: 9.02 min Scan# 1025  
Delta R.T. 0.00 min  
Lab File: BN003530.D  
Acq: 14 Nov 2018 01:58

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 82    | Resp: | 634256 |
| Ion      | Ratio | Lower | Upper  |
| 82       | 100   |       |        |
| 128      | 50.3  | 40.0  | 60.0   |
| 54       | 45.0  | 36.1  | 54.1   |

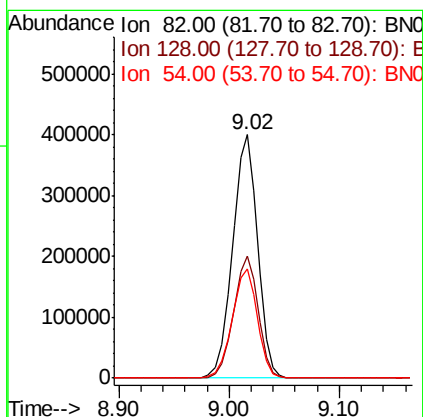

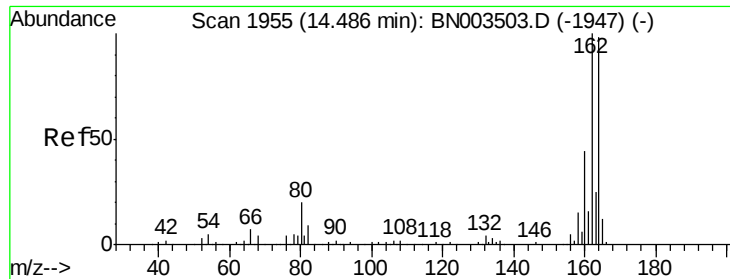

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.48 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BN003530.D

Acq: 14 Nov 2018 01:58

Instrument :

BNA\_N

ClientSampleId :

110918-JETT-F-U-S


Tgt Ion:164 Resp: 237652

Ion Ratio Lower Upper

164 100

162 103.3 81.8 122.6




160 45.9 36.2 54.2

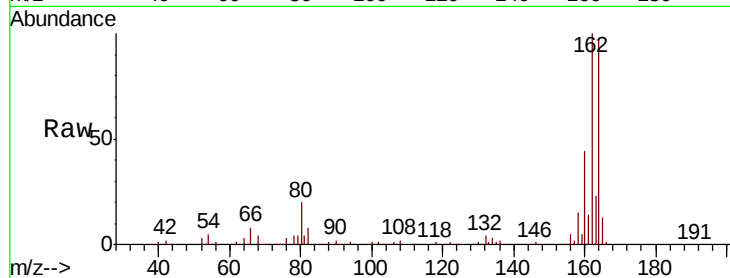

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

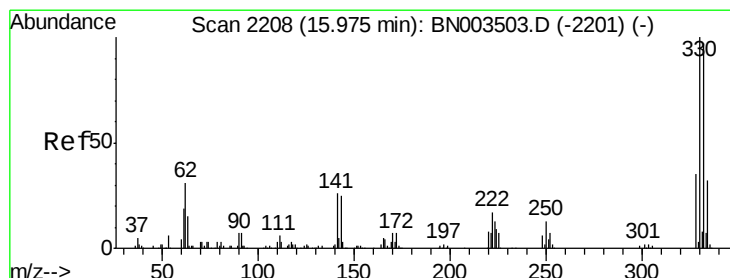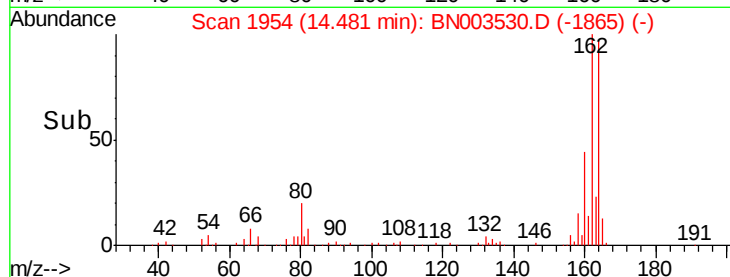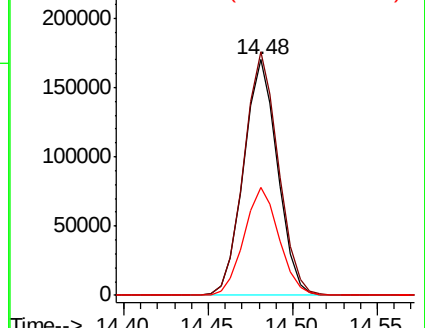

#42

2,4,6-Tribromophenol

Concen: 95.675 ng

RT: 15.97 min Scan# 2207

Delta R.T. -0.01 min

Lab File: BN003530.D

Acq: 14 Nov 2018 01:58


Tgt Ion:330 Resp: 338958

Ion Ratio Lower Upper

330 100

332 96.6 76.8 115.2



141 27.4 21.6 32.4

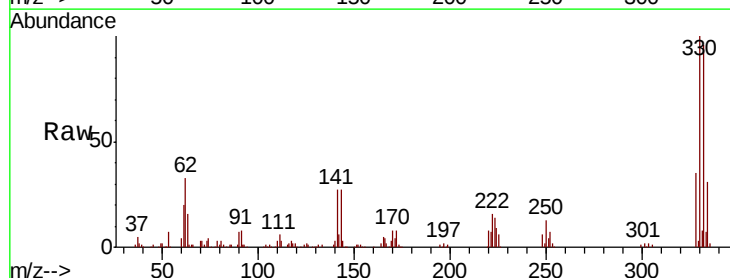


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



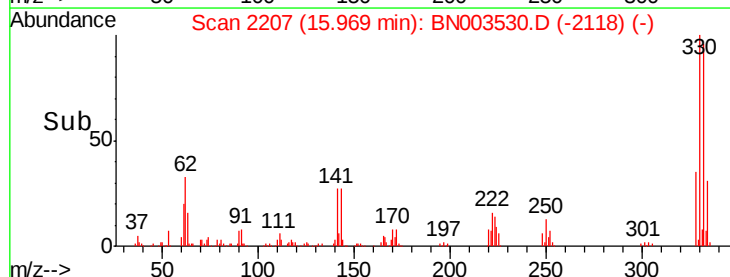
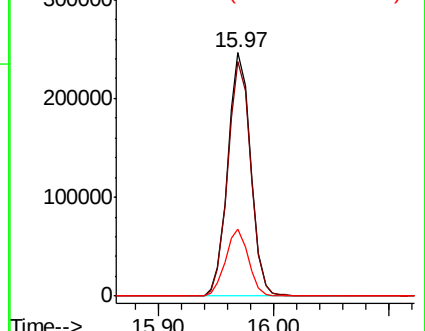




#45  
 2-Fluorobiphenyl  
 Concen: 98.924 ng  
 RT: 13.10 min Scan# 1720  
 Delta R.T. 0.00 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58




Instrument :  
 BNA\_N  
 ClientSampleId :  
 110918-JETT-F-U-S


Tgt Ion:172 Resp: 1761339  
 Ion Ratio Lower Upper  
 172 100  
 171 36.4 28.3 42.5  
 170 23.3 18.7 28.1

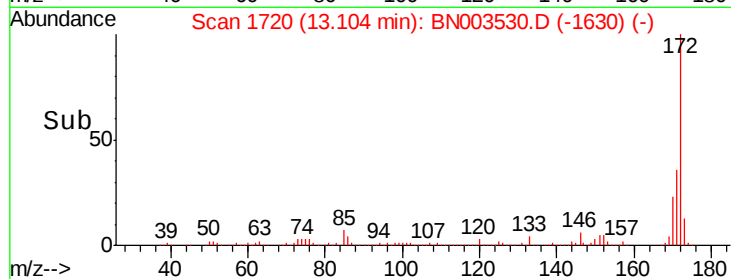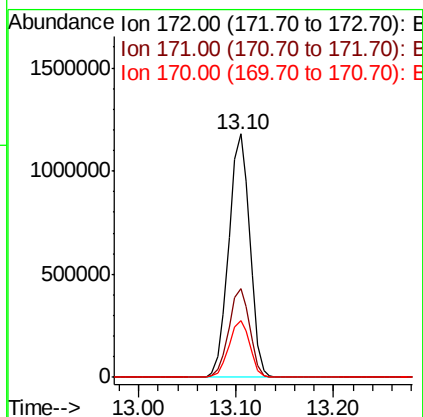

#51  
 2,6-Dinitrotoluene  
 Concen: 6.969 ng  
 RT: 14.48 min Scan# 1954  
 Delta R.T. 0.41 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Tgt Ion:165 Resp: 30285  
 Ion Ratio Lower Upper  
 165 100  
 63 0.0 34.3 51.5#  
 89 0.0 36.7 55.1#

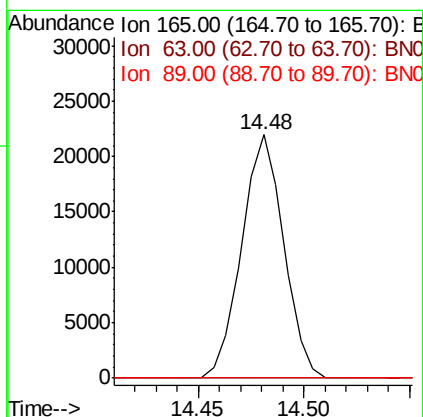







#57  
 2,4-Dinitrotoluene  
 Concen: 5.156 ng  
 RT: 14.48 min Scan# 1954  
 Delta R.T. -0.38 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Instrument :  
 BNA\_N  
 ClientSampleId :  
 110918-JETT-F-U-S

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 165   | Resp: | 30285 |
| Ion      | Ratio | Lower | Upper |
| 165      | 100   |       |       |
| 63       | 0.0   | 25.4  | 38.2# |
| 89       | 0.0   | 44.7  | 67.1# |
| 182      | 0.0   | 2.6   | 3.8#  |

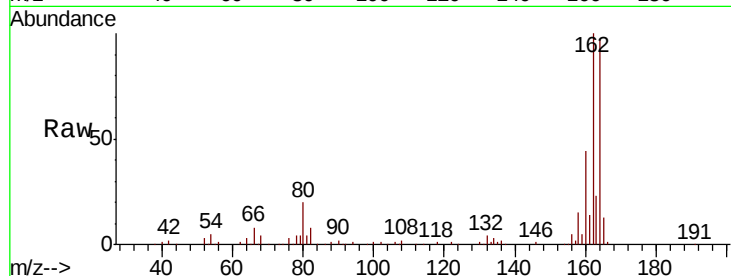


Abundance Ion 165.00 (164.70 to 165.70): E  
 Ion 63.00 (62.70 to 63.70): BNC  
 Ion 89.00 (88.70 to 89.70): BNC  
 Ion 182.00 (181.70 to 182.70): E

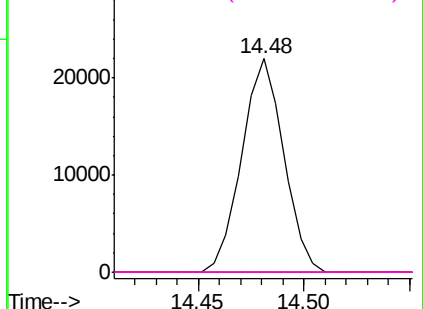




#64  
 Phenanthrene-d10  
 Concen: 20.000 ng  
 RT: 17.22 min Scan# 2420  
 Delta R.T. -0.01 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 188   | Resp: | 507583 |
| Ion      | Ratio | Lower | Upper  |
| 188      | 100   |       |        |
| 94       | 9.8   | 7.6   | 11.4   |
| 80       | 10.6  | 8.2   | 12.2   |



Abundance Ion 188.00 (187.70 to 188.70): E  
 Ion 94.00 (93.70 to 94.70): BNC  
 Ion 80.00 (79.70 to 80.70): BNC

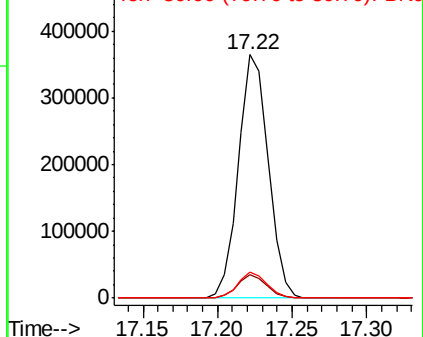


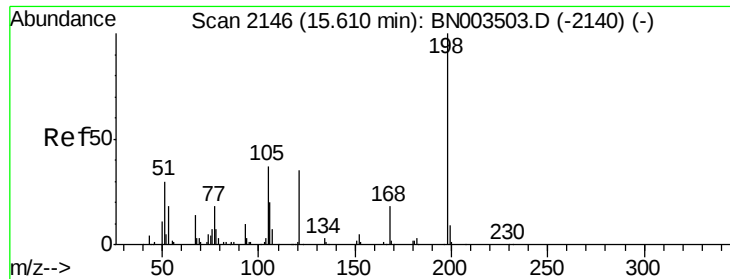




#65  
 4,6-Dinitro-2-methylphenol  
 Concen: 5.063 ng  
 RT: 15.97 min Scan# 2207  
 Delta R.T. 0.36 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Instrument :  
 BNA\_N  
 ClientSampleId :  
 110918-JETT-F-U-S

Tgt Ion:198 Resp: 494  
 Ion Ratio Lower Upper  
 198 100  
 51 110.5 13.8 53.8#  
 105 167.2 18.3 58.3#

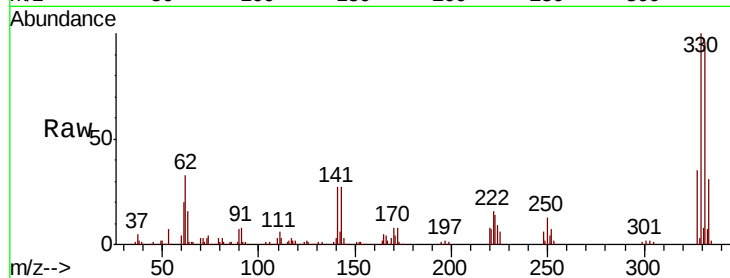


Abundance Ion 198.00 (197.70 to 198.70): E  
 Ion 51.00 (50.70 to 51.70): BNO  
 Ion 105.00 (104.70 to 105.70): E

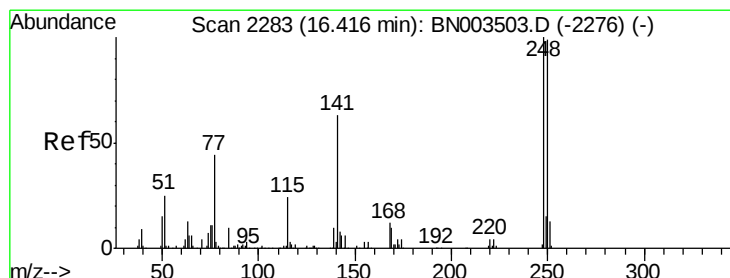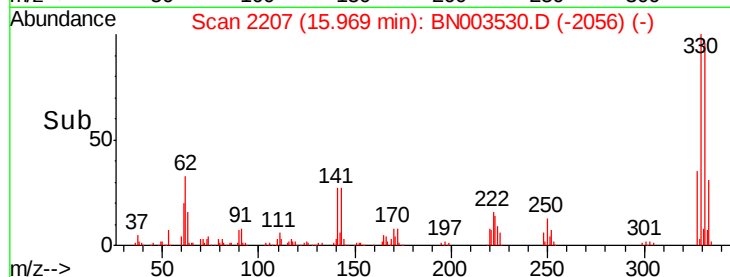
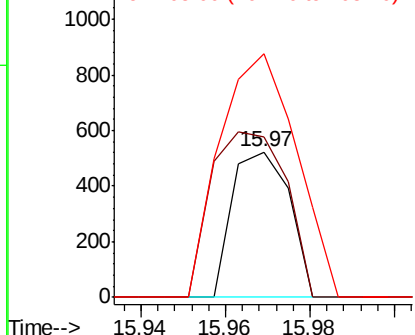



#67  
 4-Bromophenyl-phenylether  
 Concen: 3.432 ng  
 RT: 15.97 min Scan# 2207  
 Delta R.T. -0.45 min  
 Lab File: BN003530.D  
 Acq: 14 Nov 2018 01:58

Tgt Ion:248 Resp: 21974  
 Ion Ratio Lower Upper  
 248 100  
 250 202.1 79.0 118.6#  
 141 421.7 50.7 76.1#

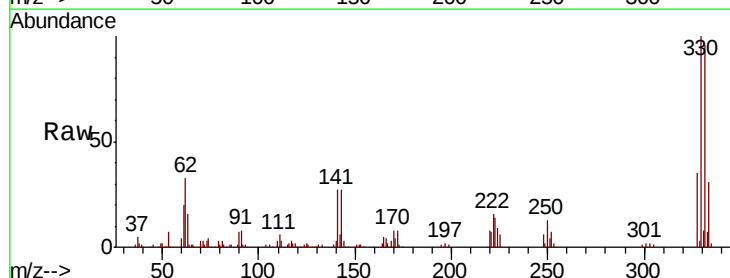

Abundance Ion 248.00 (247.70 to 248.70): E  
 Ion 250.00 (249.70 to 250.70): E  
 Ion 141.00 (140.70 to 141.70): E



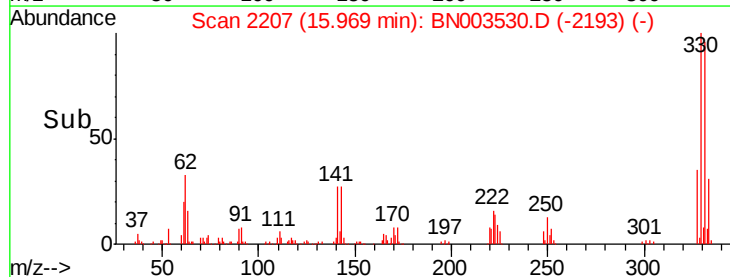
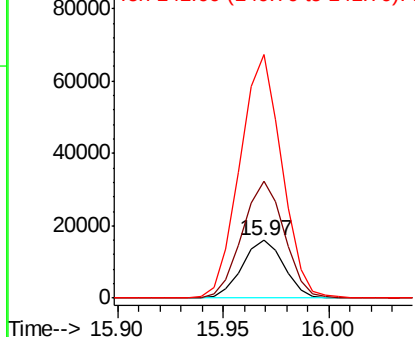




#76  
Chrysene-d12  
Concen: 20.000 ng  
RT: 21.40 min Scan# 3130  
Delta R.T. -0.01 min  
Lab File: BN003530.D  
Acq: 14 Nov 2018 01:58




Instrument :  
BNA\_N  
ClientSampleId :  
110918-JETT-F-U-S


Tgt Ion:240 Resp: 410041  
Ion Ratio Lower Upper  
240 100  
120 11.4 9.1 13.7  
236 25.9 20.6 30.8

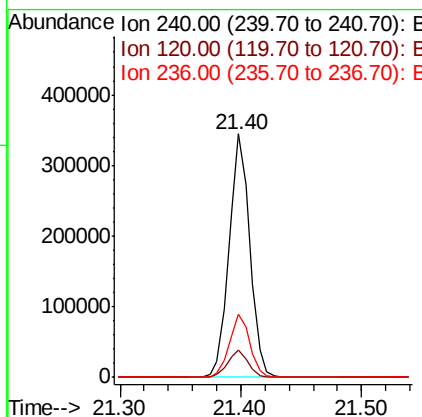

#79  
Terphenyl-d14  
Concen: 96.323 ng  
RT: 19.84 min Scan# 2865  
Delta R.T. -0.01 min  
Lab File: BN003530.D  
Acq: 14 Nov 2018 01:58

Tgt Ion:244 Resp: 2006183  
Ion Ratio Lower Upper  
244 100  
212 6.7 5.4 8.0  
122 11.0 8.2 12.2

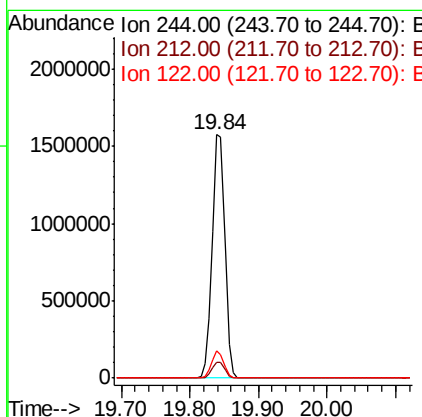

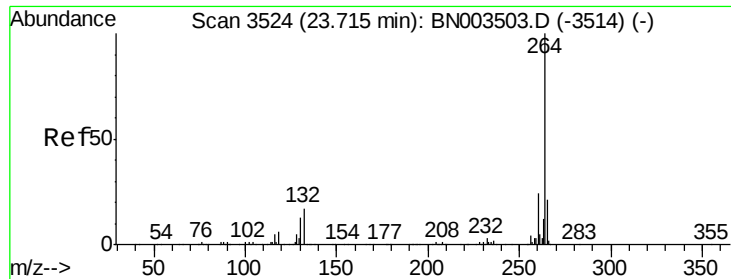

#87  
Perylene-d12  
Concen: 20.000 ng  
RT: 23.71 min Scan# 3523  
Delta R.T. -0.01 min  
Lab File: BN003530.D  
Acq: 14 Nov 2018 01:58

Instrument :  
BNA\_N  
ClientSampleId :  
110918-JETT-F-U-S

Tgt Ion: 264 Resp: 414511  
Ion Ratio Lower Upper  
264 100  
260 23.6 18.8 28.2  
265 22.0 17.2 25.8

