
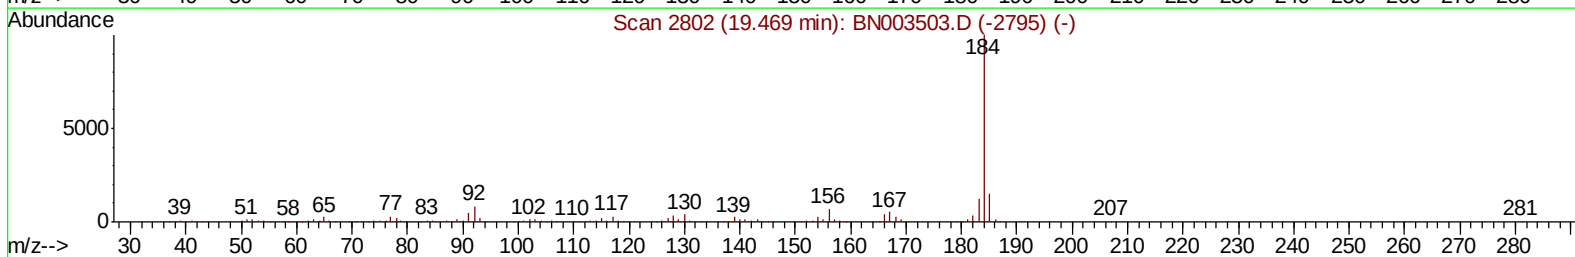
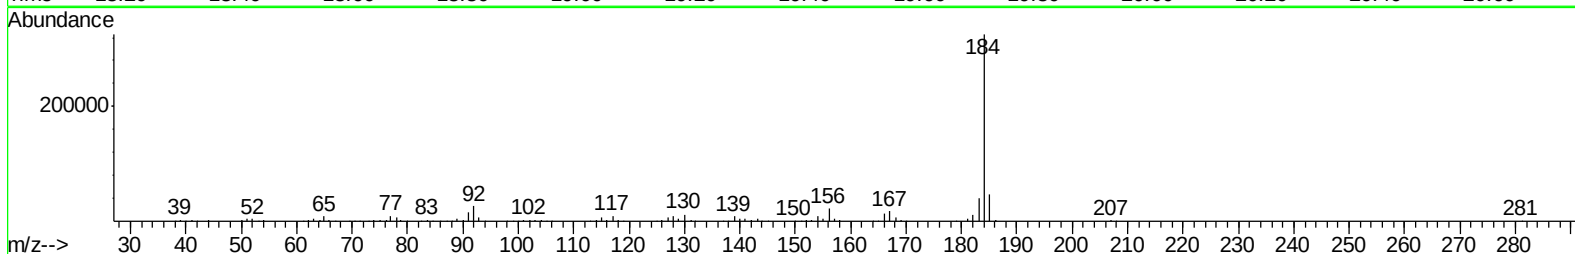


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111318\
Data File : BN003513.D
Acq On : 13 Nov 2018 16:00
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 04:14:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 15:59:25 2018
Response via : Initial Calibration

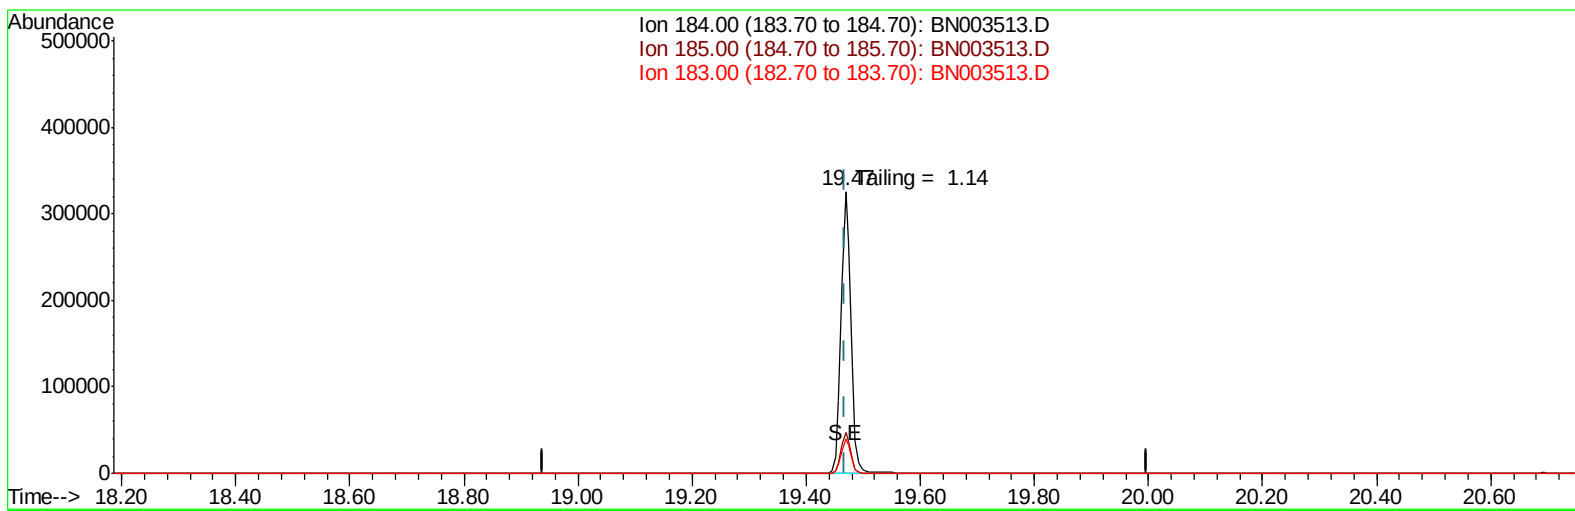

TIC: BN003513.D

(77) Benzidine




19.469min (+0.000) 0.00ng

response 394591

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.51
183.00	12.40	12.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111318\
Data File : BN003513.D
Acq On : 13 Nov 2018 16:00
Operator : MJ/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 04:14:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 15:59:25 2018
Response via : Initial Calibration

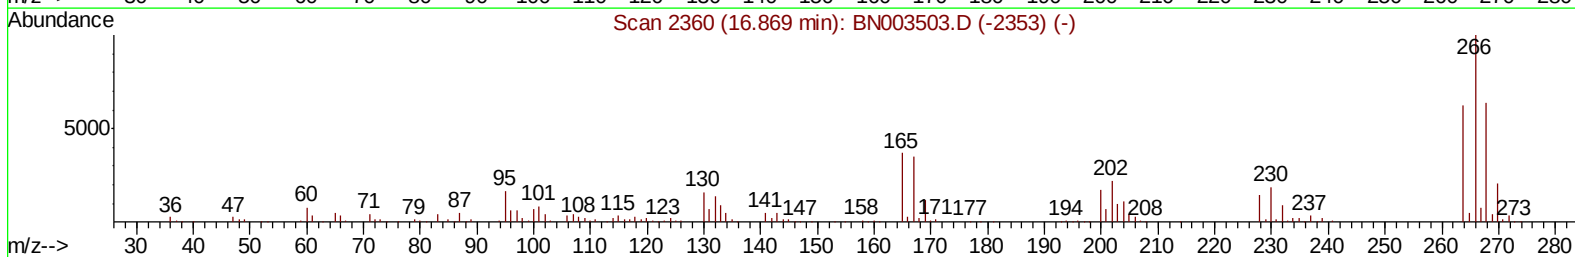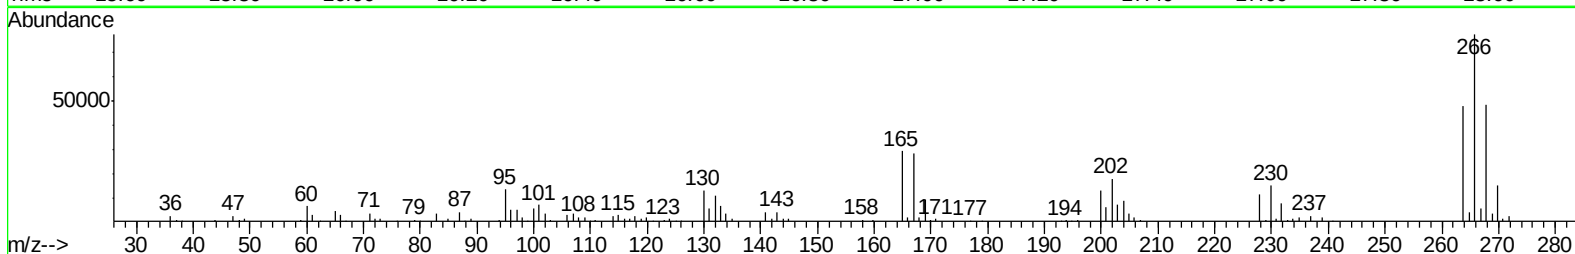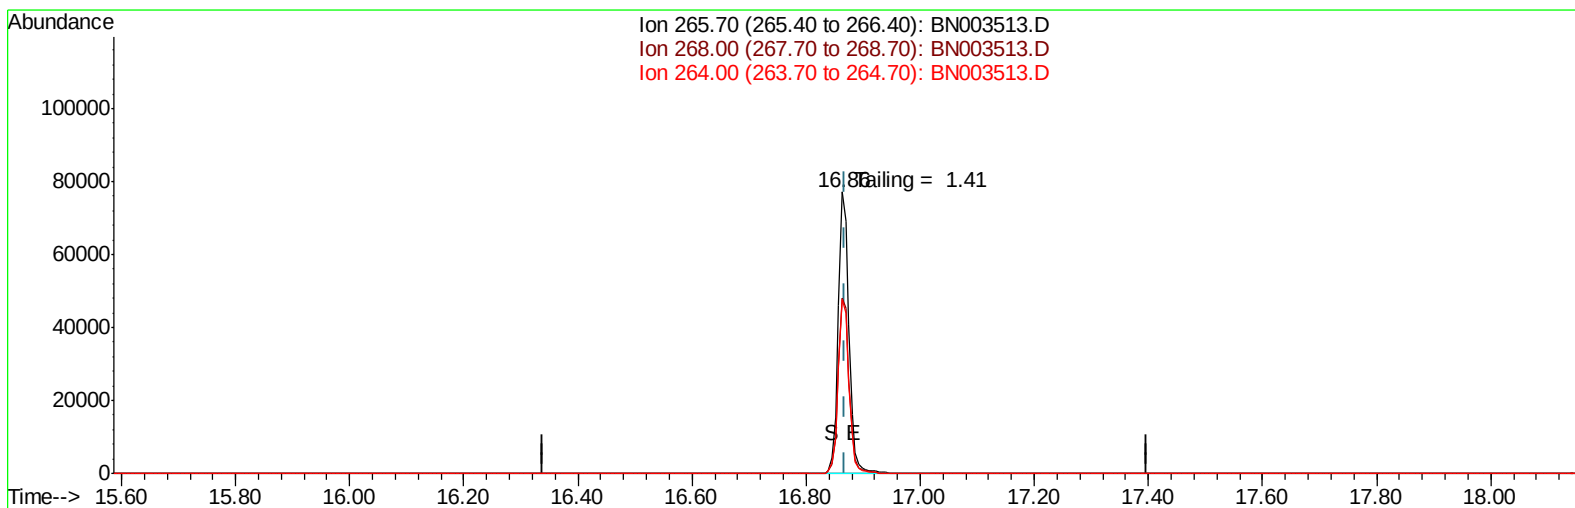

TIC: BN003513.D

(70) Pentachlorophenol (C)

16.863min (-0.006) 33810.35ng

response 99906

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	62.22
264.00	62.60	61.82
0.00	0.00	0.00