


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111318\
 Data File : BN003513.D
 Acq On : 13 Nov 2018 16:00
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 15:59:25 2018

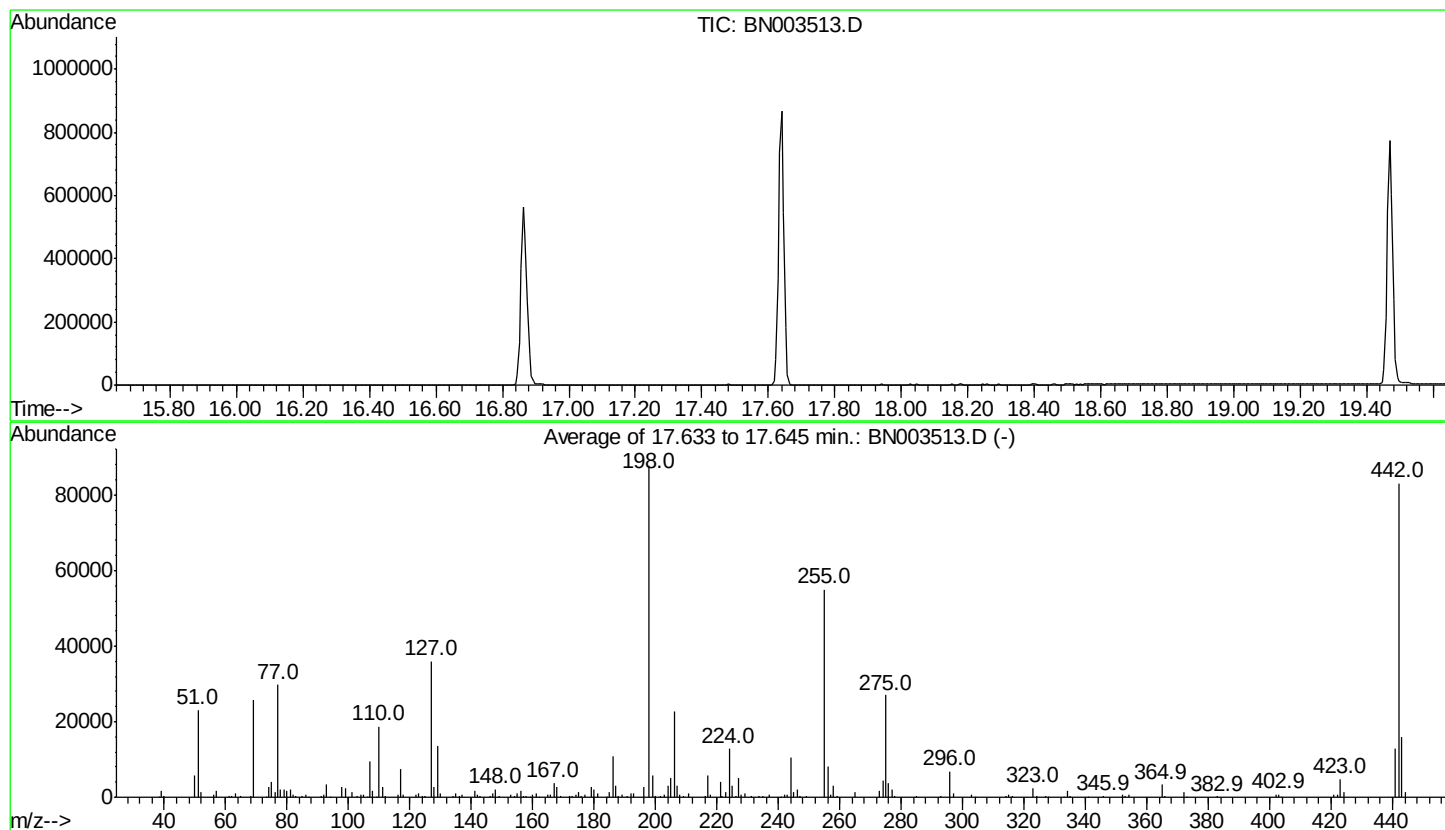

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	23100	PASS
68	69	0.00	2	2.0	503	PASS
69	198	0.00	100	29.4	25758	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	36018	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87744	PASS
199	198	5	9	6.7	5886	PASS
275	198	10	60	30.8	27013	PASS
365	198	1	100	3.9	3382	PASS
441	198	0.01	100	14.5	12728	PASS
442	198	50	100	94.7	83130	PASS
443	442	15	24	19.3	16053	PASS