

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111323\
 Data File : BN028582.D
 Acq On : 13 Nov 2023 13:59
 Operator : MA/JU
 Sample : 05337-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDH6

Quant Time: Nov 13 14:43:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	9586	0.400	ng/ul	0.00
4) Naphthalene-d8	10.489	136	30973	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.348	164	18233	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.098	188	41074	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	28622	0.400	ng/ul	0.00
23) Perylene-d12	23.615	264	28024	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	30898	2.916	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.084	152	9218	0.198	ng/ul	-0.01
18) Fluoranthene-d10	19.135	212	26802	0.291	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.184	88	2252	0.192	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111323\
Data File : BN028582.D
Acq On : 13 Nov 2023 13:59
Operator : MA/JU
Sample : 05337-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GCDH6


Quant Time: Nov 13 14:43:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

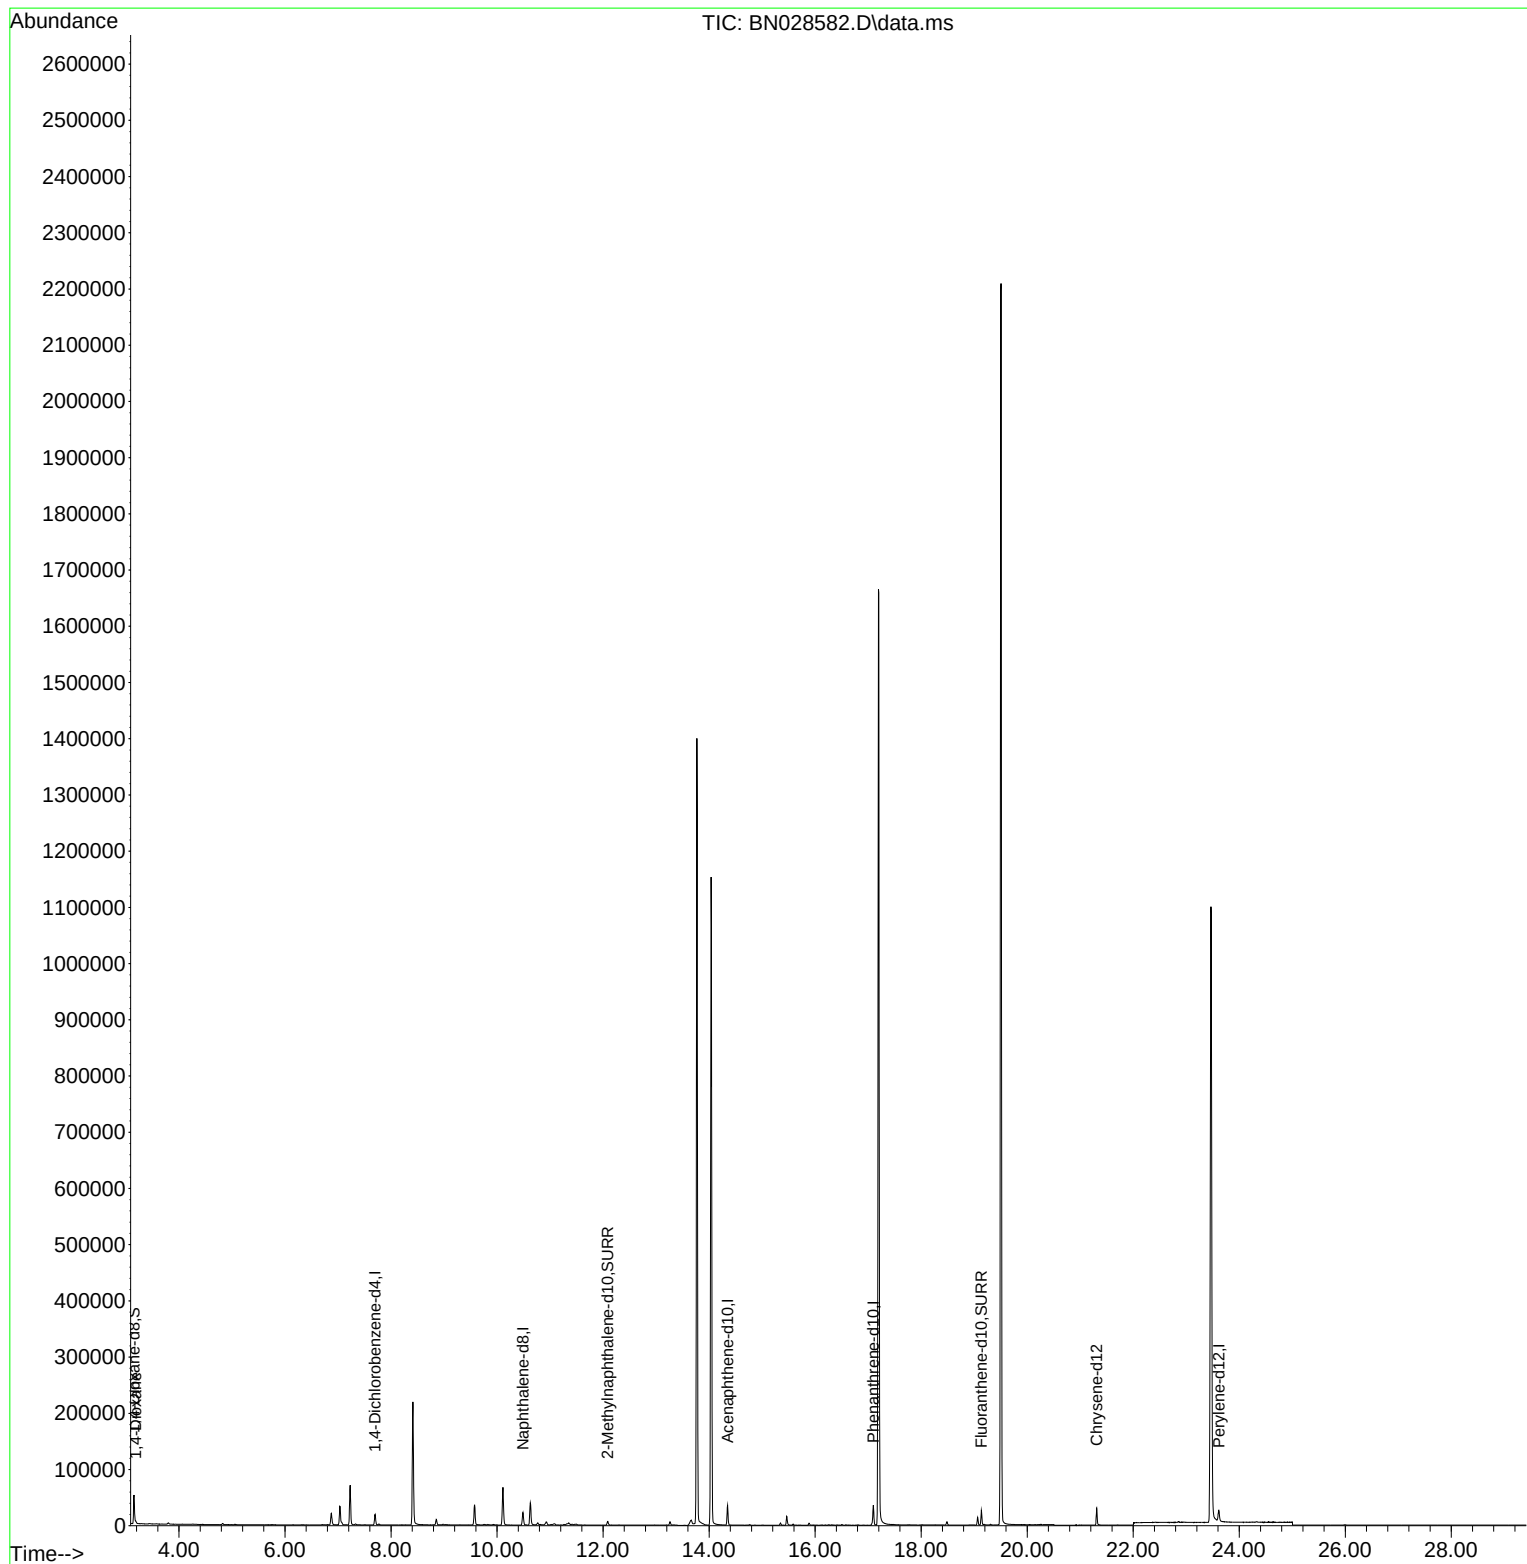

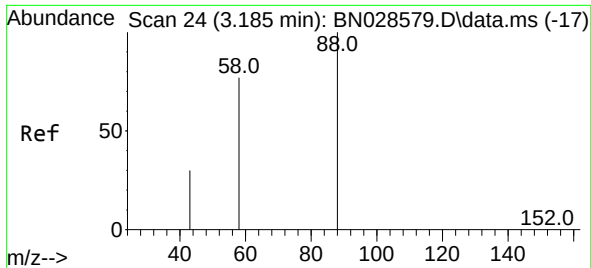

#2
 1,4-Dioxane
 Concen: 0.192 ng/ul
 RT: 3.184 min Scan# 24
 Delta R.T. -0.004 min
 Lab File: BN028582.D
 Acq: 13 Nov 2023 13:59

Instrument :
 BNA_N
 ClientSampleId :
 GCDH6

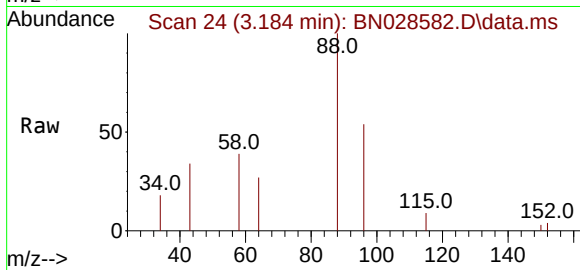

Tgt Ion: 88 Resp: 2252

Ion	Ratio	Lower	Upper
88	100		
43	33.9	32.9	49.3
58	38.6	41.8	62.8

