

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111323\
 Data File : BN028584.D
 Acq On : 13 Nov 2023 15:12
 Operator : MA/JU
 Sample : 05337-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GCDH8


Quant Time: Nov 13 15:39:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 09 16:30:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	7288	0.400	ng/u1	0.00
4) Naphthalene-d8	10.491	136	23253	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.349	164	13795	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.099	188	30070	0.400	ng/u1	0.00
17) Chrysene-d12	21.312	240	20539	0.400	ng/u1	0.00
23) Perylene-d12	23.612	264	21040	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	28561	3.546	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.086	152	11316	0.323	ng/u1	0.00
18) Fluoranthene-d10	19.137	212	33230	0.503	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.189	88	2024	0.227	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 13 15:39:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Nov 09 16:30:32 2023
Response via : Initial Calibration

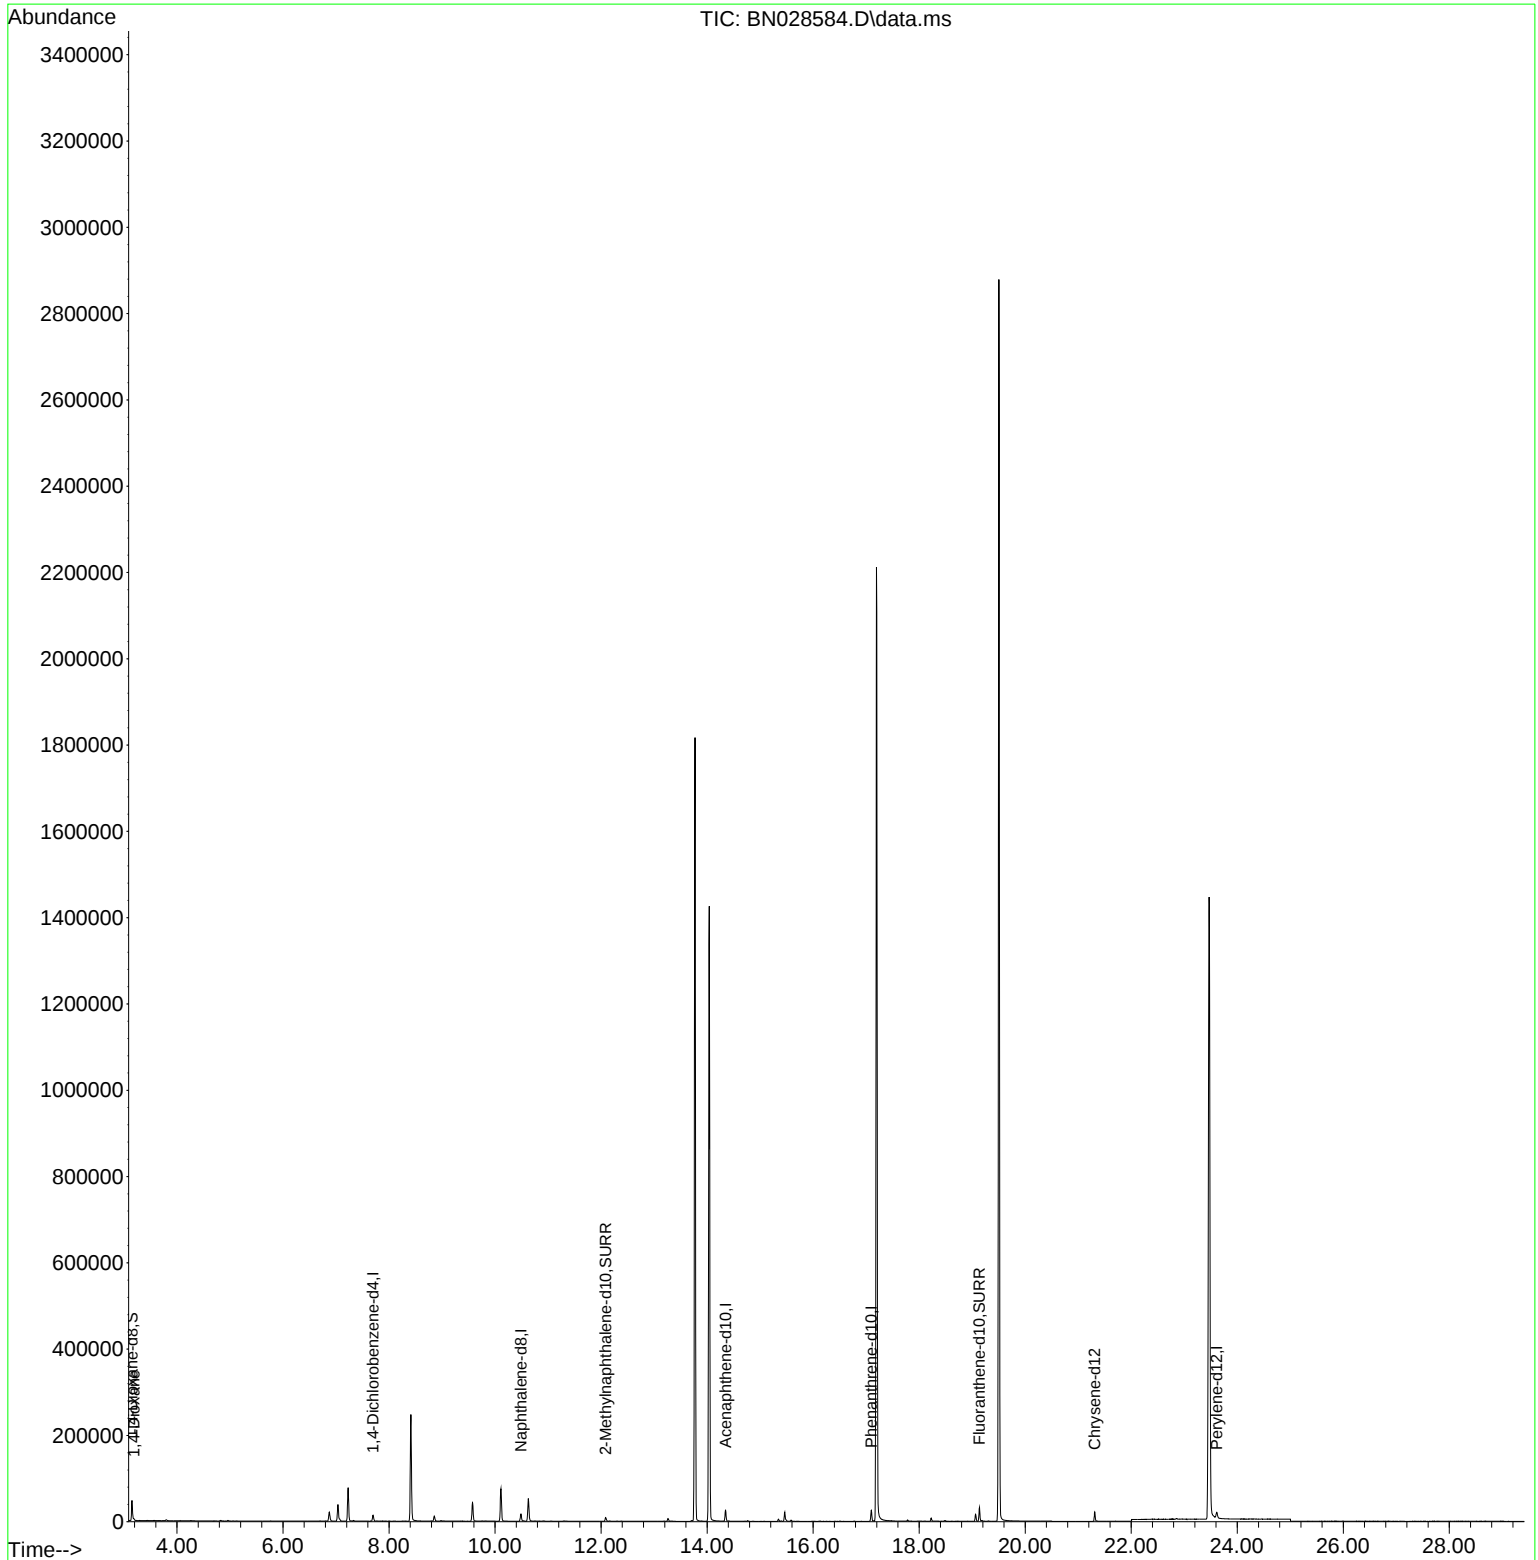

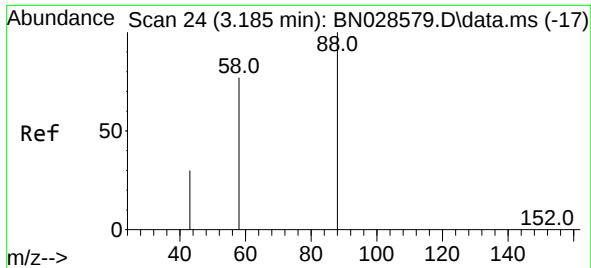

#2
 1,4-Dioxane
 Concen: 0.227 ng/ul
 RT: 3.189 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN028584.D
 Acq: 13 Nov 2023 15:12

Instrument :
 BNA_N
 ClientSampleId :
 GCDH8

Tgt Ion: 88 Resp: 2024

Ion	Ratio	Lower	Upper
88	100		
43	45.2	32.9	49.3
58	54.1	41.8	62.8

