
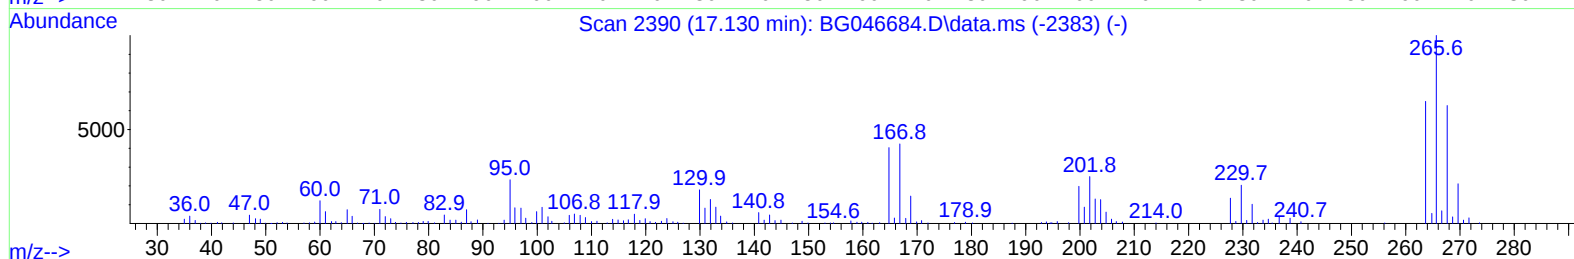
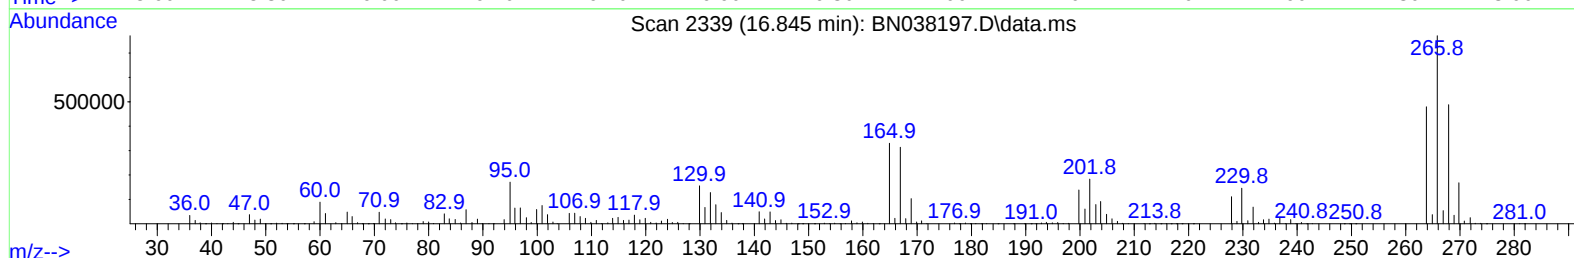


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111325\
Data File : BN038197.D
Acq On : 13 Nov 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 17:42:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 13 17:42:14 2025
Response via : Initial Calibration

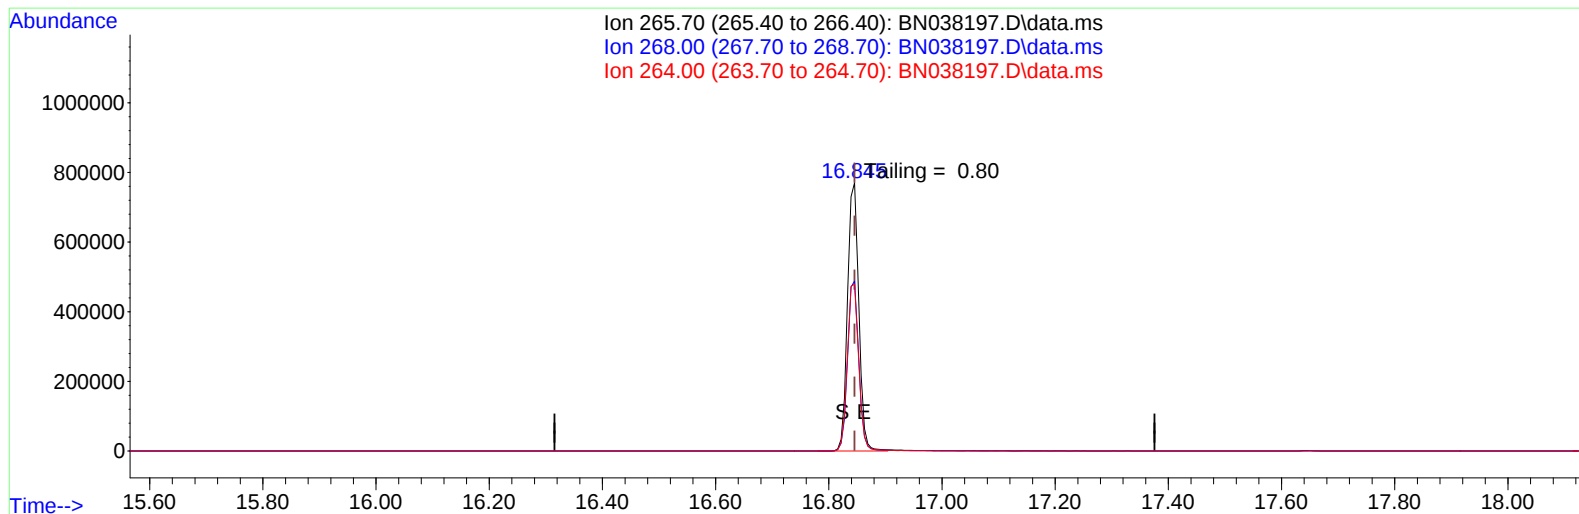

TIC: BN038197.D\data.ms

(70) Pentachlorophenol (C)




16.845min (0.000) 277.89 ng

response 1078097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.33
264.00	61.60	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111325\
Data File : BN038197.D
Acq On : 13 Nov 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 17:42:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 13 17:42:14 2025
Response via : Initial Calibration

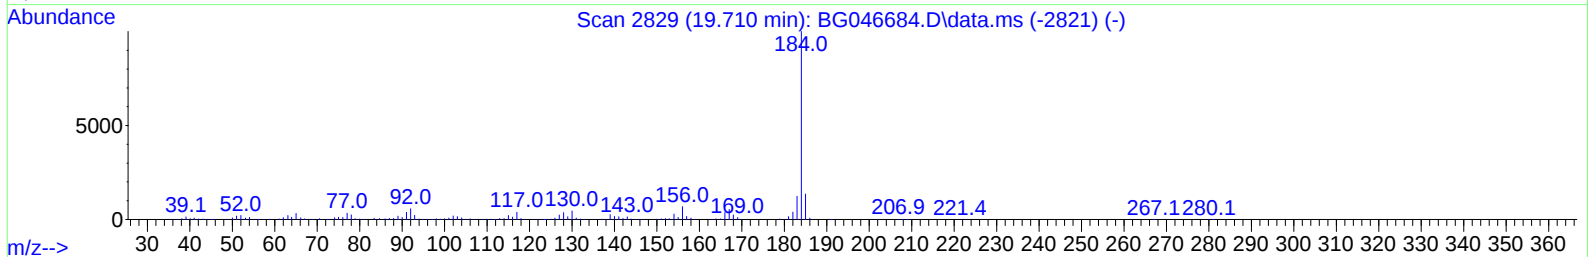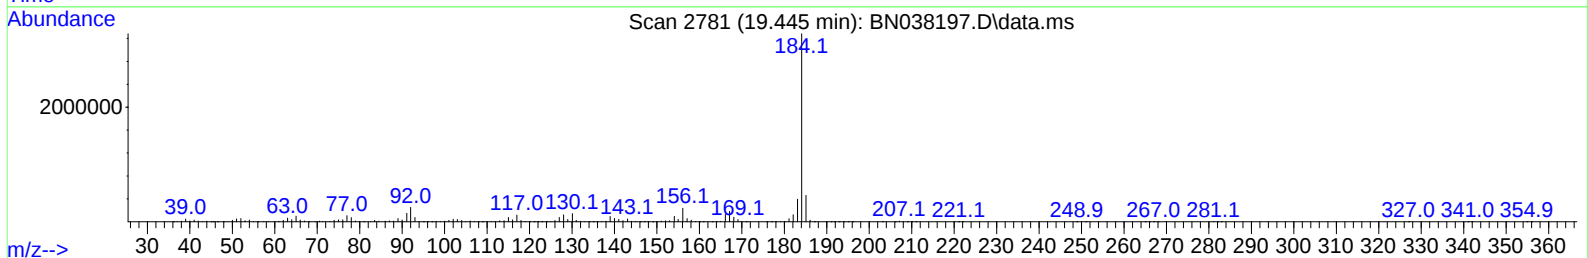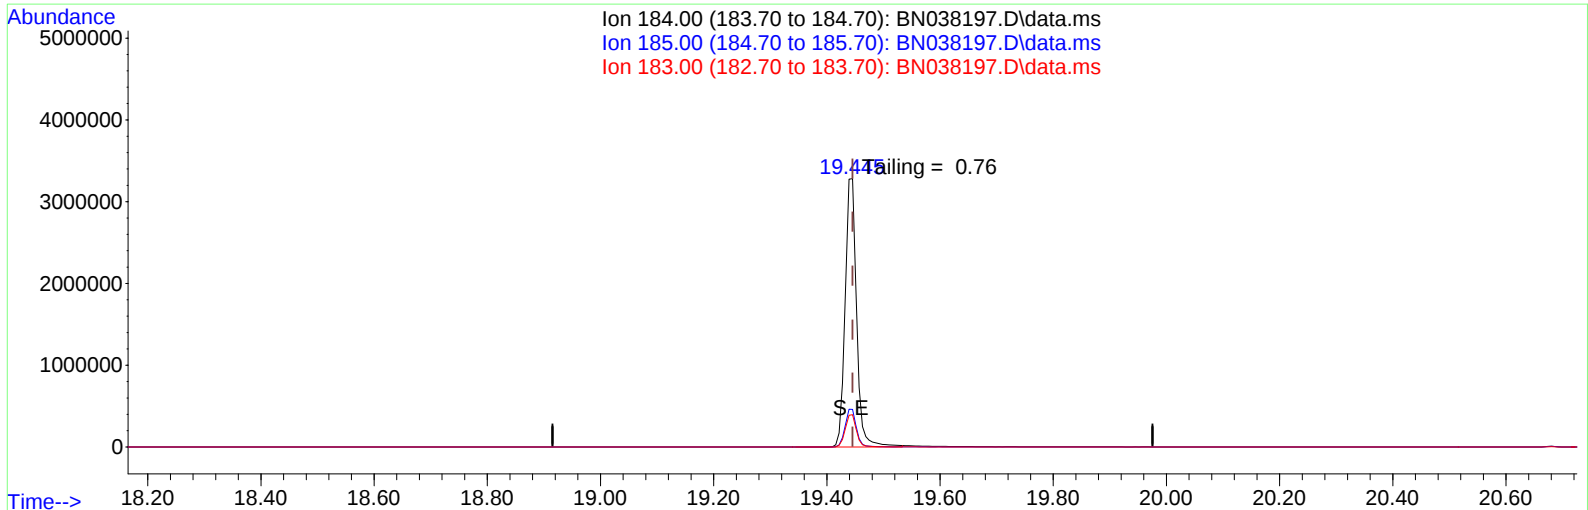

TIC: BN038197.D\data.ms

(77) Benzidine

19.445min (0.000) 0.00 ng

response 4694755

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	12.05
0.00	0.00	0.00