
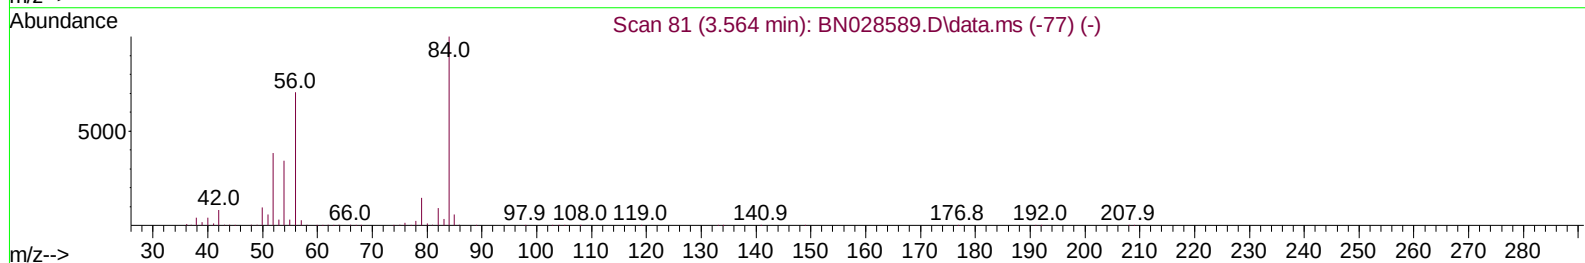
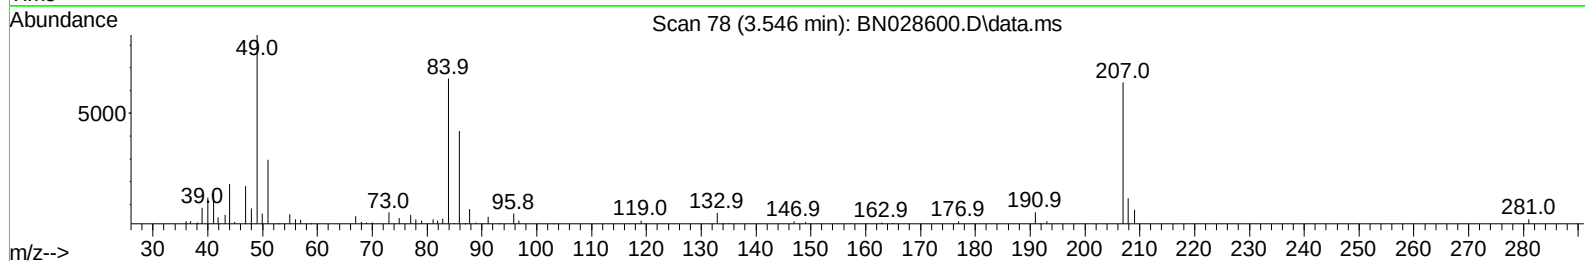


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 14 15:21:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 04:50:19 2023
Response via : Initial Calibration

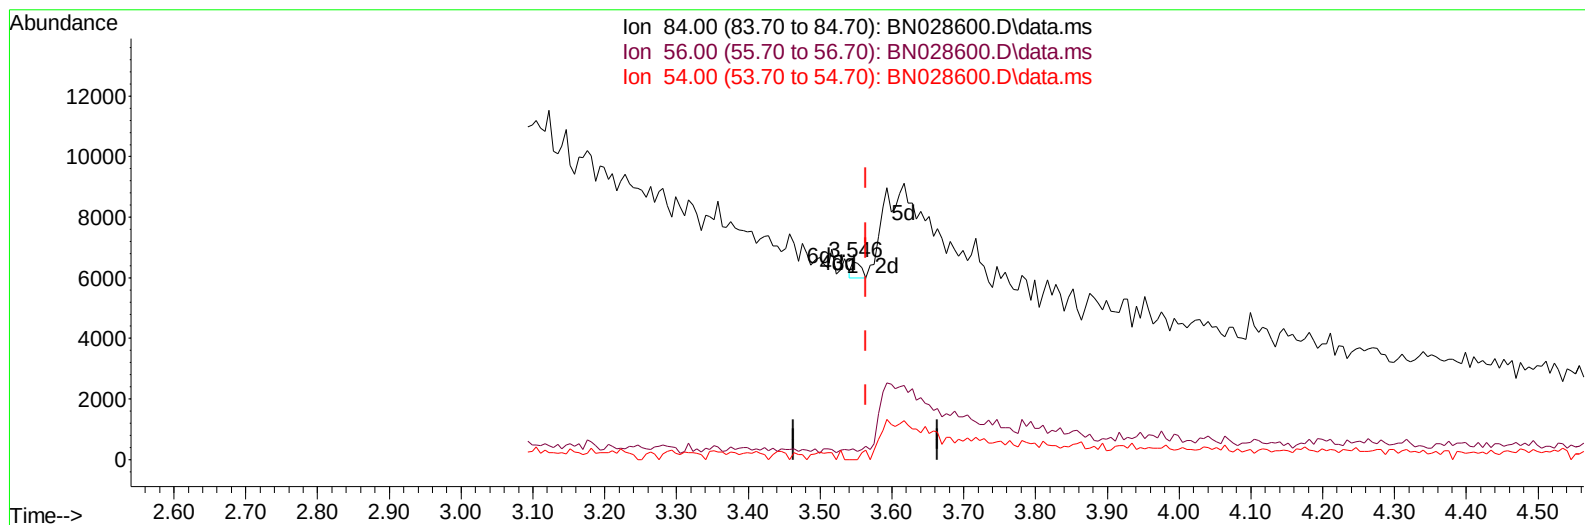

TIC: BN028600.D\data.ms

(4) Pyridine-d5 (S)




3.546min (-0.018) 0.04 ng/u1

response 473

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.50	5.49#
54.00	32.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028600.D
 Acq On : 14 Nov 2023 13:34
 Operator : MA/JU
 Sample : 05281-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 14 15:21:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 04:50:19 2023
 Response via : Initial Calibration

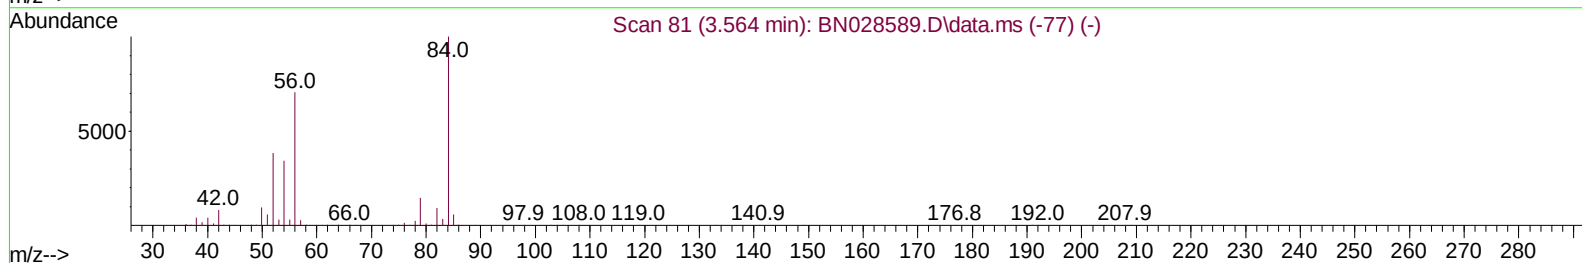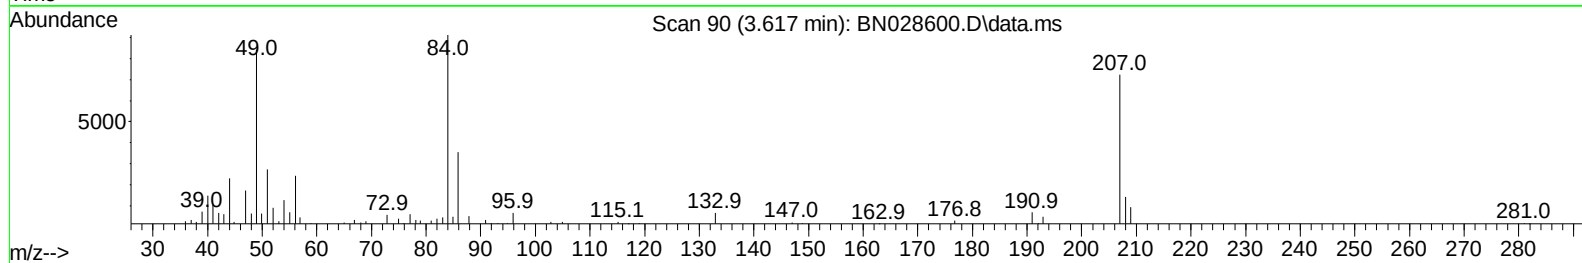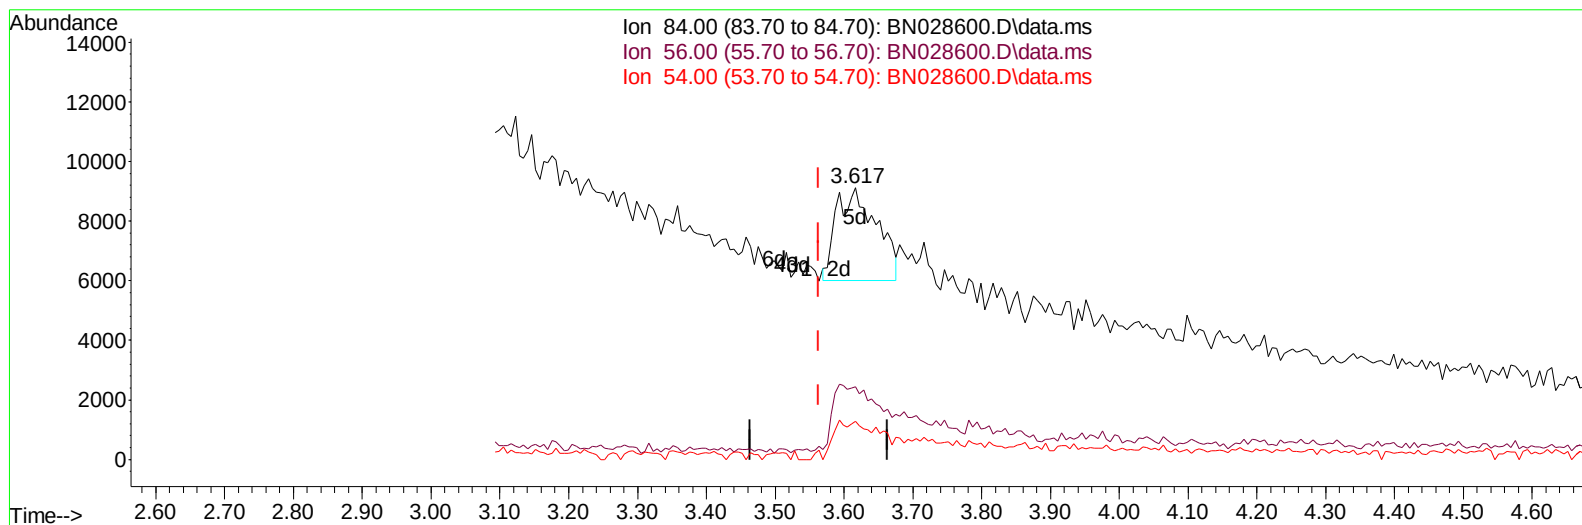

TIC: BN028600.D\data.ms

(4) Pyridine-d5 (S)**3.617min (+ 0.053) 1.07 ng/ul m****response 12479**

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.50	26.82#
54.00	32.50	13.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028600.D
 Acq On : 14 Nov 2023 13:34
 Operator : MA/JU
 Sample : 05281-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 14 15:22:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 04:50:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	191096	20.000	ng/ul	0.00
20) Naphthalene-d8	10.487	136	1096362	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.345	164	771641	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	1612282	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1309991	20.000	ng/ul	0.00
88) Perylene-d12	23.604	264	1358657	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	18228	3.415	ng/uL	0.00
4) Pyridine-d5	3.617	84	12479m	1.067	ng/ul	0.05
7) Phenol-d5	6.940	99	34466	1.888	ng/ul	0.05
9) Bis-(2-Chloroethyl)eth...	7.046	67	301070	26.663	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	313047	19.621	ng/ul	0.00
15) 4-Methylphenol-d8	8.434	113	114184	7.596	ng/ul	0.00
21) Nitrobenzene-d5	8.863	128	199552	20.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.581	143	205319	19.925	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	287070	16.385	ng/ul	0.00
31) 4-Chloroaniline-d4	10.657	131	370325	13.947	ng/ul	0.01
46) Dimethylphthalate-d6	13.763	166	2317300	33.306	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	2302526	28.713	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.340	176	1866590	32.541	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	224951	25.117	ng/ul	0.00
73) Anthracene-d10	17.192	188	3387140	37.635	ng/ul	0.00
81) Pyrene-d10	19.498	212	3992783	40.187	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.463	264	3402880	40.007	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 14 15:22:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 04:50:19 2023
Response via : Initial Calibration

