

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028603.D
 Acq On : 14 Nov 2023 15:22
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Quant Time: Nov 14 16:43:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 04:50:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.704	152	132788	20.000	ng/u1	0.00
20) Naphthalene-d8	10.487	136	743081	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.345	164	466104	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	949744	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	745839	20.000	ng/u1	# 0.00
88) Perylene-d12	23.604	264	893569	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	29465	7.945	ng/uL	0.00
4) Pyridine-d5	3.575	84	52055	6.403	ng/u1	0.01
7) Phenol-d5	6.934	99	57675	4.547	ng/u1	0.05
9) Bis-(2-Chloroethyl)eth...	7.040	67	393816	50.192	ng/u1	0.00
11) 2-Chlorophenol-d4	7.234	132	409277	36.917	ng/u1	0.00
15) 4-Methylphenol-d8	8.434	113	147160	14.088	ng/u1	0.00
21) Nitrobenzene-d5	8.863	128	247969	37.167	ng/u1	0.00
24) 2-Nitrophenol-d4	9.581	143	244297	34.979	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	365609	30.789	ng/u1	0.00
31) 4-Chloroaniline-d4	10.651	131	508475	28.255	ng/u1	0.00
46) Dimethylphthalate-d6	13.763	166	2085002	49.611	ng/u1	0.00
49) Acenaphthylene-d8	14.033	160	2350274	48.521	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/u1	
60) Fluorene-d10	15.339	176	1761551	50.840	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	177960	33.732	ng/u1	0.00
73) Anthracene-d10	17.192	188	2565794	48.397	ng/u1	0.00
81) Pyrene-d10	19.498	212	3156033	55.792	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.462	264	2924430	52.277	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.181	88	4907	1.239	ng/uL#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028603.D
Acq On : 14 Nov 2023 15:22
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Time: Nov 14 16:43:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 04:50:19 2023
Response via : Initial Calibration

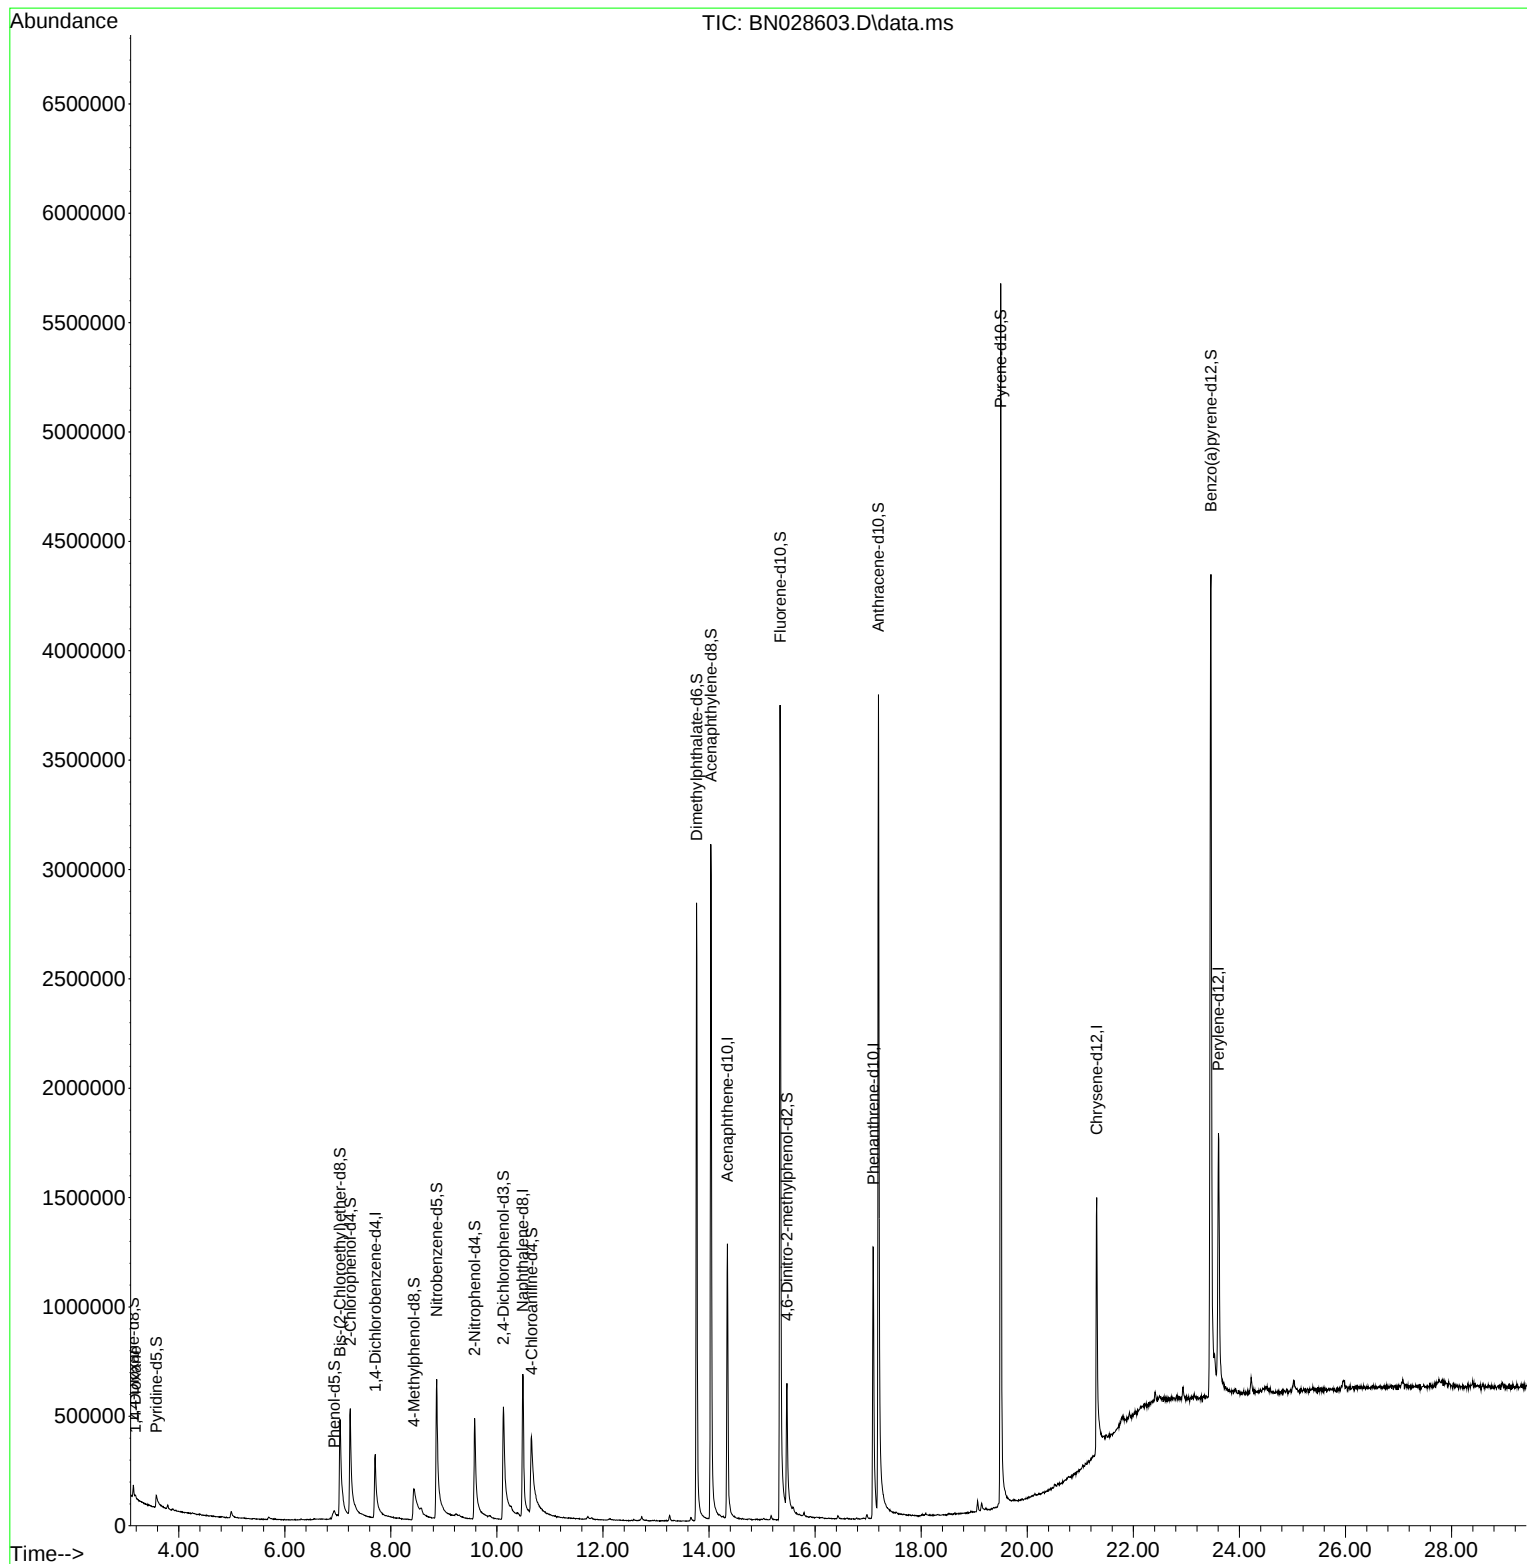

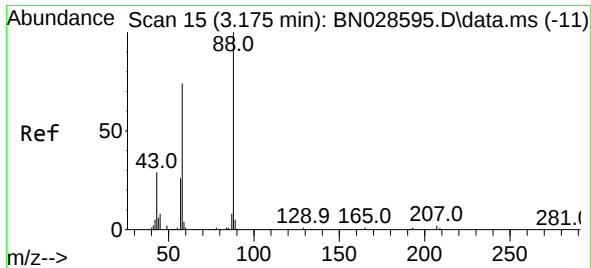

#2
 1,4-Dioxane
 Concen: 1.239 ng/uL
 RT: 3.181 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: BN028603.D
 Acq: 14 Nov 2023 15:22

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Tgt Ion: 88 Resp: 4907
 Ion Ratio Lower Upper
 88 100
 43 27.5 25.3 37.9
 58 43.9 56.8 85.2#

