

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028596.D
 Acq On : 14 Nov 2023 11:09
 Operator : MA/JU
 Sample : PB156978BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK978

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	19	rVB	70896	104965	1.28%	0.142%
2	3.564	77	81	107	rBV	370527	982626	11.96%	1.329%
3	6.887	639	646	667	rBV	353875	1326505	16.14%	1.794%
4	7.040	667	672	699	rVV	499035	1365842	16.62%	1.847%
5	7.234	699	705	738	rVB	593227	1585815	19.29%	2.144%
6	7.699	777	784	814	rBV	471151	1321960	16.08%	1.788%
7	8.428	901	908	927	rBV	502146	1734324	21.10%	2.345%
8	8.863	975	982	1010	rBV	600207	1709733	20.80%	2.312%
9	9.581	1095	1104	1125	rBV	438386	1244921	15.15%	1.683%
10	10.122	1189	1196	1218	rBV	513871	1707451	20.77%	2.309%
11	10.487	1251	1258	1276	rBV	1016582	2202105	26.79%	2.978%
12	10.646	1279	1285	1319	rVV	500543	1901292	23.13%	2.571%
13	11.710	1462	1466	1471	rBV6	11588	25061	0.30%	0.034%
14	12.734	1632	1640	1652	rBV3	22772	55430	0.67%	0.075%
15	13.257	1724	1729	1735	rBV	27838	48028	0.58%	0.065%
16	13.657	1792	1797	1807	rVB2	24540	44725	0.54%	0.060%
17	13.769	1809	1816	1832	rBV	2696776	4307328	52.41%	5.824%
18	14.034	1854	1861	1891	rBV2	2926189	5093485	61.97%	6.887%
19	14.269	1899	1901	1906	rVB5	7728	10604	0.13%	0.014%
20	14.345	1907	1914	1930	rBV	2089413	3450378	41.98%	4.666%
21	14.634	1954	1963	1967	rBV4	68340	218034	2.65%	0.295%
22	15.169	2050	2054	2060	rVB2	26154	38567	0.47%	0.052%
23	15.339	2077	2083	2100	rBV	3678744	6272529	76.32%	8.482%
24	15.469	2100	2105	2121	rVB	554290	1140801	13.88%	1.543%
25	15.786	2157	2159	2165	rVB	21249	31166	0.38%	0.042%
26	16.434	2264	2269	2275	rBV4	15502	25272	0.31%	0.034%
27	16.975	2357	2361	2367	rVB4	17011	28203	0.34%	0.038%
28	17.092	2375	2381	2392	rBV	2417250	4086409	49.72%	5.526%
29	17.192	2392	2398	2431	rVB	3790076	6955750	84.63%	9.405%
30	18.016	2535	2538	2543	rBV6	8044	12492	0.15%	0.017%
31	19.063	2711	2716	2724	rBV3	51926	102696	1.25%	0.139%
32	19.139	2726	2729	2739	rVB	31242	67583	0.82%	0.091%
33	19.498	2784	2790	2811	rBV2	5432837	8218923	100.00%	11.114%
34	21.310	3093	3098	3119	rBV	2130455	4751313	57.81%	6.425%
35	23.463	3457	3464	3474	rBV	3436664	7350483	89.43%	9.939%
36	23.604	3482	3488	3506	rVB	1946183	4431486	53.92%	5.992%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028596.D
Acq On : 14 Nov 2023 11:09
Operator : MA/JU
Sample : PB156978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 73954285

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028596.D
Acq On : 14 Nov 2023 11:09
Operator : MA/JU
Sample : PB156978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

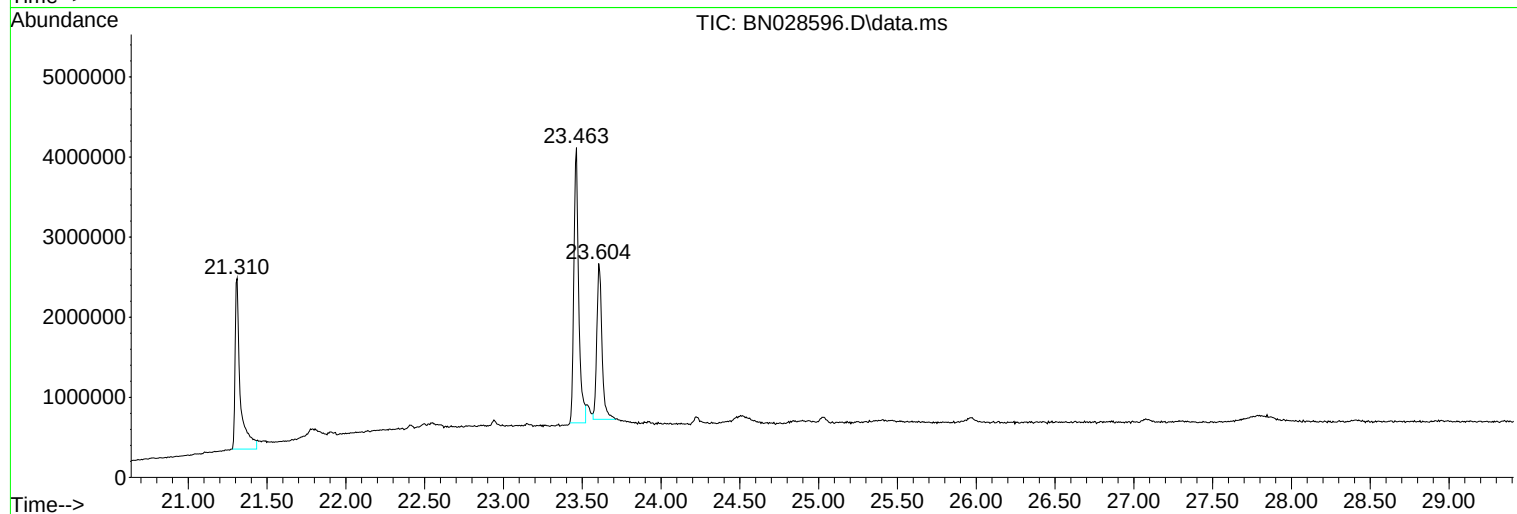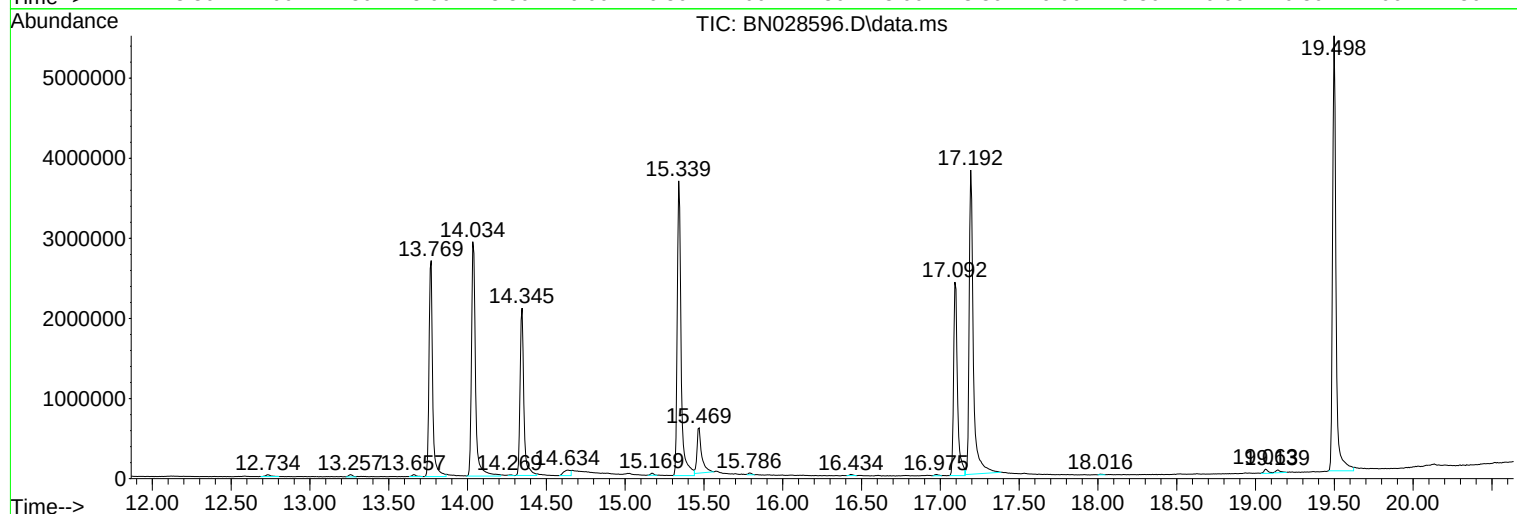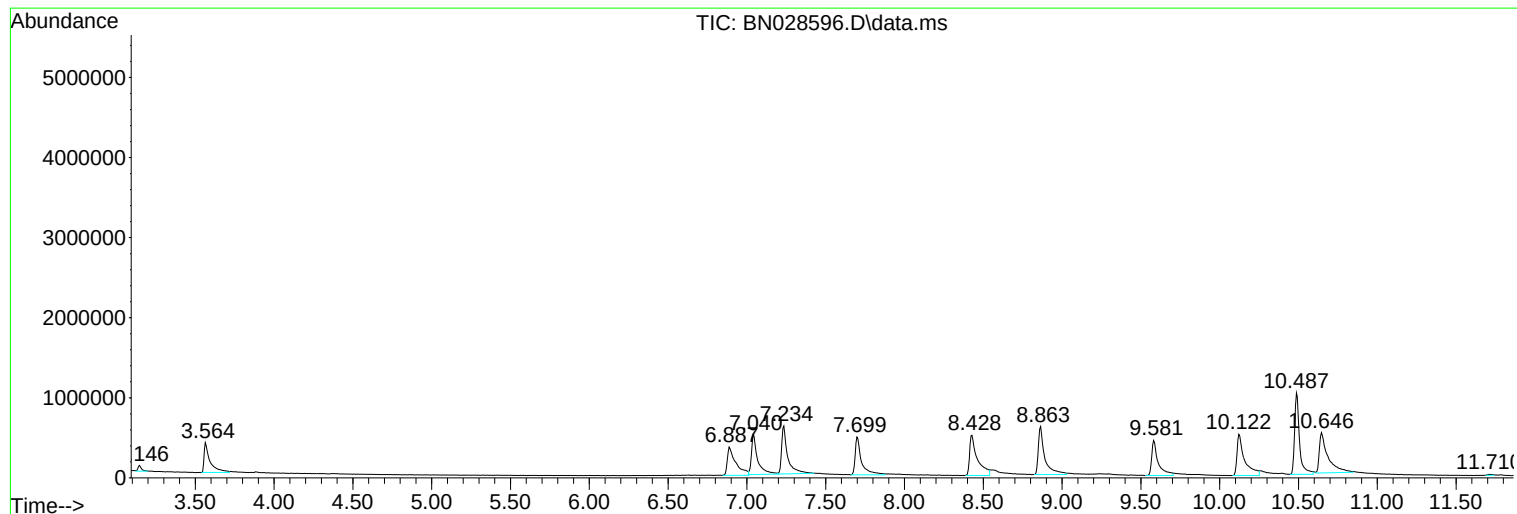

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028596.D
Acq On : 14 Nov 2023 11:09
Operator : MA/JU
Sample : PB156978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028596.D
Acq On : 14 Nov 2023 11:09
Operator : MA/JU
Sample : PB156978BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc