

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028597.D
 Acq On : 14 Nov 2023 11:46
 Operator : MA/JU
 Sample : PB156980BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK980

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	24	rVB	85647	139154	1.37%	0.153%
2	3.564	77	81	105	rBV	469642	1318277	12.96%	1.453%
3	4.381	216	220	223	rBV5	5737	10747	0.11%	0.012%
4	6.887	638	646	661	rBV	473596	1544288	15.18%	1.702%
5	7.040	667	672	698	rVB	627011	1493890	14.68%	1.647%
6	7.234	699	705	730	rBV	766304	1865821	18.34%	2.057%
7	7.699	777	784	814	rBV	525765	1452052	14.27%	1.601%
8	8.422	901	907	929	rBV	688253	2253942	22.16%	2.485%
9	8.863	975	982	1018	rBV	795282	2188696	21.51%	2.413%
10	9.581	1097	1104	1128	rBV	580348	1588059	15.61%	1.751%
11	10.122	1188	1196	1220	rBV	718048	2268602	22.30%	2.501%
12	10.487	1251	1258	1276	rBV	1125435	2444667	24.03%	2.695%
13	10.646	1279	1285	1320	rVV	672793	2433363	23.92%	2.682%
14	11.716	1460	1467	1474	rBV4	13216	35073	0.34%	0.039%
15	12.122	1528	1536	1537	rBV8	7847	18493	0.18%	0.020%
16	12.728	1631	1639	1652	rBV2	29728	77590	0.76%	0.086%
17	13.257	1723	1729	1737	rBV3	33491	61222	0.60%	0.067%
18	13.657	1793	1797	1807	rVB3	27871	53126	0.52%	0.059%
19	13.763	1809	1815	1837	rBV	3376061	5435935	53.43%	5.992%
20	14.034	1855	1861	1892	rBV	3582011	6243933	61.38%	6.883%
21	14.269	1898	1901	1907	rVB7	7934	12095	0.12%	0.013%
22	14.346	1907	1914	1936	rBV	2345319	3863436	37.98%	4.259%
23	14.610	1951	1959	1961	rBV2	118678	262593	2.58%	0.289%
24	15.022	2026	2029	2039	rVB4	22675	44485	0.44%	0.049%
25	15.175	2050	2055	2061	rVB	29674	43953	0.43%	0.048%
26	15.340	2077	2083	2099	rBV	4530659	7734790	76.03%	8.526%
27	15.469	2100	2105	2121	rVB	804380	1570355	15.44%	1.731%
28	15.793	2157	2160	2166	rVB	28348	39710	0.39%	0.044%
29	16.122	2213	2216	2223	rVB9	5514	11926	0.12%	0.013%
30	16.434	2265	2269	2273	rBV3	18400	24105	0.24%	0.027%
31	16.604	2294	2298	2302	rVB6	7671	12304	0.12%	0.014%
32	16.775	2324	2327	2334	rVB8	6119	11170	0.11%	0.012%
33	16.969	2357	2360	2367	rVB4	16356	24514	0.24%	0.027%
34	17.092	2375	2381	2393	rBV	2702847	4630552	45.52%	5.104%
35	17.192	2393	2398	2431	rVB	4847204	8529260	83.84%	9.402%
36	19.063	2712	2716	2722	rBV	57808	93614	0.92%	0.103%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028597.D
Acq On : 14 Nov 2023 11:46
Operator : MA/JU
Sample : PB156980BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK980

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2735	rBV	41048	78847	0.78%	0.087%
38	19.498	2784	2790	2812	rBV	6421379	10173352	100.00%	11.214%
39	21.310	3093	3098	3119	rBV	2640093	5189003	51.01%	5.720%
40	23.463	3457	3464	3481	rBV	4536815	10167674	99.94%	11.208%
41	23.610	3483	3489	3505	rVB	2340963	5271982	51.82%	5.811%




Sum of corrected areas: 90716650

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028597.D
Acq On : 14 Nov 2023 11:46
Operator : MA/JU
Sample : PB156980BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

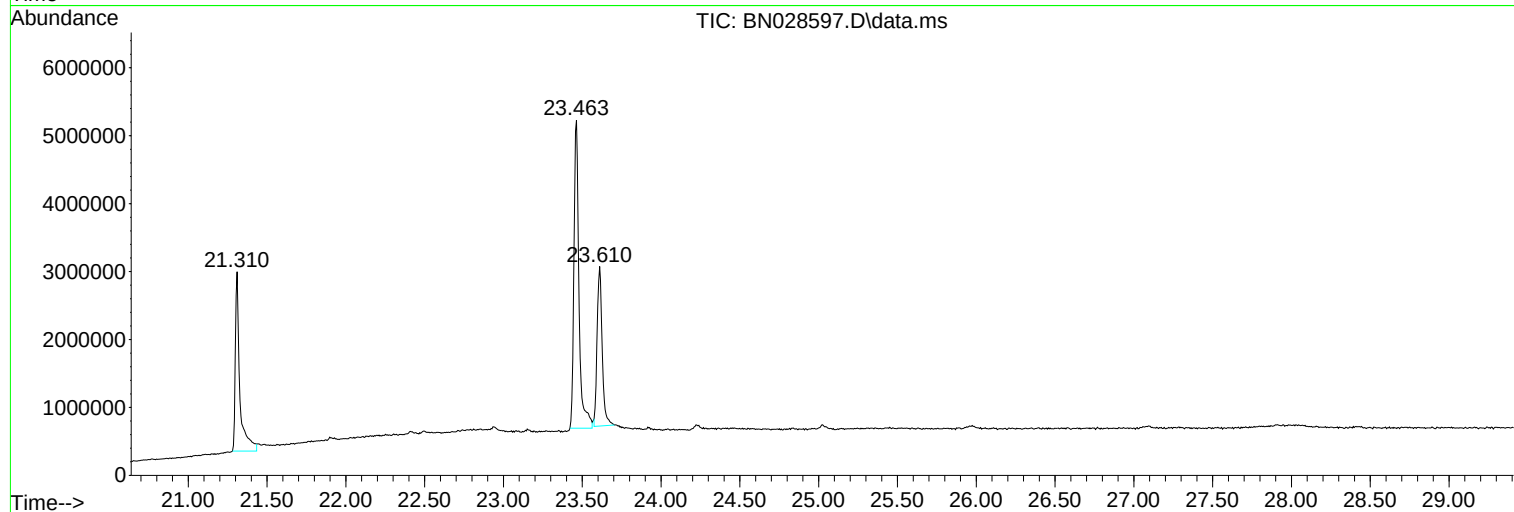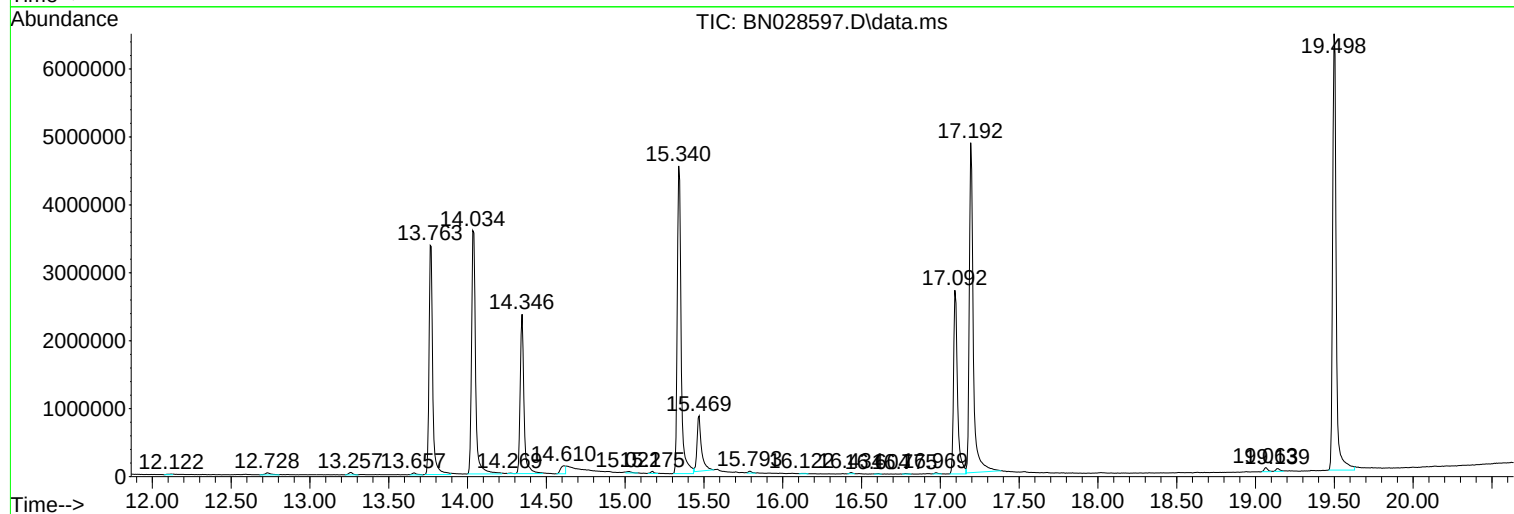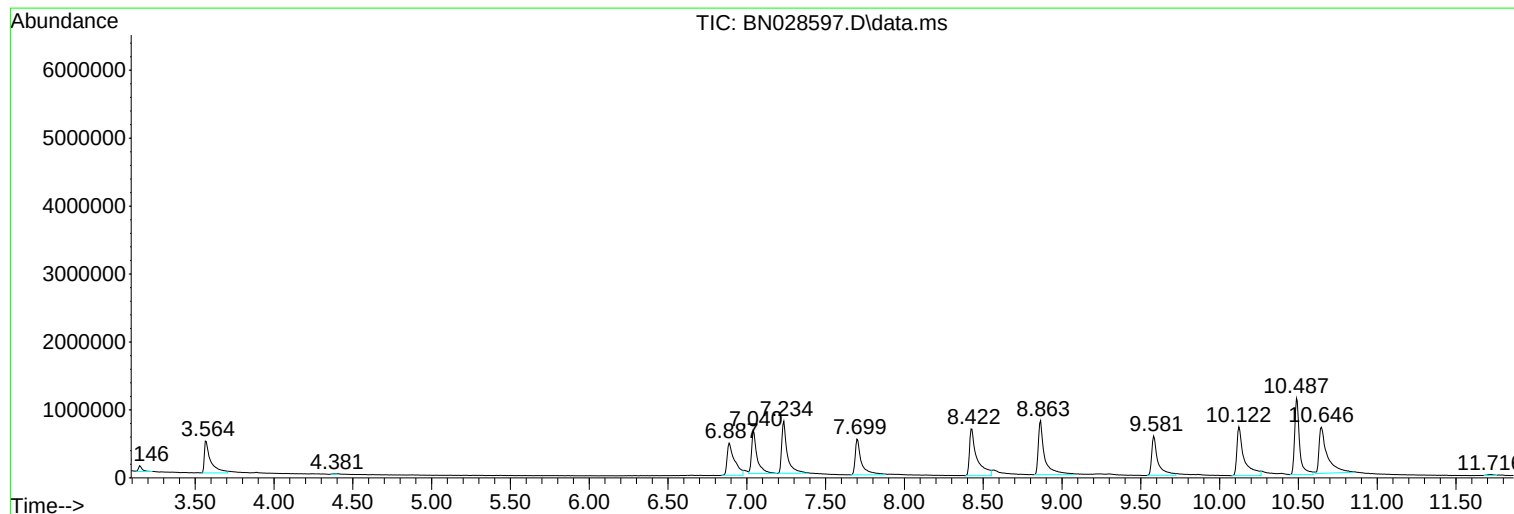

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028597.D
Acq On : 14 Nov 2023 11:46
Operator : MA/JU
Sample : PB156980BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028597.D
Acq On : 14 Nov 2023 11:46
Operator : MA/JU
Sample : PB156980BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc