

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028599.D
 Acq On : 14 Nov 2023 12:58
 Operator : MA/JU
 Sample : 05281-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	14	rBV	42985	53795	0.51%	0.064%
2	3.887	132	136	142	rBV2	12349	23028	0.22%	0.027%
3	6.852	635	640	644	rBV3	9278	17255	0.16%	0.020%
4	6.934	644	654	659	rBV3	37840	129437	1.23%	0.153%
5	7.040	667	672	699	rBV	462480	1269655	12.05%	1.503%
6	7.234	699	705	739	rVB	470638	1290104	12.24%	1.527%
7	7.699	777	784	819	rBV	594347	1680861	15.95%	1.989%
8	8.434	902	909	928	rBV	167586	786160	7.46%	0.930%
9	8.863	975	982	1019	rBV	697193	2071342	19.66%	2.451%
10	9.222	1040	1043	1048	rBV6	7175	14994	0.14%	0.018%
11	9.293	1053	1055	1061	rVB5	12825	16378	0.16%	0.019%
12	9.581	1097	1104	1132	rBV	516507	1486746	14.11%	1.760%
13	10.122	1189	1196	1217	rBV	564302	1814764	17.22%	2.148%
14	10.487	1251	1258	1276	rBV	1368030	2819634	26.76%	3.337%
15	10.657	1280	1287	1311	rVV	256354	1055480	10.02%	1.249%
16	11.722	1458	1468	1472	rBV6	12940	31436	0.30%	0.037%
17	12.116	1530	1535	1537	rBV6	6644	11451	0.11%	0.014%
18	12.581	1611	1614	1621	rVV8	5855	11644	0.11%	0.014%
19	12.734	1631	1640	1648	rBV3	23172	57563	0.55%	0.068%
20	12.957	1676	1678	1685	rVB8	5935	10791	0.10%	0.013%
21	13.257	1722	1729	1736	rBV2	27747	49409	0.47%	0.058%
22	13.657	1790	1797	1803	rBV2	22057	43550	0.41%	0.052%
23	13.769	1809	1816	1846	rBV	3522700	5634881	53.48%	6.669%
24	14.039	1855	1862	1887	rBV	3725270	6273796	59.54%	7.425%
25	14.345	1907	1914	1936	rBV	2719576	4442845	42.16%	5.258%
26	15.169	2048	2054	2060	rBV5	27353	49514	0.47%	0.059%
27	15.339	2077	2083	2100	rBV	4559281	7955390	75.50%	9.415%
28	15.469	2100	2105	2121	rVB	851371	1643156	15.59%	1.945%
29	15.792	2156	2160	2165	rVB2	21871	33123	0.31%	0.039%
30	16.428	2264	2268	2275	rBV5	14523	32640	0.31%	0.039%
31	16.886	2339	2346	2349	rBV7	6646	14782	0.14%	0.017%
32	16.975	2356	2361	2367	rVB4	19843	30048	0.29%	0.036%
33	17.092	2375	2381	2393	rBV	2914293	5132986	48.71%	6.075%
34	17.192	2393	2398	2425	rVB2	5078703	8892124	84.39%	10.524%
35	19.063	2712	2716	2722	rBV	64656	107392	1.02%	0.127%
36	19.139	2725	2729	2737	rVV	41116	78548	0.75%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028599.D
Acq On : 14 Nov 2023 12:58
Operator : MA/JU
Sample : 05281-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.457	2780	2783	2784	rBV3	25613	25151	0.24%	0.030%
38	19.498	2784	2790	2811	rVV	7064468	10537362	100.00%	12.471%
39	21.304	3092	3097	3114	rBV2	3005116	5278161	50.09%	6.247%
40	23.463	3457	3464	3474	rBV	4176464	8724594	82.80%	10.326%
41	23.604	3482	3488	3503	rVB	2203516	4861866	46.14%	5.754%




Sum of corrected areas: 84493836

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028599.D
Acq On : 14 Nov 2023 12:58
Operator : MA/JU
Sample : 05281-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

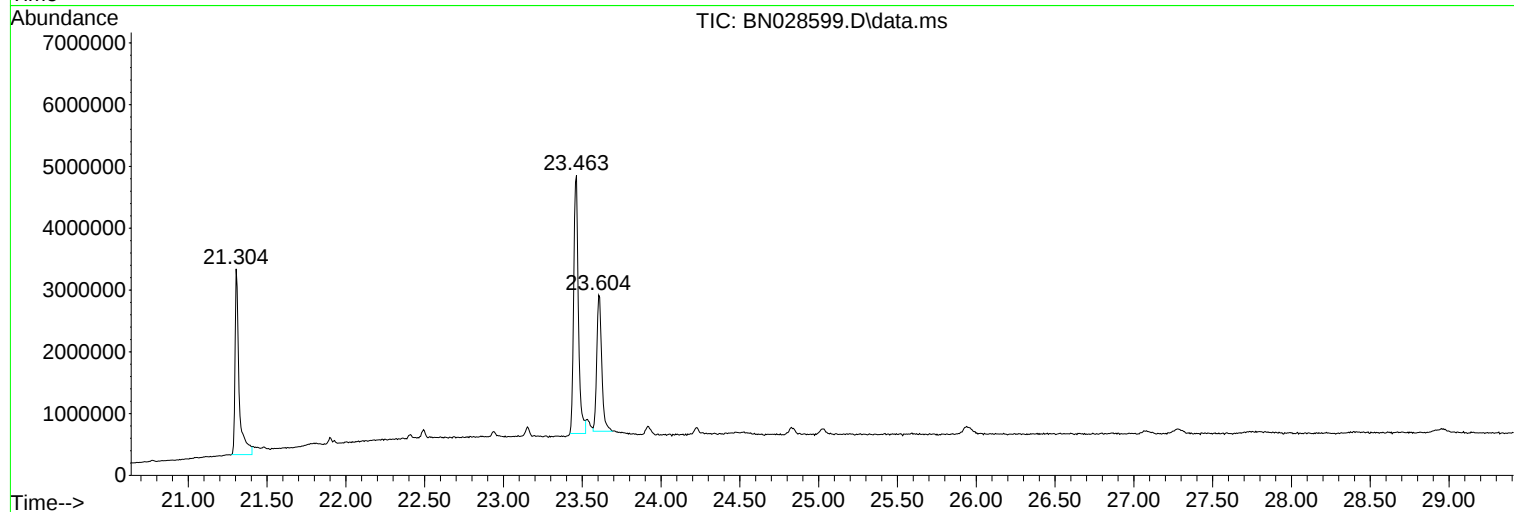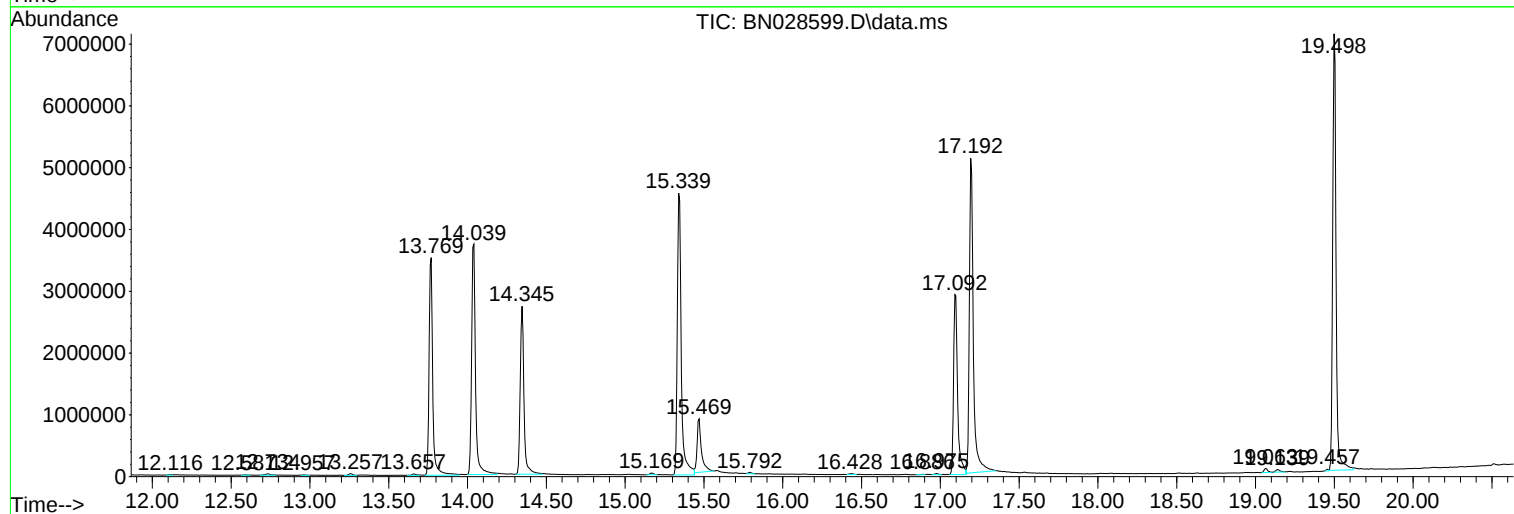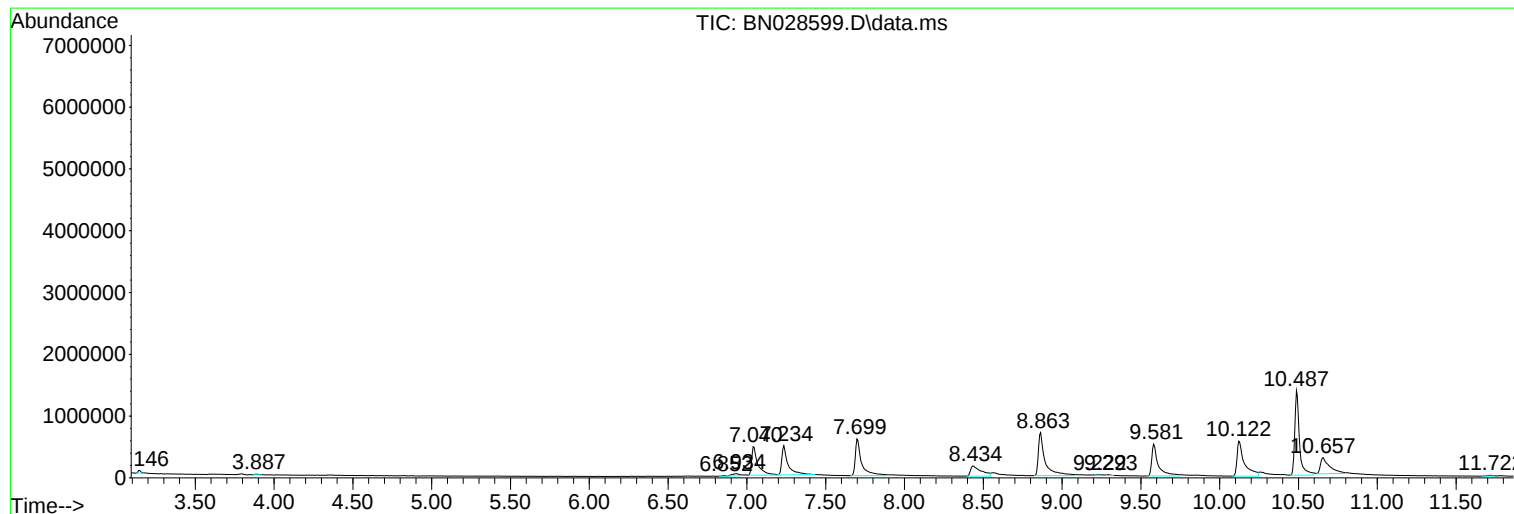

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028599.D
Acq On : 14 Nov 2023 12:58
Operator : MA/JU
Sample : 05281-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028599.D
Acq On : 14 Nov 2023 12:58
Operator : MA/JU
Sample : 05281-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc