

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028600.D
 Acq On : 14 Nov 2023 13:34
 Operator : MA/JU
 Sample : 05281-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	13	rBV	30276	32605	0.32%	0.044%
2	3.787	117	119	125	rVB4	13180	18892	0.18%	0.026%
3	3.887	133	136	140	rVB3	8770	13583	0.13%	0.018%
4	6.934	645	654	663	rVV2	24661	98040	0.96%	0.133%
5	7.046	667	673	698	rVV	319326	1003928	9.78%	1.360%
6	7.234	699	705	740	rVB	349751	1047343	10.21%	1.419%
7	7.699	777	784	803	rBV	418438	1193157	11.63%	1.617%
8	8.440	903	910	927	rBV3	102258	529212	5.16%	0.717%
9	8.863	975	982	1005	rBV	492976	1511143	14.73%	2.048%
10	9.581	1097	1104	1128	rBV	350150	1106960	10.79%	1.500%
11	10.122	1190	1196	1237	rBV	389857	1625053	15.84%	2.202%
12	10.487	1251	1258	1280	rBV	1043567	2255410	21.98%	3.056%
13	10.657	1280	1287	1329	rVB	249108	1261769	12.30%	1.710%
14	11.716	1461	1467	1471	rBV3	13028	23900	0.23%	0.032%
15	12.734	1631	1640	1649	rBV2	17778	43610	0.43%	0.059%
16	13.257	1722	1729	1738	rBV	135802	232554	2.27%	0.315%
17	13.657	1793	1797	1803	rBV2	18975	31491	0.31%	0.043%
18	13.763	1809	1815	1848	rBV	2966505	4897516	47.73%	6.636%
19	14.034	1855	1861	1881	rBV2	2962684	5120640	49.91%	6.939%
20	14.345	1907	1914	1935	rBV	2101832	3434642	33.47%	4.654%
21	15.169	2048	2054	2060	rBV4	20625	39036	0.38%	0.053%
22	15.340	2077	2083	2100	rBV	4035511	6872889	66.98%	9.313%
23	15.463	2100	2104	2121	rVB	786011	1583663	15.43%	2.146%
24	15.787	2156	2159	2164	rVB3	20239	29753	0.29%	0.040%
25	16.434	2265	2269	2275	rVB4	12145	20441	0.20%	0.028%
26	16.598	2295	2297	2305	rVB6	7318	13375	0.13%	0.018%
27	16.975	2357	2361	2365	rBV5	12388	18493	0.18%	0.025%
28	17.092	2375	2381	2393	rBV	2295828	3945357	38.45%	5.346%
29	17.192	2393	2398	2429	rVB2	5039630	8717725	84.97%	11.813%
30	18.975	2698	2701	2704	rBV4	17907	21756	0.21%	0.029%
31	19.063	2712	2716	2721	rBV	62466	94863	0.92%	0.129%
32	19.133	2725	2728	2733	rBV2	42960	70423	0.69%	0.095%
33	19.451	2779	2782	2784	rBV3	25518	31408	0.31%	0.043%
34	19.498	2784	2790	2810	rVV	7076218	10260341	100.00%	13.903%
35	21.304	3092	3097	3112	rBV	2083843	3980161	38.79%	5.393%
36	23.463	3457	3464	3475	rBV	4115480	8739942	85.18%	11.843%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	23.604	3482	3488	3504	rVB	1738243	3877920	37.80%	5.255%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 73798994

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

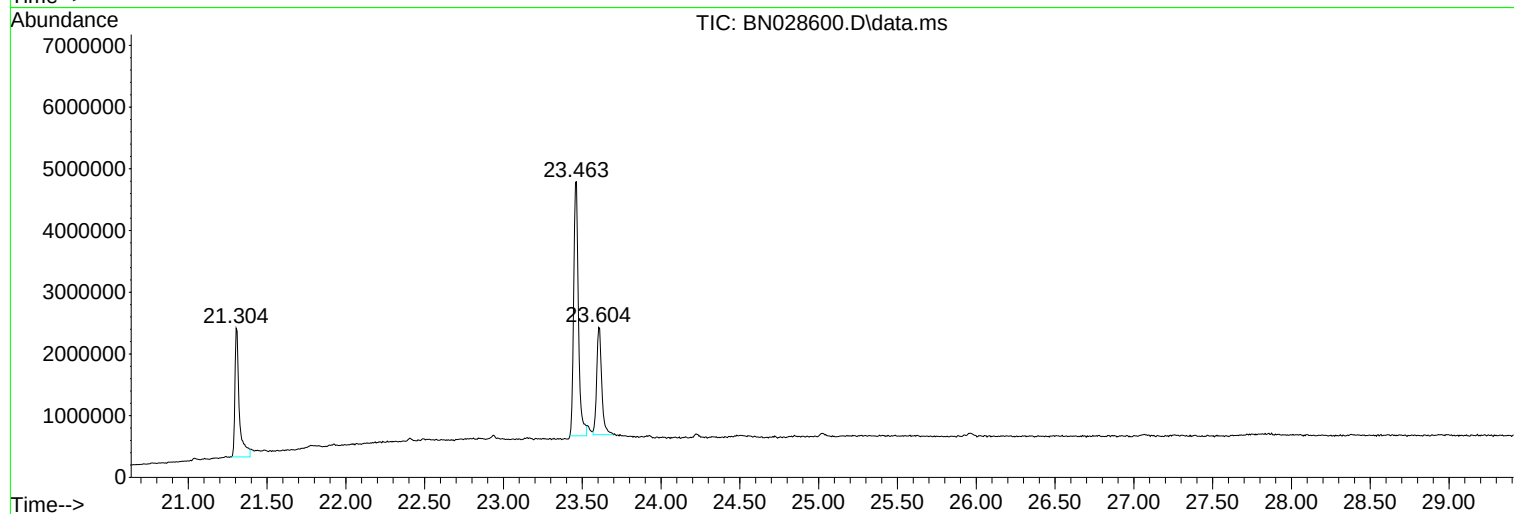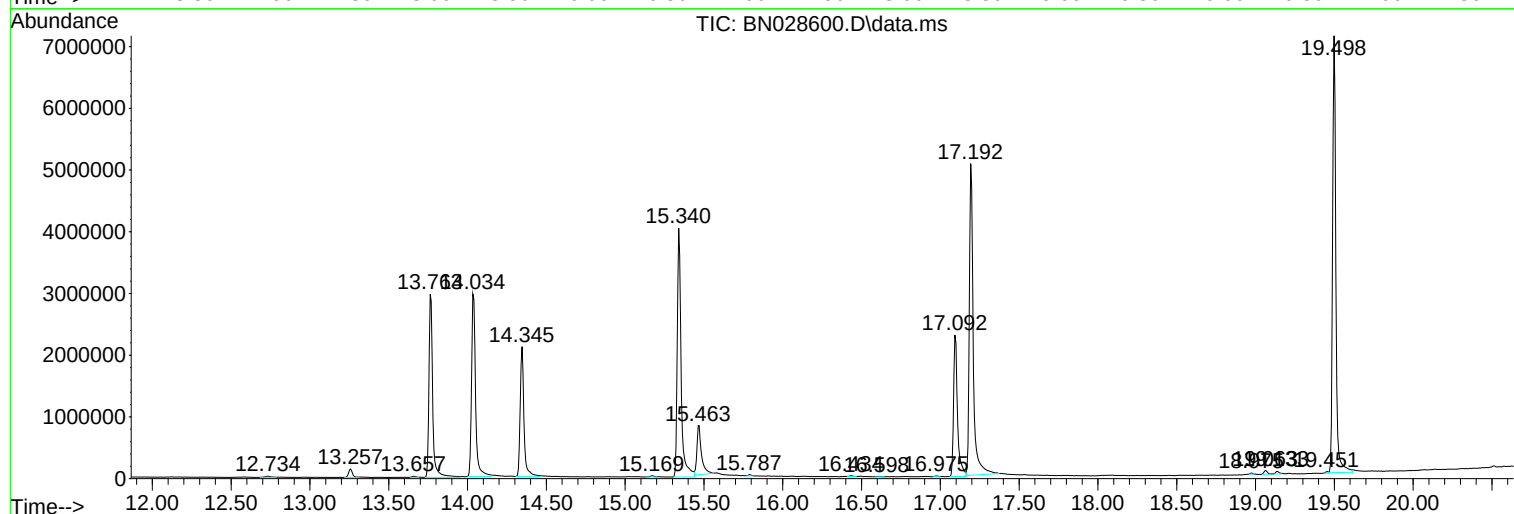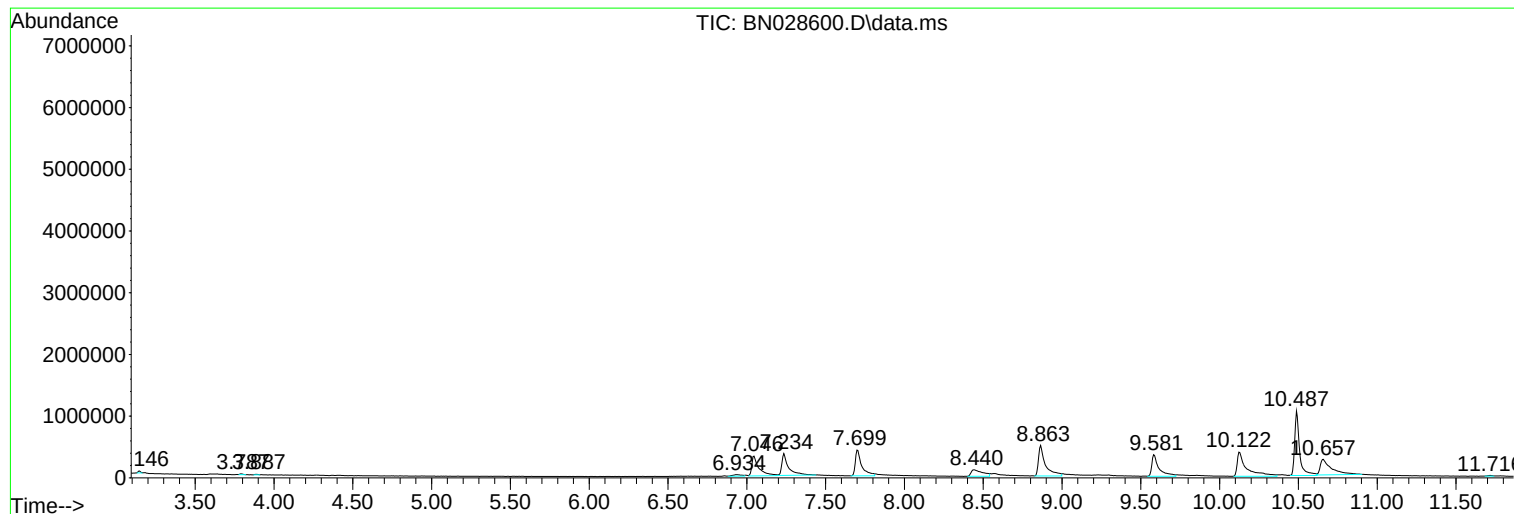

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028600.D
Acq On : 14 Nov 2023 13:34
Operator : MA/JU
Sample : 05281-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc