

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028601.D
 Acq On : 14 Nov 2023 14:10
 Operator : MA/JU
 Sample : 05281-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	6	9	13	rBV	42312	55316	0.51%	0.072%
2	3.587	82	85	88	rBV5	12255	19308	0.18%	0.025%
3	6.864	637	642	644	rBV6	8019	10948	0.10%	0.014%
4	6.934	644	654	661	rBV3	30691	112525	1.05%	0.147%
5	7.040	667	672	696	rBV	325307	969061	9.02%	1.269%
6	7.234	699	705	738	rVB	368562	1076759	10.02%	1.410%
7	7.699	778	784	818	rBV	421406	1277908	11.89%	1.674%
8	8.440	902	910	929	rBV2	131524	688391	6.41%	0.902%
9	8.863	975	982	1008	rBV	510915	1585677	14.76%	2.077%
10	9.581	1097	1104	1134	rBV	373090	1174557	10.93%	1.538%
11	10.122	1189	1196	1219	rBV	421036	1489783	13.87%	1.951%
12	10.487	1251	1258	1281	rBV	1034172	2254624	20.98%	2.953%
13	10.657	1281	1287	1312	rVV2	162140	780973	7.27%	1.023%
14	11.710	1459	1466	1468	rBV6	10557	18814	0.18%	0.025%
15	12.728	1633	1639	1644	rBV2	17668	27704	0.26%	0.036%
16	13.257	1722	1729	1737	rBV	82361	137970	1.28%	0.181%
17	13.663	1788	1798	1807	rBV3	19404	45894	0.43%	0.060%
18	13.763	1809	1815	1844	rBV	2857711	4574204	42.57%	5.991%
19	14.040	1854	1862	1884	rBV	3057175	5216006	48.54%	6.832%
20	14.345	1907	1914	1943	rBV	2125899	3588516	33.40%	4.700%
21	15.169	2048	2054	2060	rBV5	20408	37747	0.35%	0.049%
22	15.340	2077	2083	2099	rBV	3865254	6581264	61.25%	8.620%
23	15.463	2099	2104	2120	rVB	927087	1733188	16.13%	2.270%
24	15.792	2156	2160	2164	rVB3	15858	23680	0.22%	0.031%
25	16.434	2265	2269	2274	rVB6	12523	18690	0.17%	0.024%
26	16.981	2357	2362	2367	rVB2	10280	18334	0.17%	0.024%
27	17.092	2375	2381	2392	rBV	2437262	4133941	38.47%	5.414%
28	17.192	2392	2398	2431	rVB	5156201	9017816	83.93%	11.811%
29	17.775	2493	2497	2506	rVB10	20811	36292	0.34%	0.048%
30	18.028	2536	2540	2543	rBV6	16236	30440	0.28%	0.040%
31	18.945	2692	2696	2698	rBV5	14627	25080	0.23%	0.033%
32	18.975	2698	2701	2706	rVB5	34940	46987	0.44%	0.062%
33	19.063	2712	2716	2723	rBV3	66136	115520	1.08%	0.151%
34	19.139	2725	2729	2738	rVB2	47356	90917	0.85%	0.119%
35	19.245	2743	2747	2757	rVV	135532	210733	1.96%	0.276%
36	19.451	2778	2782	2784	rBV3	43158	58192	0.54%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028601.D
Acq On : 14 Nov 2023 14:10
Operator : MA/JU
Sample : 05281-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.498	2784	2790	2815	rVV	7175230	10744832	100.00%	14.073%
38	19.763	2832	2835	2843	rVB2	59942	73796	0.69%	0.097%
39	21.304	3092	3097	3116	rBV	2352239	4314236	40.15%	5.651%
40	23.463	3456	3464	3481	rBV	4346559	9695565	90.23%	12.699%
41	23.604	3482	3488	3506	rVB	1904138	4237827	39.44%	5.551%




Sum of corrected areas: 76350015

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028601.D
Acq On : 14 Nov 2023 14:10
Operator : MA/JU
Sample : 05281-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

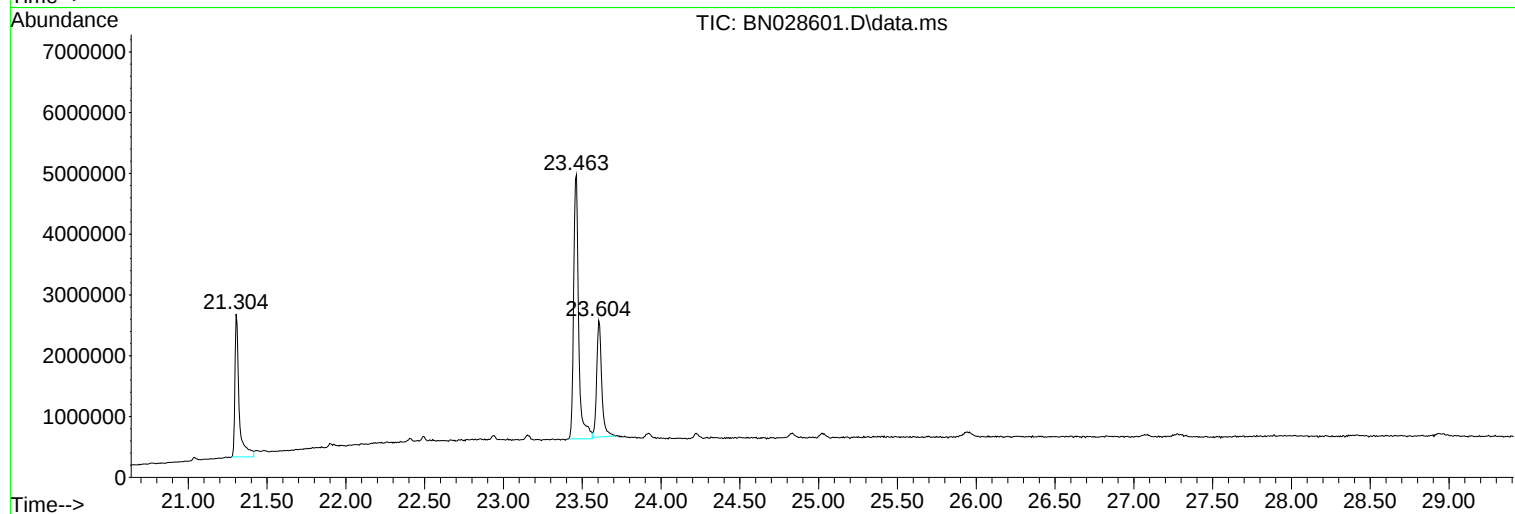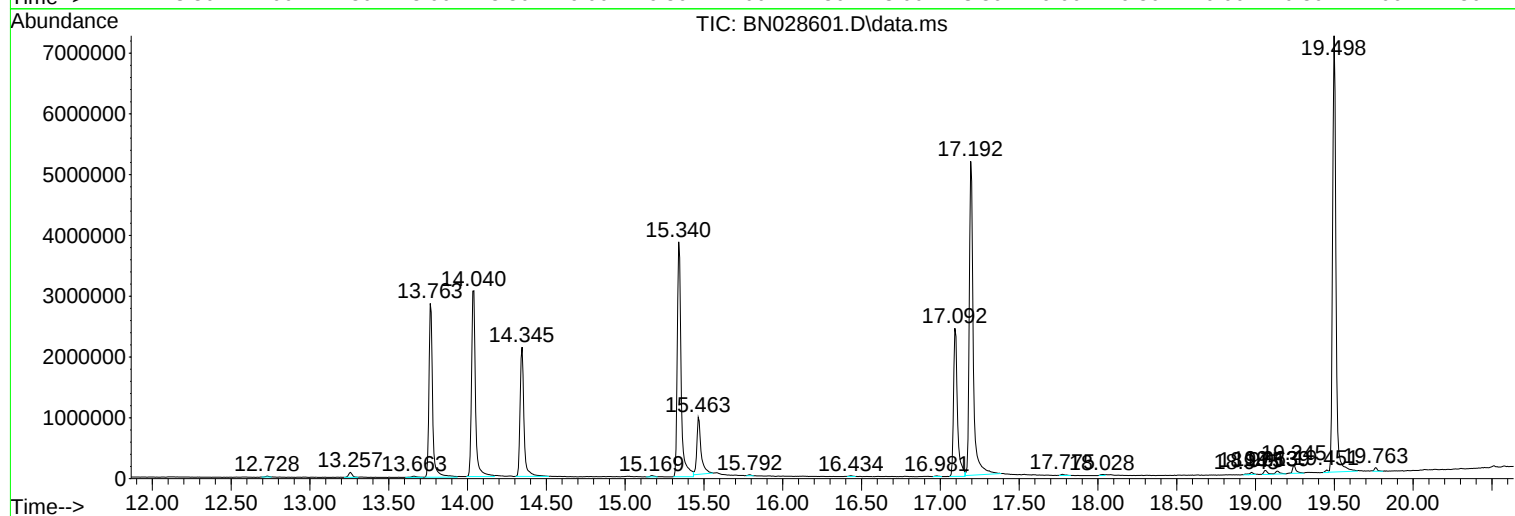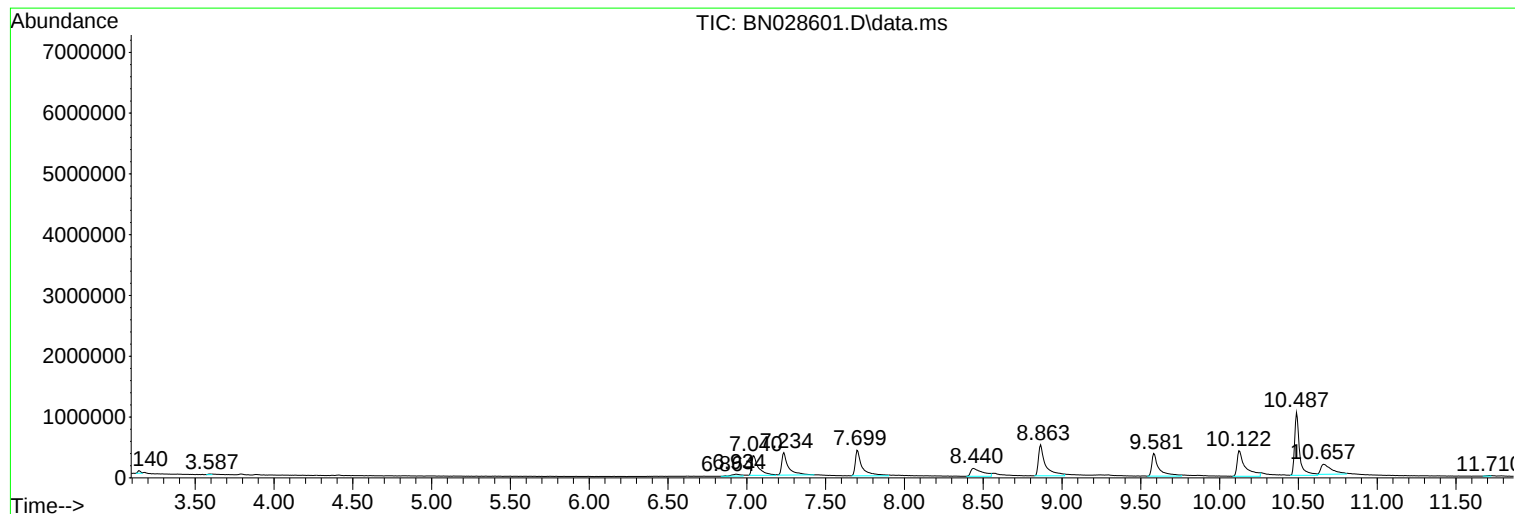

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028601.D
Acq On : 14 Nov 2023 14:10
Operator : MA/JU
Sample : 05281-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028601.D
Acq On : 14 Nov 2023 14:10
Operator : MA/JU
Sample : 05281-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc