

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028602.D
 Acq On : 14 Nov 2023 14:46
 Operator : MA/JU
 Sample : 05281-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	13	rBV	45333	59375	0.57%	0.083%
2	3.587	82	85	89	rBV2	18429	34470	0.33%	0.048%
3	3.793	117	120	125	rVB2	16646	25777	0.25%	0.036%
4	3.881	131	135	141	rBV7	6622	13689	0.13%	0.019%
5	6.863	637	642	644	rBV4	7865	11535	0.11%	0.016%
6	6.928	644	653	661	rBV2	39891	154825	1.48%	0.216%
7	7.046	667	673	698	rBV	385578	1103318	10.54%	1.537%
8	7.234	698	705	734	rVV	453219	1242141	11.87%	1.730%
9	7.705	777	785	807	rBV	254831	810090	7.74%	1.128%
10	8.434	901	909	929	rBV	173510	833127	7.96%	1.160%
11	8.863	975	982	1012	rBV	593079	1816921	17.36%	2.531%
12	9.581	1098	1104	1132	rBV	460947	1324786	12.66%	1.845%
13	10.122	1189	1196	1215	rBV	513122	1625065	15.53%	2.264%
14	10.487	1252	1258	1280	rBV	644924	1463964	13.99%	2.039%
15	10.657	1280	1287	1318	rVV2	183280	891041	8.51%	1.241%
16	11.716	1459	1467	1468	rBV5	11561	20317	0.19%	0.028%
17	12.593	1609	1616	1621	rBV9	7159	13645	0.13%	0.019%
18	12.728	1632	1639	1644	rBV2	17625	40830	0.39%	0.057%
19	13.257	1723	1729	1736	rBV	23695	42170	0.40%	0.059%
20	13.657	1792	1797	1801	rBV2	16844	29607	0.28%	0.041%
21	13.763	1809	1815	1842	rBV	3368611	5302405	50.66%	7.386%
22	14.034	1855	1861	1884	rBV	3547294	5830338	55.71%	8.121%
23	14.345	1907	1914	1937	rBV	1376119	2403125	22.96%	3.347%
24	15.169	2047	2054	2059	rBV5	22595	38470	0.37%	0.054%
25	15.339	2077	2083	2100	rBV	4515652	7577142	72.40%	10.554%
26	15.463	2100	2104	2121	rVB	847595	1630137	15.58%	2.271%
27	15.792	2157	2160	2164	rVB2	19713	26129	0.25%	0.036%
28	16.434	2265	2269	2275	rVB3	17597	31478	0.30%	0.044%
29	16.975	2355	2361	2367	rBV4	13269	24285	0.23%	0.034%
30	17.092	2375	2381	2392	rBV	1582380	2753474	26.31%	3.835%
31	17.192	2392	2398	2430	rVB	5077044	8717674	83.29%	12.143%
32	18.022	2536	2539	2541	rBV3	17985	22474	0.21%	0.031%
33	18.304	2585	2587	2593	rBV6	6743	10796	0.10%	0.015%
34	19.063	2711	2716	2723	rBV	67290	111604	1.07%	0.155%
35	19.139	2725	2729	2735	rVV2	41210	76230	0.73%	0.106%
36	19.451	2779	2782	2784	rBV4	27307	31510	0.30%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028602.D
Acq On : 14 Nov 2023 14:46
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.498	2784	2790	2814	rVV	7316540	10466123	100.00%	14.578%
38	21.039	3048	3052	3059	rBV5	92051	182906	1.75%	0.255%
39	21.304	3093	3097	3116	rBV	1563778	2877998	27.50%	4.009%
40	23.463	3456	3464	3474	rBV	4299462	9295452	88.81%	12.948%
41	23.604	3482	3488	3504	rVB	1279935	2825796	27.00%	3.936%




Sum of corrected areas: 71792239

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028602.D
Acq On : 14 Nov 2023 14:46
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

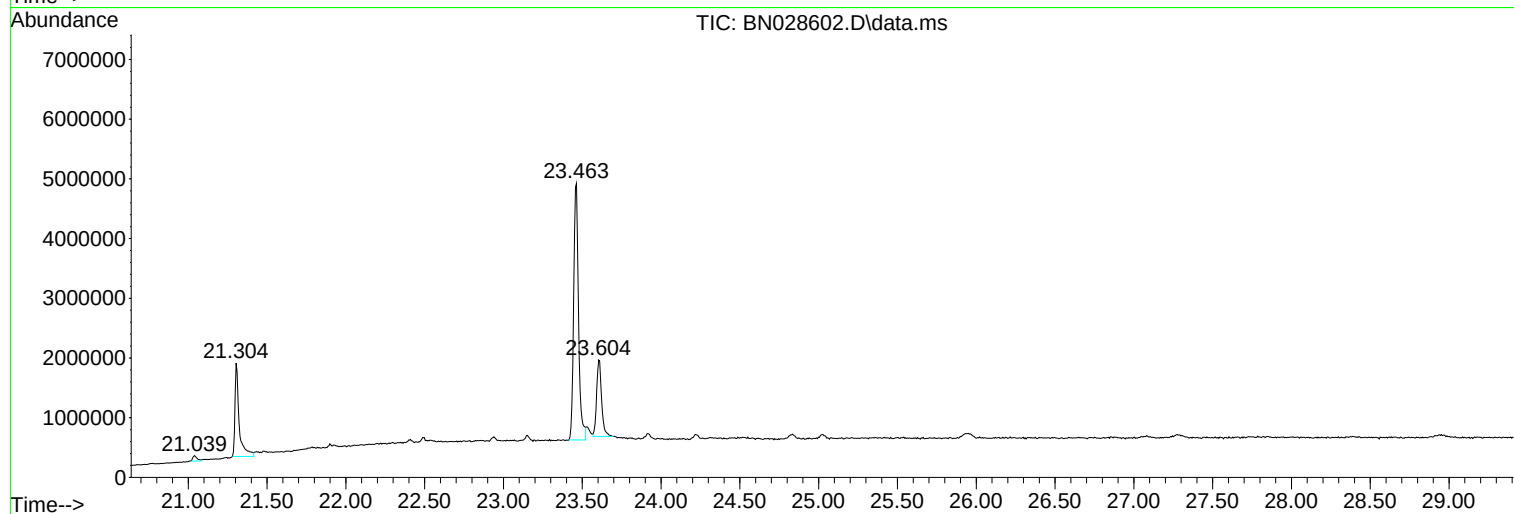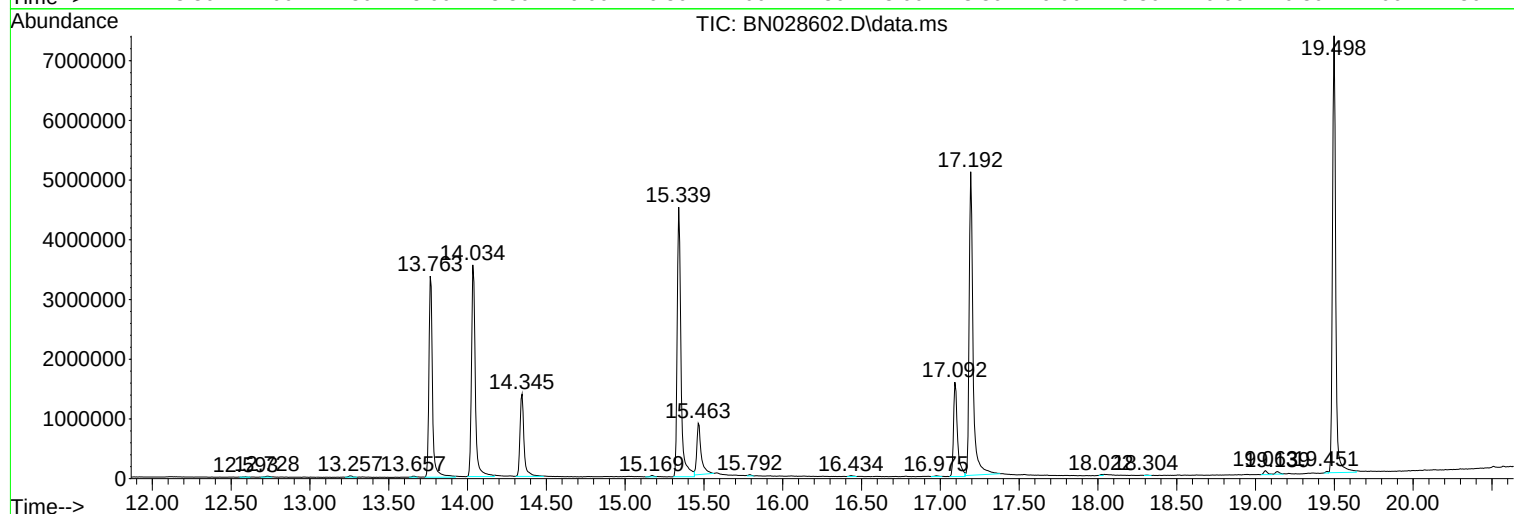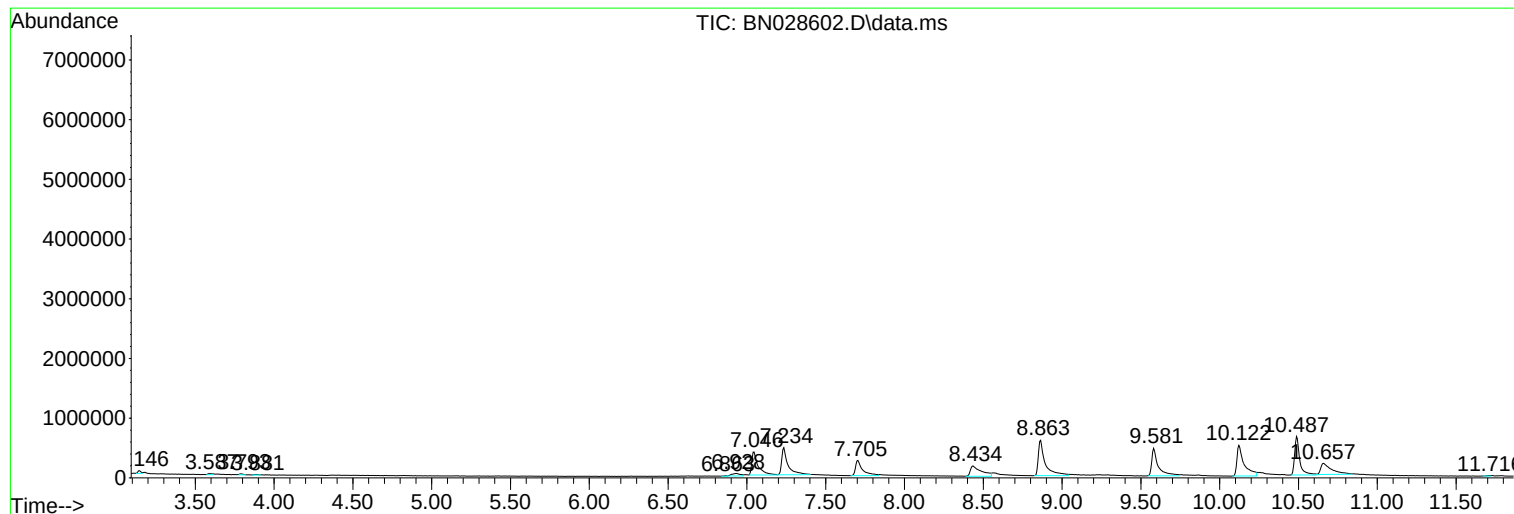

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028602.D
Acq On : 14 Nov 2023 14:46
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028602.D
Acq On : 14 Nov 2023 14:46
Operator : MA/JU
Sample : 05281-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc