

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028603.D
 Acq On : 14 Nov 2023 15:22
 Operator : MA/JU
 Sample : 05281-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	14	rVB	49386	54148	0.66%	0.087%
2	3.575	80	83	98	rBV	53230	154694	1.89%	0.249%
3	4.987	319	323	328	rBV	26146	49243	0.60%	0.079%
4	5.699	440	444	451	rBV5	10362	26023	0.32%	0.042%
5	6.934	644	654	661	rBV2	37964	141582	1.73%	0.228%
6	7.040	667	672	699	rBV	439963	1259109	15.38%	2.027%
7	7.234	699	705	733	rVV	480824	1316141	16.08%	2.119%
8	7.704	778	785	808	rBV	288356	877245	10.72%	1.412%
9	8.434	901	909	928	rBV2	142880	732637	8.95%	1.179%
10	8.863	975	982	1016	rBV	634563	1967070	24.03%	3.166%
11	9.581	1097	1104	1132	rBV	460170	1380182	16.86%	2.222%
12	10.122	1189	1196	1218	rBV	514158	1718087	20.99%	2.766%
13	10.487	1251	1258	1280	rBV	649559	1517518	18.54%	2.443%
14	10.651	1280	1286	1311	rBV	342679	1363141	16.65%	2.194%
15	11.716	1462	1467	1474	rBV8	9997	20199	0.25%	0.033%
16	12.728	1632	1639	1644	rBV2	17841	32903	0.40%	0.053%
17	13.257	1721	1729	1736	rBV2	26516	49977	0.61%	0.080%
18	13.657	1793	1797	1803	rBV4	15730	29881	0.37%	0.048%
19	13.763	1809	1815	1842	rBV	2824405	4452432	54.40%	7.167%
20	14.033	1854	1861	1883	rBV	3082693	5291920	64.65%	8.518%
21	14.345	1907	1914	1936	rBV	1251647	2139500	26.14%	3.444%
22	15.033	2026	2031	2035	rVB8	5742	9053	0.11%	0.015%
23	15.169	2050	2054	2061	rVB4	19082	30794	0.38%	0.050%
24	15.339	2077	2083	2100	rBV	3725380	6442519	78.71%	10.370%
25	15.469	2100	2105	2121	rVB	581285	1195410	14.60%	1.924%
26	15.792	2157	2160	2167	rVB	19927	29451	0.36%	0.047%
27	16.427	2265	2268	2273	rBV4	13009	18915	0.23%	0.030%
28	16.604	2292	2298	2302	rBV8	5784	10525	0.13%	0.017%
29	16.780	2323	2328	2332	rBV8	7328	13527	0.17%	0.022%
30	16.980	2357	2362	2368	rBV6	20065	37835	0.46%	0.061%
31	17.092	2375	2381	2393	rBV	1241790	2321287	28.36%	3.737%
32	17.192	2393	2398	2434	rVB	3745723	6864959	83.87%	11.050%
33	18.086	2547	2550	2554	rVB2	9485	8593	0.10%	0.014%
34	19.063	2711	2716	2724	rBV2	51743	91788	1.12%	0.148%
35	19.139	2725	2729	2739	rVV	34001	74258	0.91%	0.120%
36	19.498	2784	2790	2811	rBV	5578085	8185108	100.00%	13.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028603.D
Acq On : 14 Nov 2023 15:22
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	21.310	3093	3098	3112	rBV	1171190	2295174	28.04%	3.694%
38	23.462	3457	3464	3474	rBV	3716335	7483657	91.43%	12.046%
39	23.604	3483	3488	3502	rVB	1142427	2437949	29.79%	3.924%




Sum of corrected areas: 62124434

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028603.D
Acq On : 14 Nov 2023 15:22
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

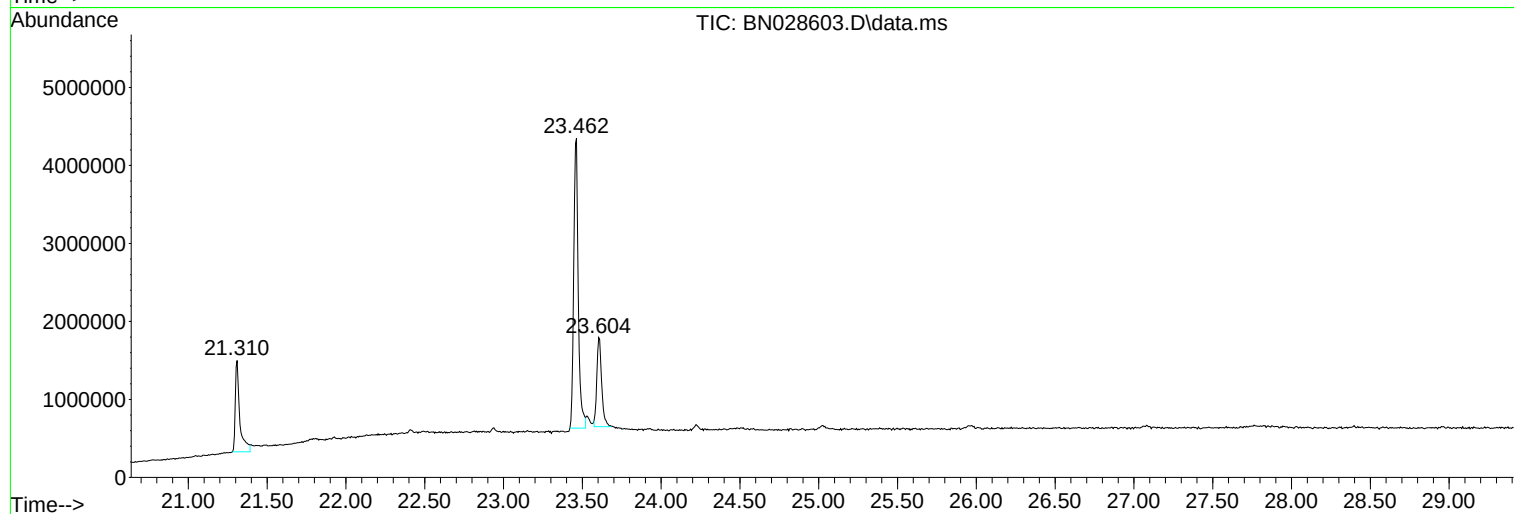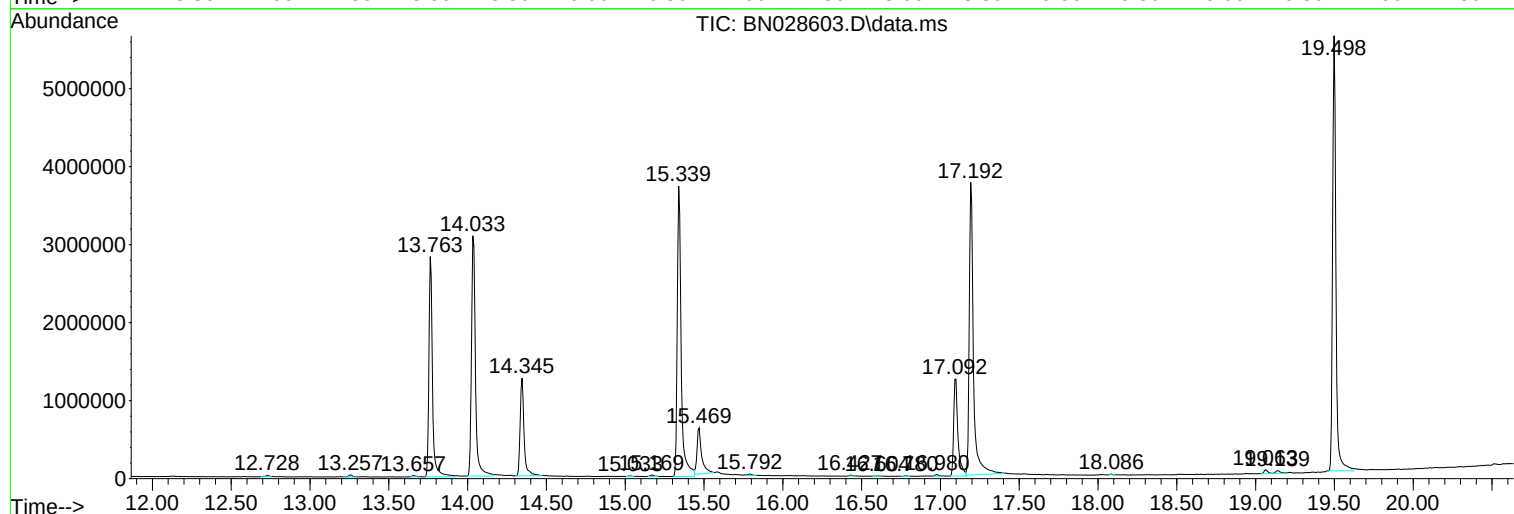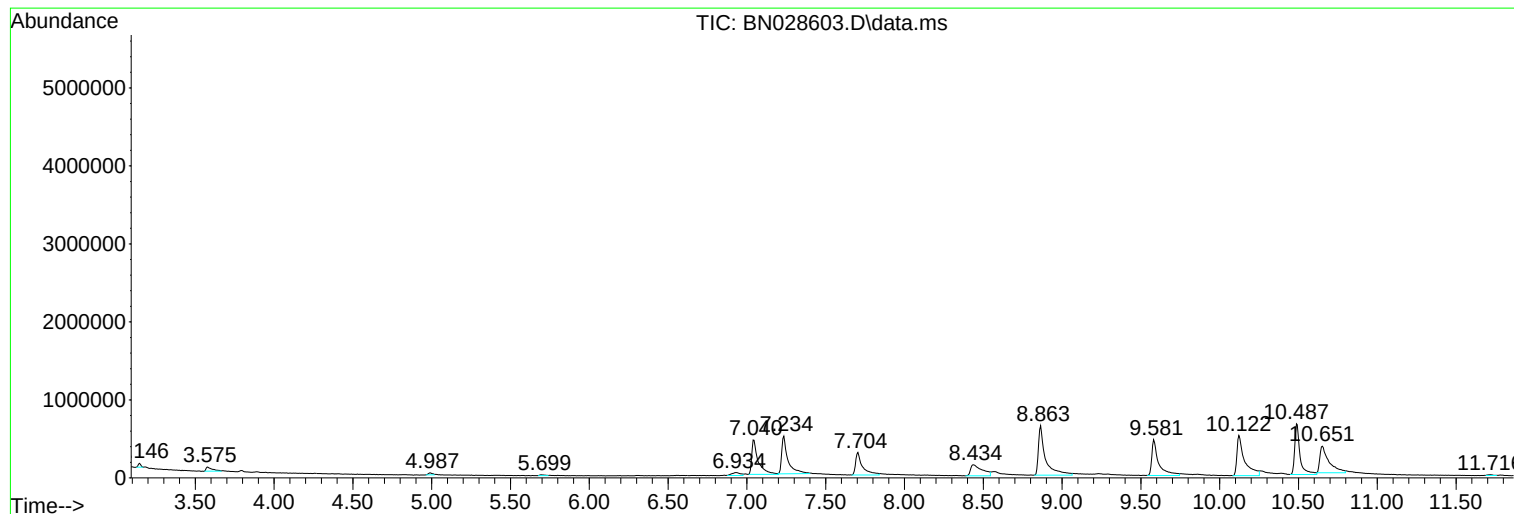

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028603.D
Acq On : 14 Nov 2023 15:22
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028603.D
Acq On : 14 Nov 2023 15:22
Operator : MA/JU
Sample : 05281-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------