

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
 Data File : BN028604.D
 Acq On : 14 Nov 2023 15:58
 Operator : MA/JU
 Sample : 05281-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN028604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	20	rVB2	48430	83627	0.81%	0.108%
2	3.587	80	85	90	rBV3	27692	68103	0.66%	0.088%
3	3.793	117	120	128	rVB2	20648	34784	0.34%	0.045%
4	4.993	319	324	330	rBV4	14475	29706	0.29%	0.038%
5	6.558	586	590	594	rBV7	5367	10834	0.10%	0.014%
6	6.934	643	654	662	rBV	41476	163593	1.58%	0.210%
7	7.040	667	672	698	rVV	446921	1288101	12.43%	1.657%
8	7.234	699	705	738	rVB	506524	1416642	13.68%	1.822%
9	7.705	778	785	811	rBV	390452	1187481	11.46%	1.527%
10	8.434	902	909	927	rBV2	173726	796551	7.69%	1.025%
11	8.863	975	982	1012	rBV	671567	2016554	19.47%	2.594%
12	9.581	1097	1104	1129	rBV	508223	1455061	14.05%	1.872%
13	10.122	1188	1196	1218	rBV	586132	1889477	18.24%	2.430%
14	10.487	1251	1258	1275	rBV	1012486	2127960	20.54%	2.737%
15	10.646	1279	1285	1324	rVB	393376	1646504	15.89%	2.118%
16	11.716	1460	1467	1471	rBV6	10234	23648	0.23%	0.030%
17	11.793	1474	1480	1483	rVB6	5942	12446	0.12%	0.016%
18	12.728	1632	1639	1644	rBV2	18214	37195	0.36%	0.048%
19	13.251	1724	1728	1737	rBV	24470	47426	0.46%	0.061%
20	13.657	1792	1797	1803	rBV2	18457	31388	0.30%	0.040%
21	13.763	1809	1815	1841	rBV	3282431	5308750	51.25%	6.828%
22	14.034	1855	1861	1881	rBV	3652669	6078199	58.68%	7.818%
23	14.269	1899	1901	1905	rVB5	10075	10496	0.10%	0.014%
24	14.345	1907	1914	1951	rVB	2029522	3404316	32.86%	4.379%
25	15.169	2049	2054	2059	rBV3	17943	30162	0.29%	0.039%
26	15.340	2077	2083	2100	rBV	4451282	7556092	72.94%	9.719%
27	15.463	2100	2104	2121	rVB	834127	1608727	15.53%	2.069%
28	15.792	2157	2160	2164	rVB4	16901	22081	0.21%	0.028%
29	16.428	2264	2268	2271	rBV3	11555	13864	0.13%	0.018%
30	16.781	2321	2328	2333	rVB8	9383	17879	0.17%	0.023%
31	16.981	2357	2362	2367	rBV6	16970	31837	0.31%	0.041%
32	17.092	2375	2381	2392	rBV	2205926	3831521	36.99%	4.928%
33	17.192	2392	2398	2427	rVB	4993837	8466485	81.73%	10.890%
34	19.063	2711	2716	2721	rBV2	68088	109189	1.05%	0.140%
35	19.139	2725	2729	2734	rVV	40656	67619	0.65%	0.087%
36	19.457	2780	2783	2784	rBV3	18083	19025	0.18%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028604.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : 05281-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Title : SVOA CALIBRATION

37	19.498	2784	2790	2809	rVV	7335187	10358771	100.00%	13.324%
38	21.304	3093	3097	3114	rBV	2264711	3958186	38.21%	5.091%
39	23.463	3457	3464	3474	rBV	4252440	8677865	83.77%	11.162%
40	23.604	3482	3488	3504	rVB	1700444	3807272	36.75%	4.897%




Sum of corrected areas: 77745417

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028604.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : 05281-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

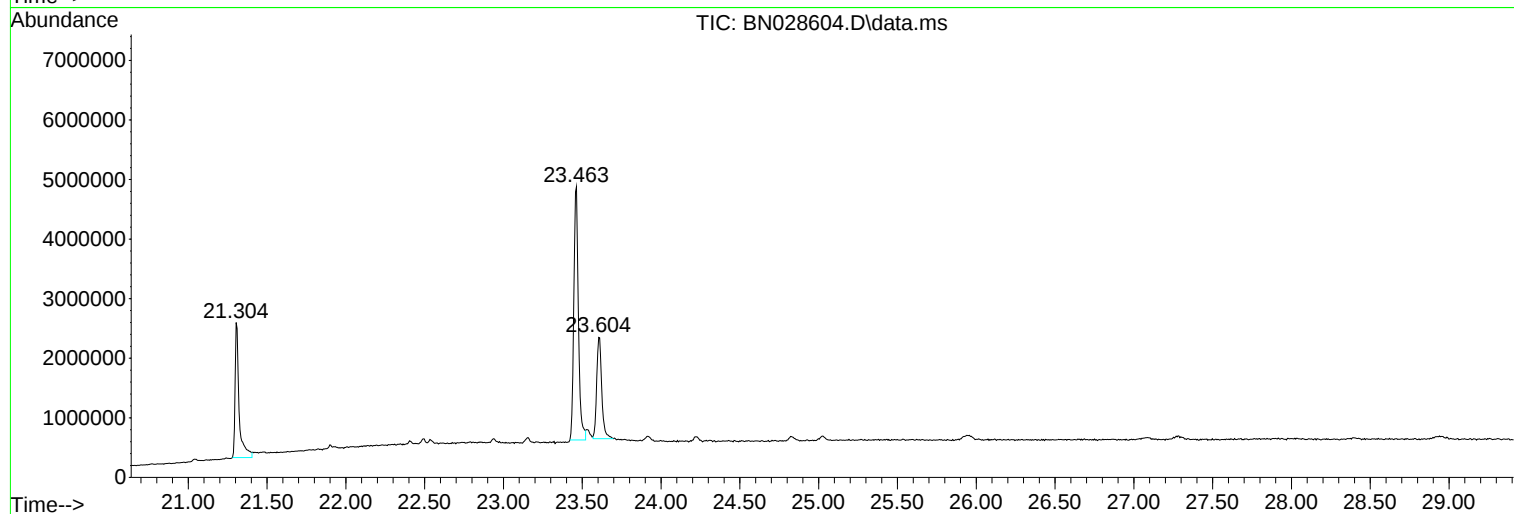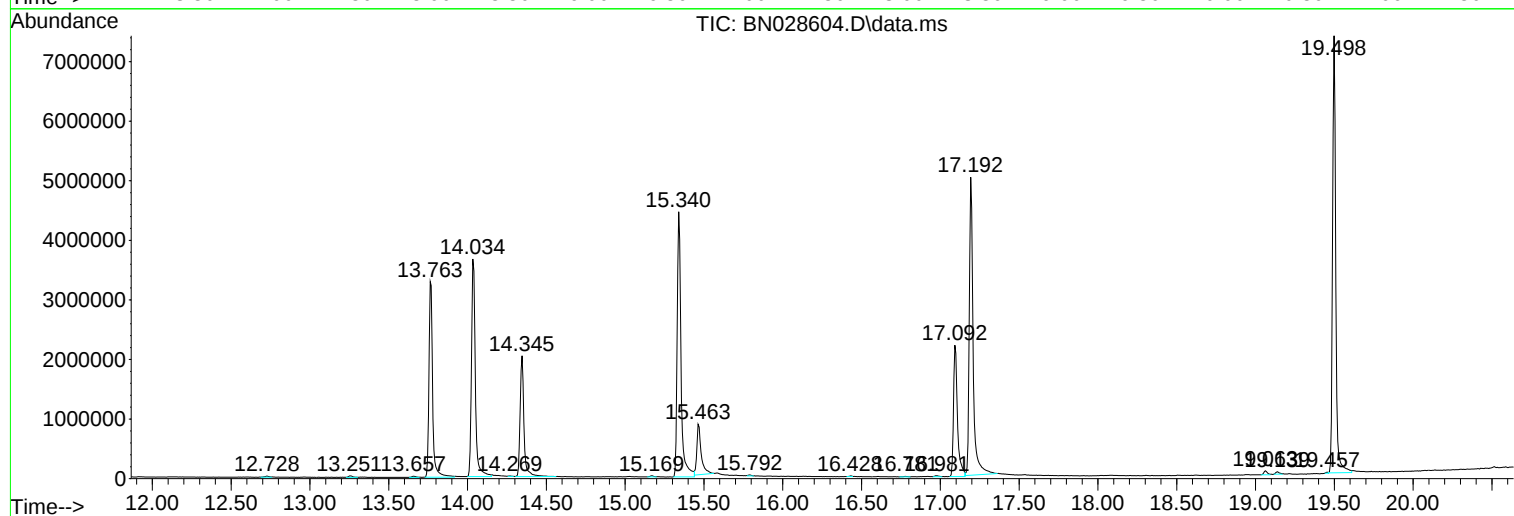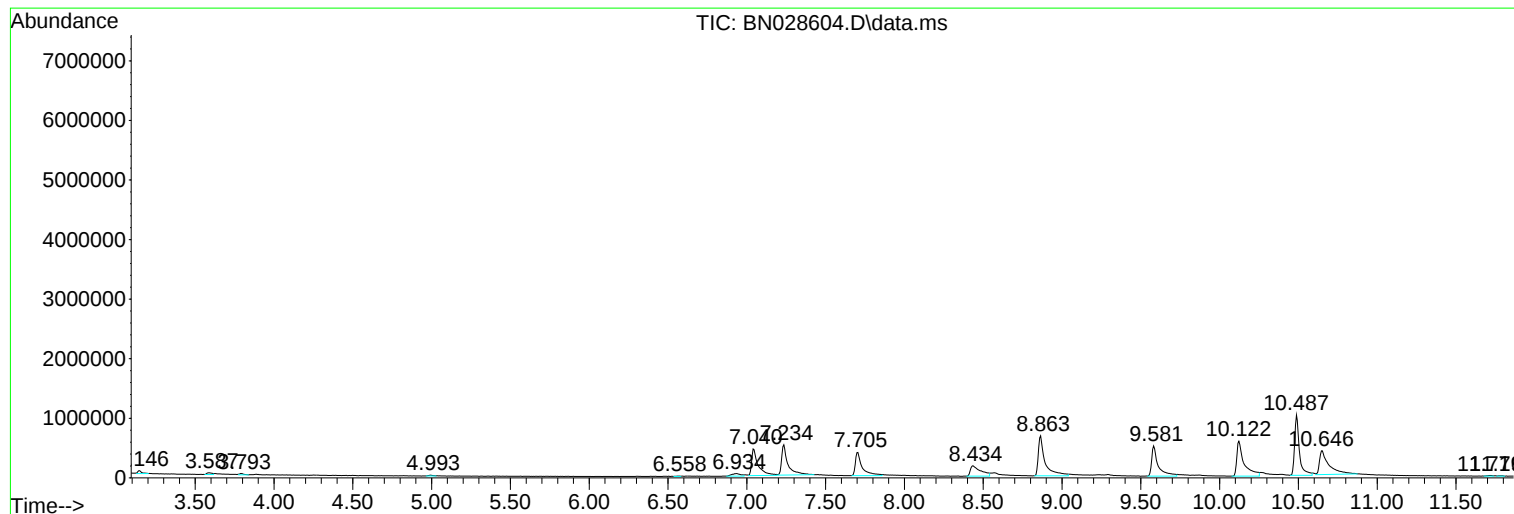

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028604.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : 05281-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111423\
Data File : BN028604.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : 05281-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111423.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc